
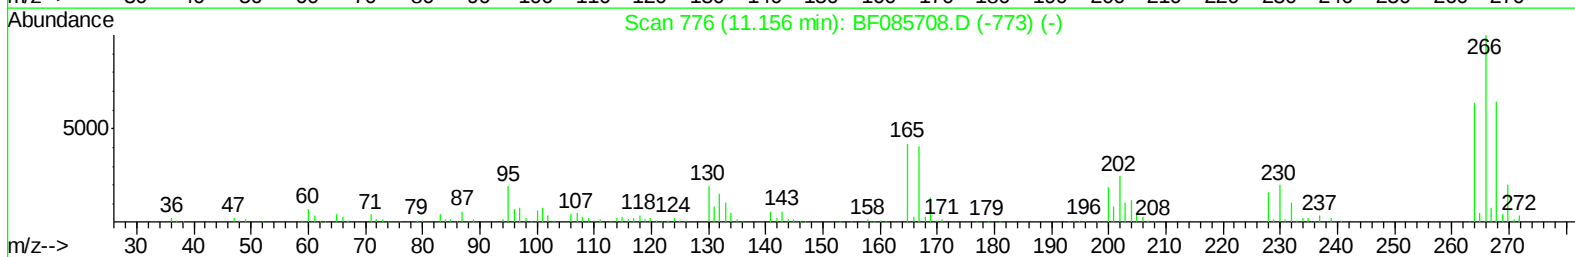
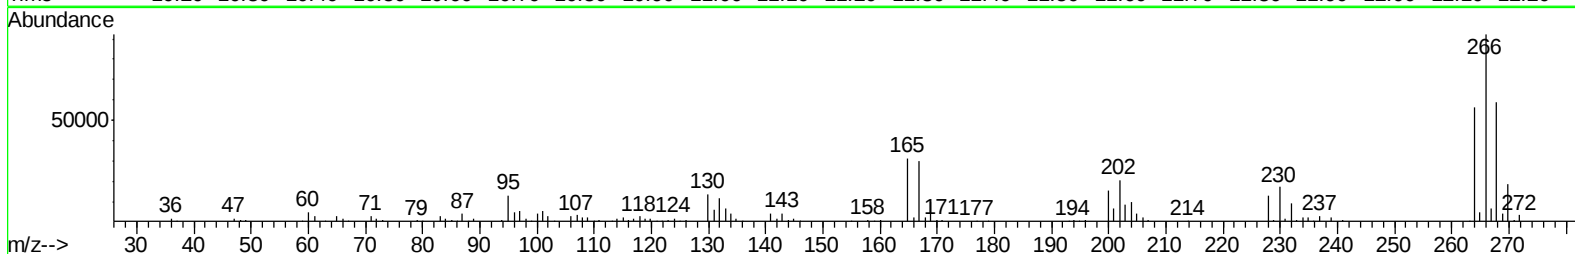


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
Data File : BF085704.D
Acq On : 24 Mar 2016 9:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 06:42:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 14:15:39 2016
Response via : Initial Calibration

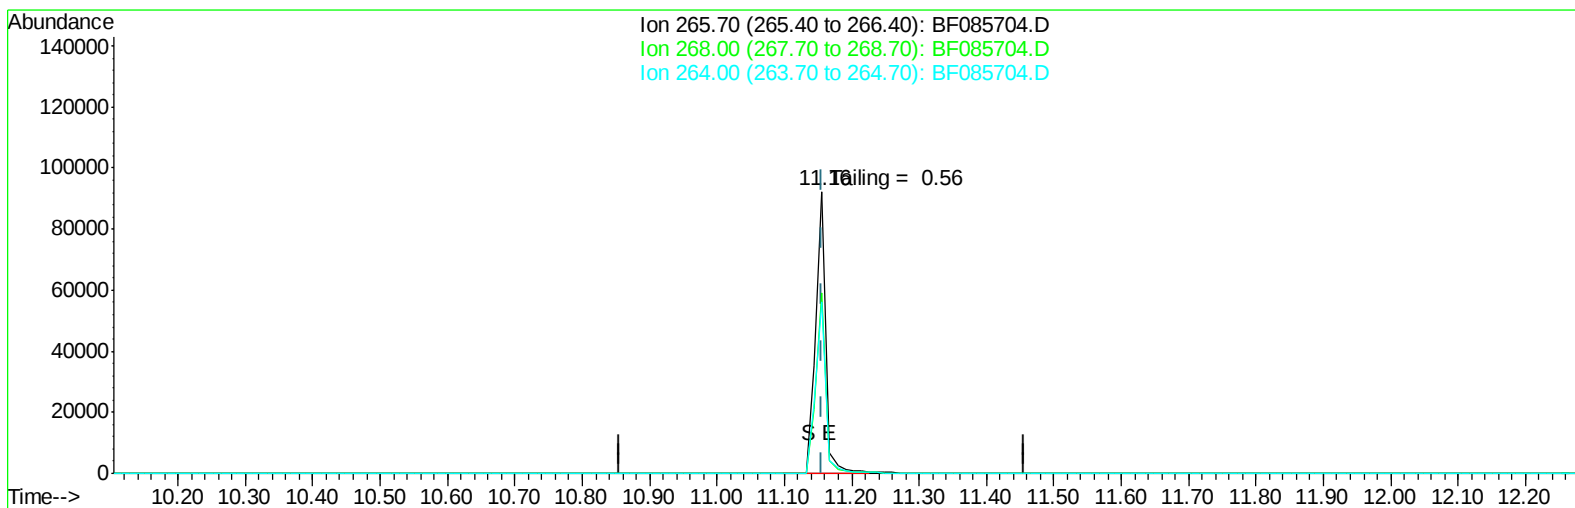

TIC: BF085704.D

(69) Pentachlorophenol (C)




11.156min (-0.000) 0.00ng

response 97046

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.08
264.00	63.30	60.94
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
Data File : BF085704.D
Acq On : 24 Mar 2016 9:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 06:42:52 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 14:15:39 2016
Response via : Initial Calibration

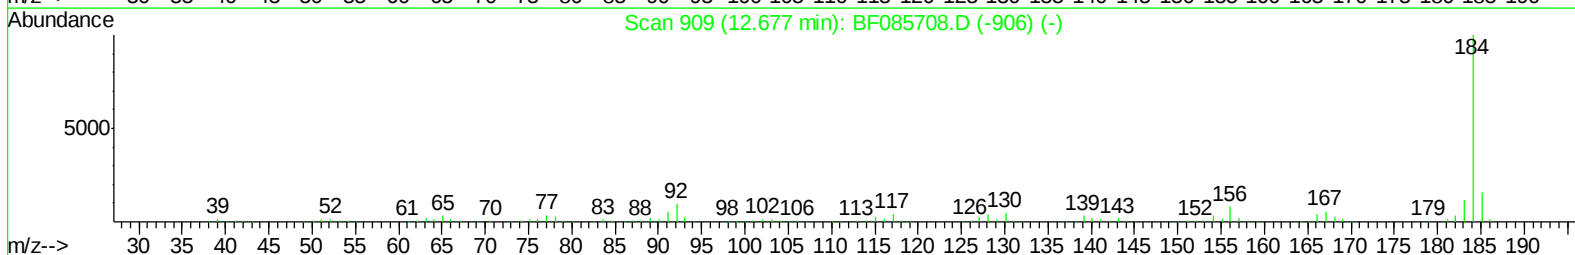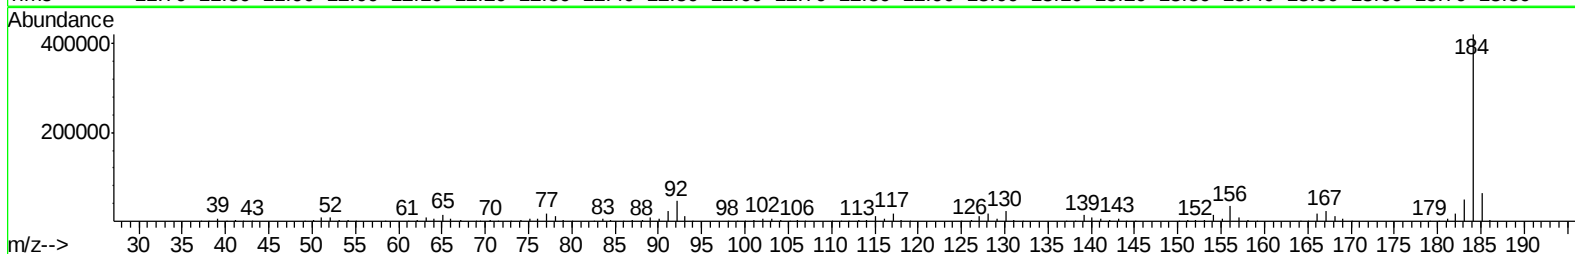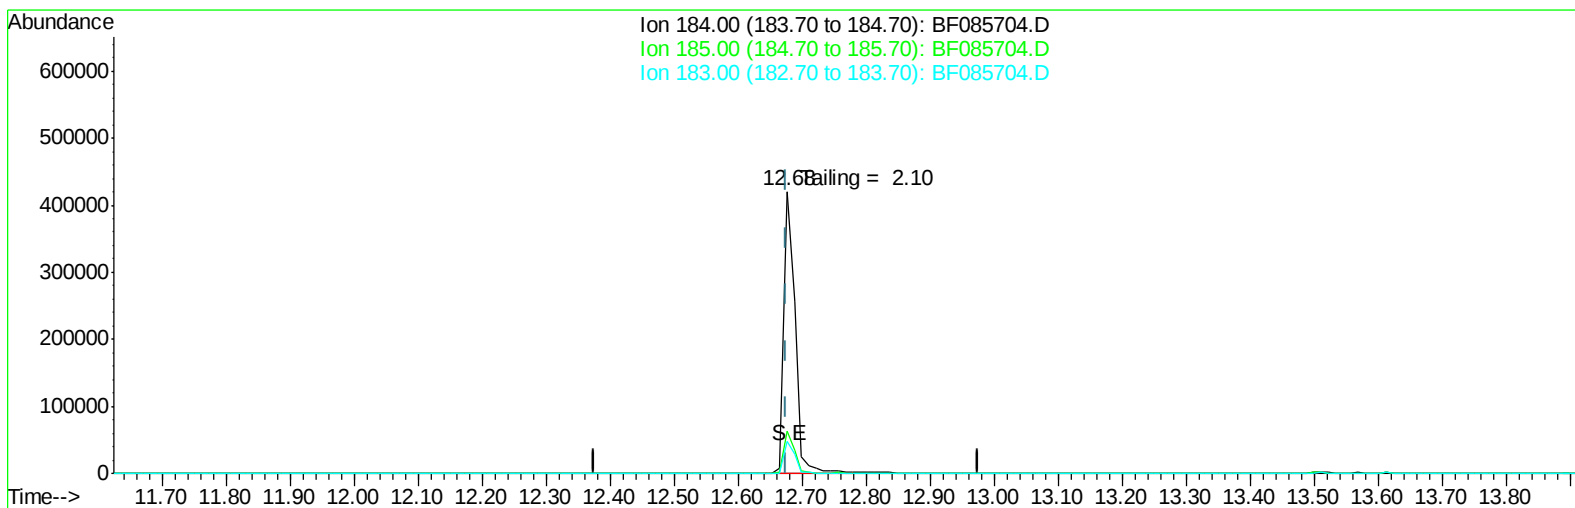

TIC: BF085704.D

(76) Benzidine

12.676min (-0.000) 0.00ng

response 517699

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	15.10
183.00	11.80	11.47
0.00	0.00	0.00