

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
 Data File : BF085742.D
 Acq On : 25 Mar 2016 5:10
 Operator : UM/SJ
 Sample : H1884-20
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 GW-01(18-20)

Quant Time: Mar 25 07:24:25 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 24 14:15:39 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.82	152	111026	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	429440	20.00	ng	-0.01
38) Acenaphthene-d10	9.86	164	205414	20.00	ng	0.00
63) Phenanthrene-d10	11.34	188	387085	20.00	ng	-0.01
75) Chrysene-d12	13.98	240	274951	20.00	ng	0.00
86) Perylene-d12	15.40	264	201885	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.43	112	949605	142.44	ng	0.02
7) Phenol-d6	6.46	99	1241172	146.43	ng	0.00
23) Nitrobenzene-d5	7.40	82	779304	102.19	ng	0.00
41) 2,4,6-Tribromophenol	10.65	330	309204	158.43	ng	0.00
44) 2-Fluorobiphenyl	9.19	172	1203701	97.90	ng	0.00
78) Terphenyl-d14	12.93	244	1046014	78.24	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.58	163	154981	9.94	ng	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
Data File : BF085742.D
Acq On : 25 Mar 2016 5:10
Operator : UM/SJ
Sample : H1884-20
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
GW-01(18-20)

Quant Time: Mar 25 07:24:25 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 24 14:15:39 2016
Response via : Initial Calibration

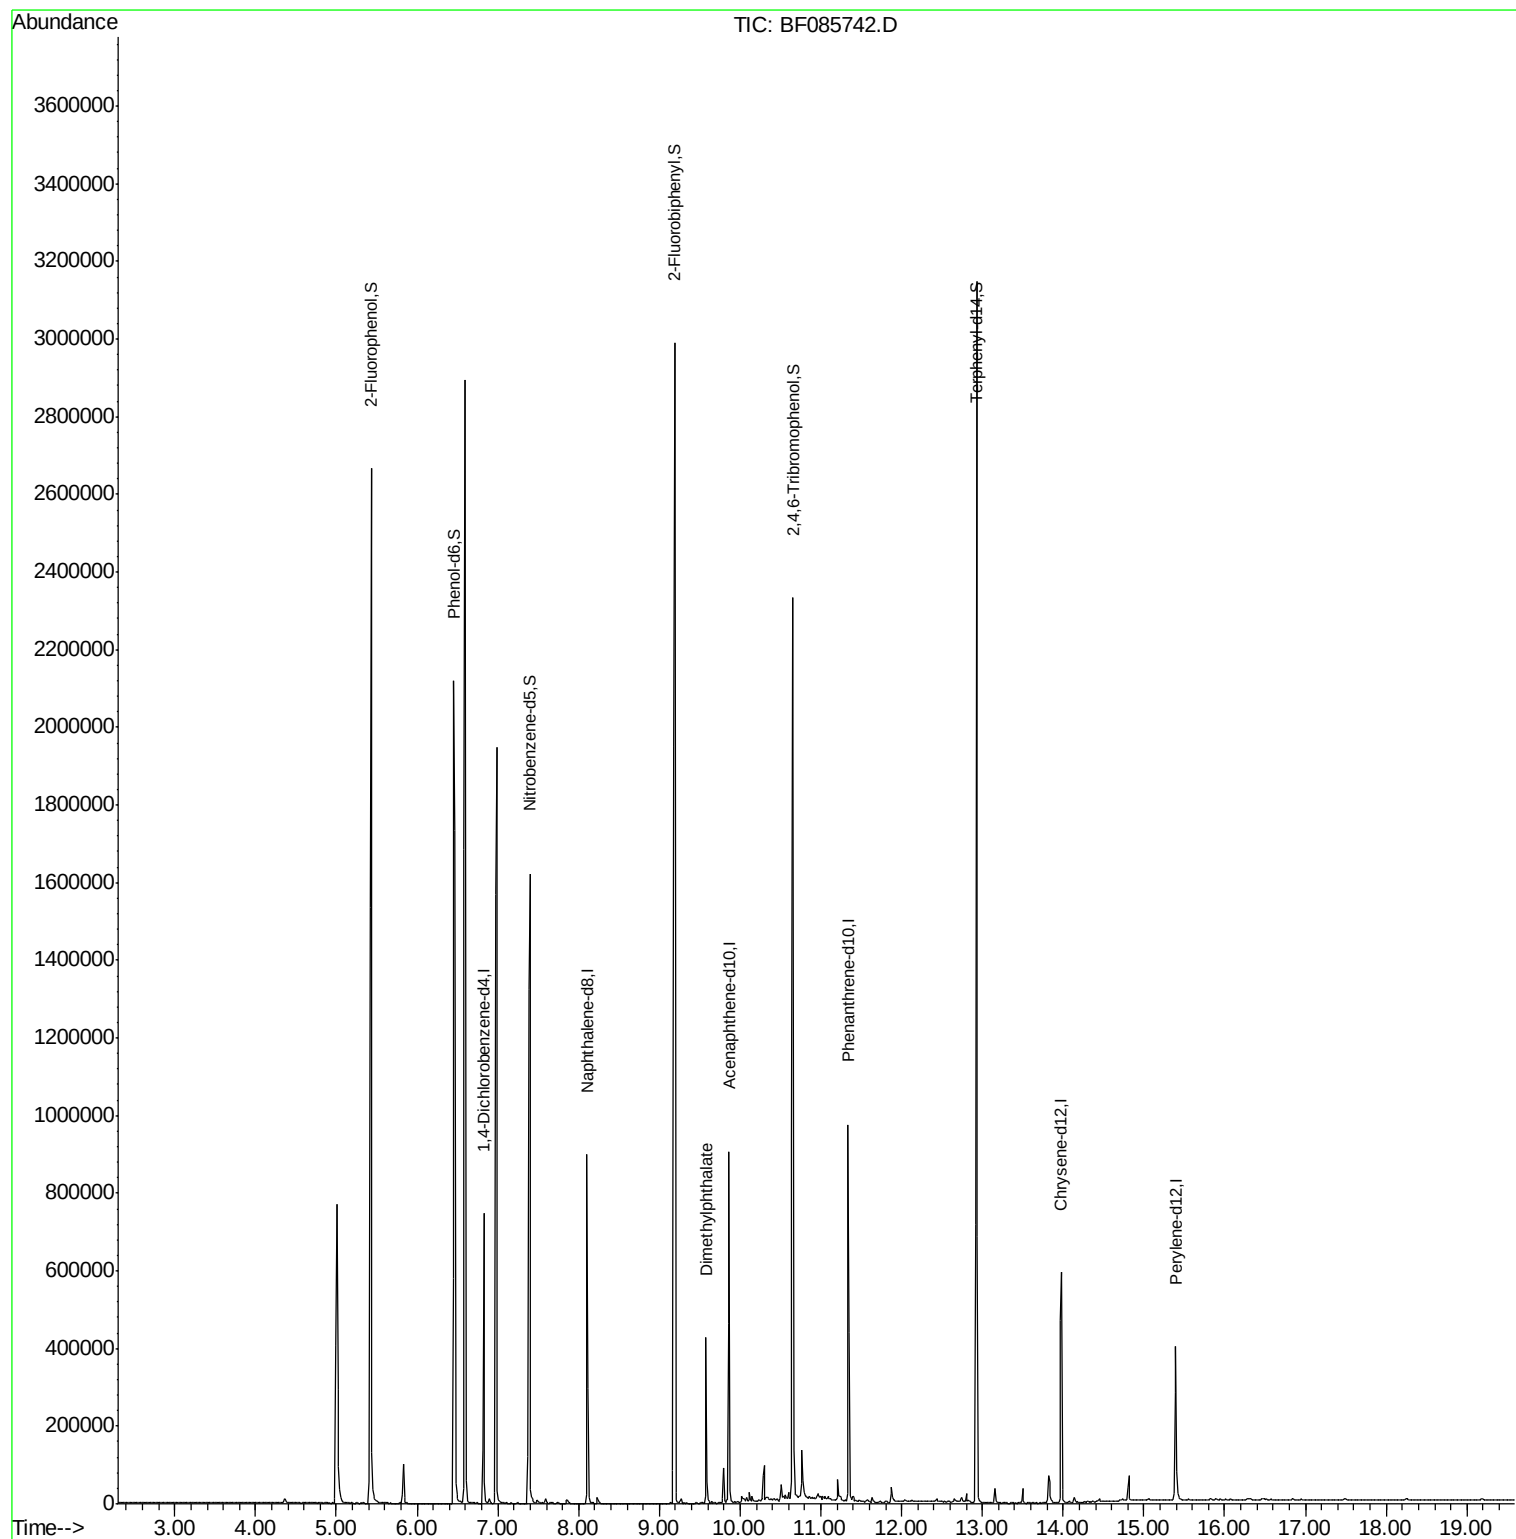

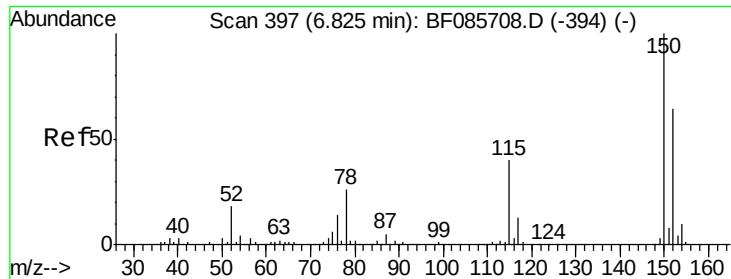

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.82 min Scan# 397

Delta R.T. -0.00 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10

Instrument :

BNA_F

ClientSampleId :

GW-01(18-20)


Tgt Ion:152 Resp: 111026

Ion Ratio Lower Upper

152 100

150 156.4 124.2 186.2




115 61.2 47.0 70.6

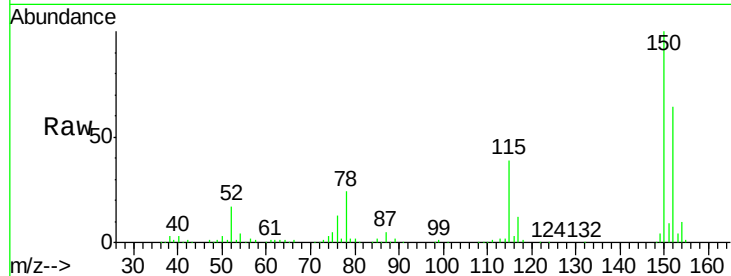

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

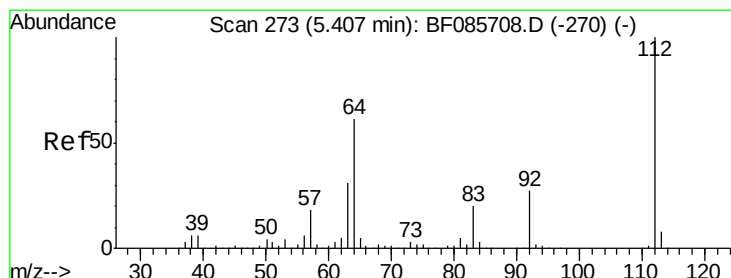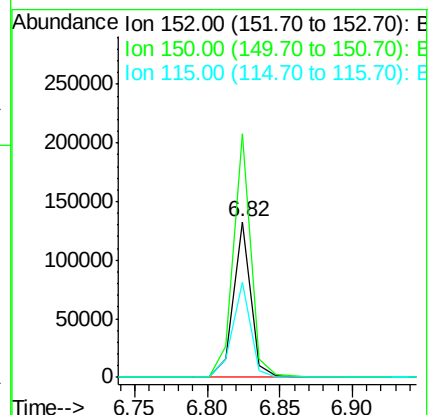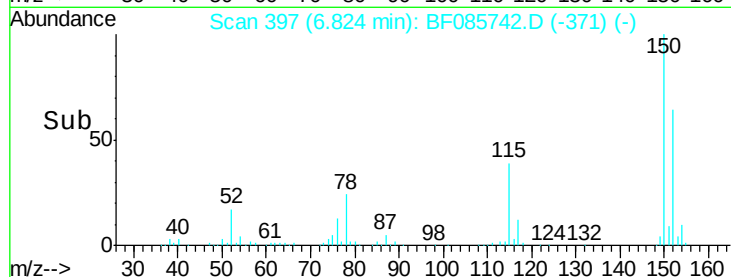

#5

2-Fluorophenol

Concen: 142.44 ng

RT: 5.43 min Scan# 275

Delta R.T. 0.02 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10


Tgt Ion:112 Resp: 949605

Ion Ratio Lower Upper

112 100

64 50.9 39.9 59.9



63 25.9 20.2 30.2

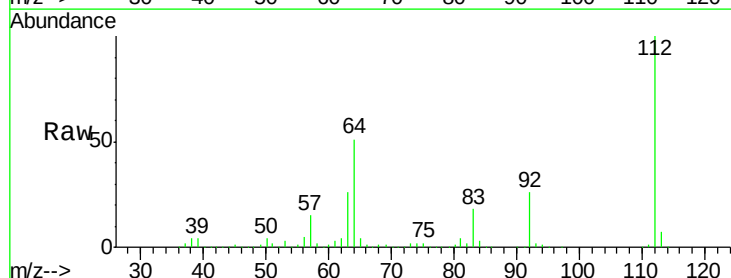


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

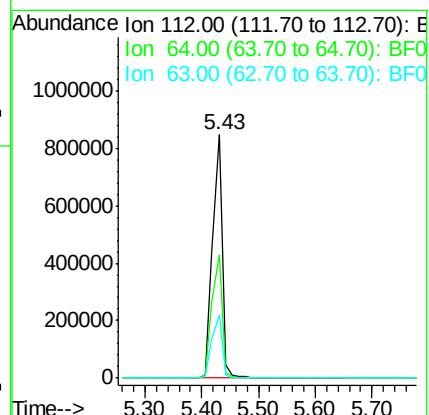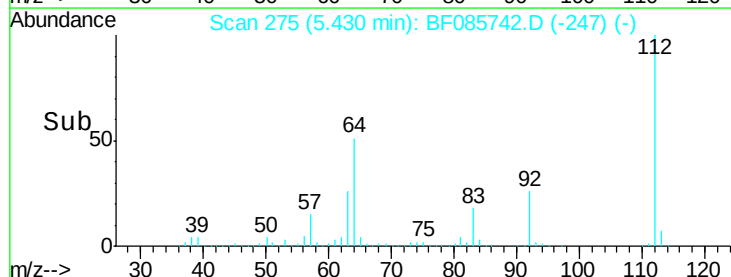

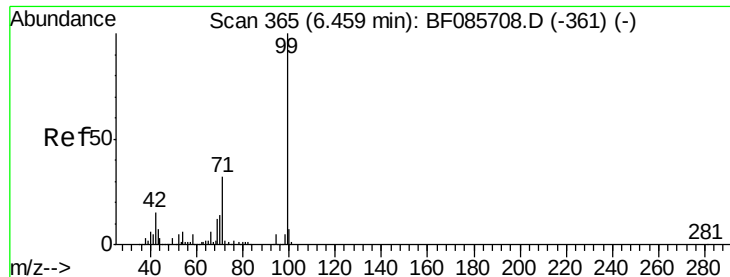

#7

Phenol-d6

Concen: 146.43 ng

RT: 6.46 min Scan# 365

Delta R.T. -0.00 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10

Instrument :

BNA_F

ClientSampleId :

GW-01(18-20)


Tgt Ion: 99 Resp: 1241172

Ion Ratio Lower Upper

99 100

42 15.6 11.1 16.7




71 32.8 24.9 37.3

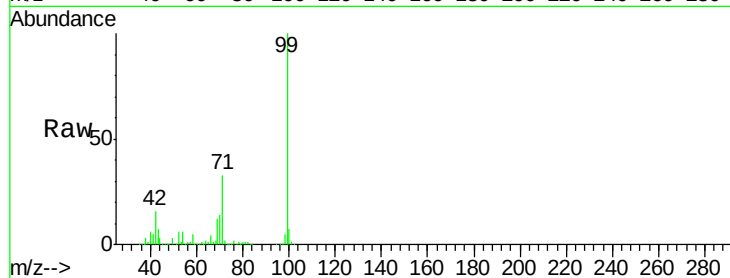

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

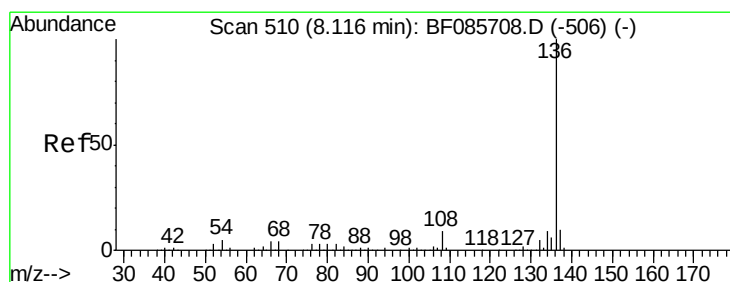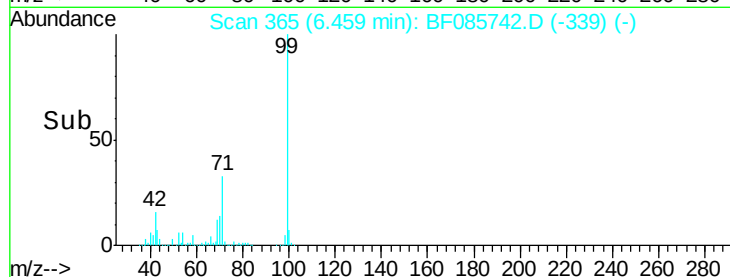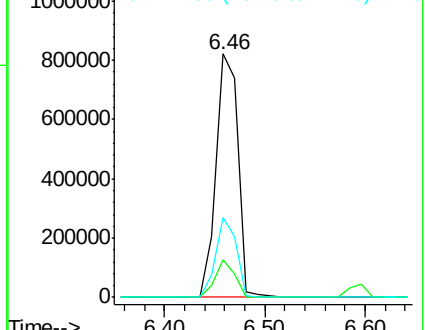

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.10 min Scan# 509

Delta R.T. -0.01 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10

Tgt Ion: 136 Resp: 429440


Ion Ratio Lower Upper

136 100

137 11.2 9.1 13.7

54 8.2 7.4 11.0

68 6.5 5.8 8.8


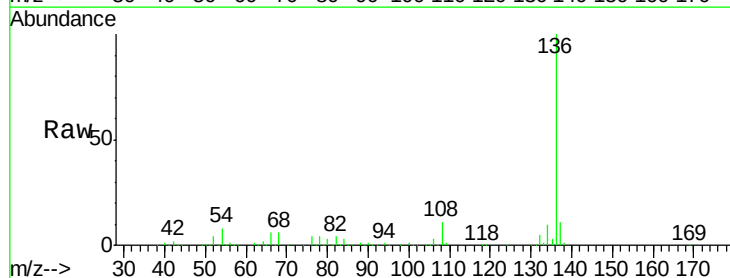



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

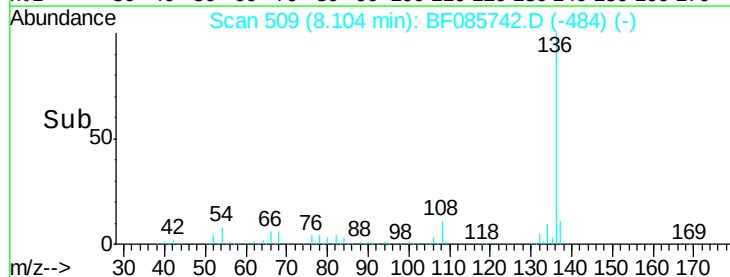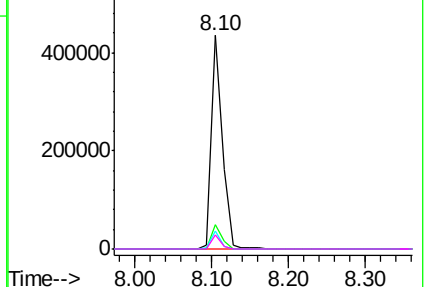


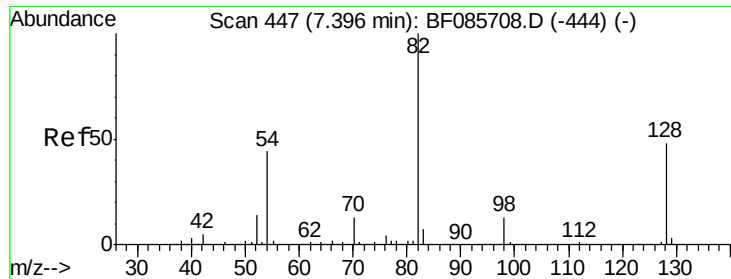




#23
 Nitrobenzene-d5
 Concen: 102.19 ng
 RT: 7.40 min Scan# 447
 Delta R.T. -0.00 min
 Lab File: BF085742.D
 Acq: 25 Mar 2016 5:10

Instrument :
 BNA_F
 ClientSampleId :
 GW-01(18-20)

Tgt Ion: 82 Resp: 779304
 Ion Ratio Lower Upper
 82 100
 128 54.2 41.8 62.8
 54 39.5 33.4 50.0

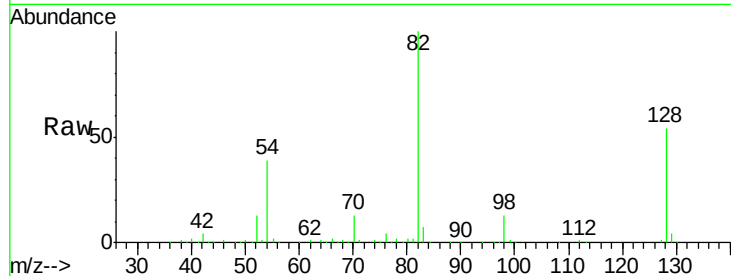


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

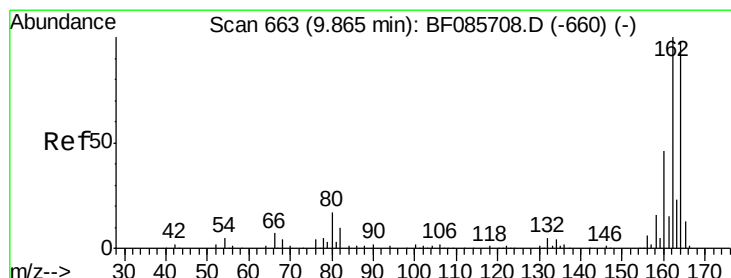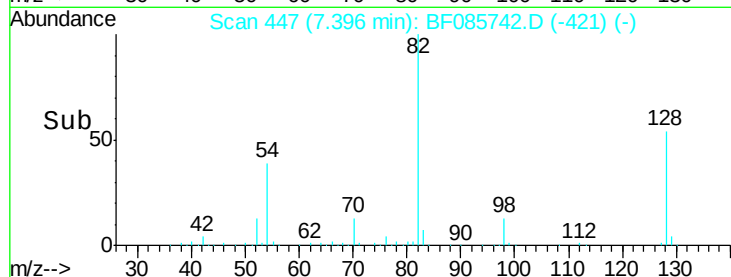
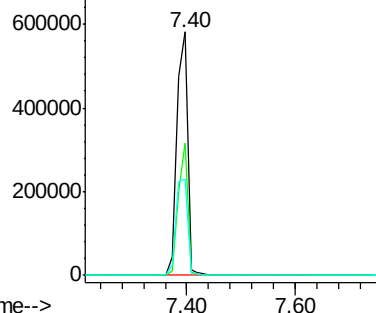



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.86 min Scan# 663
 Delta R.T. -0.00 min
 Lab File: BF085742.D
 Acq: 25 Mar 2016 5:10

Tgt Ion: 164 Resp: 205414
 Ion Ratio Lower Upper
 164 100
 162 103.4 82.1 123.1
 160 49.3 37.4 56.2

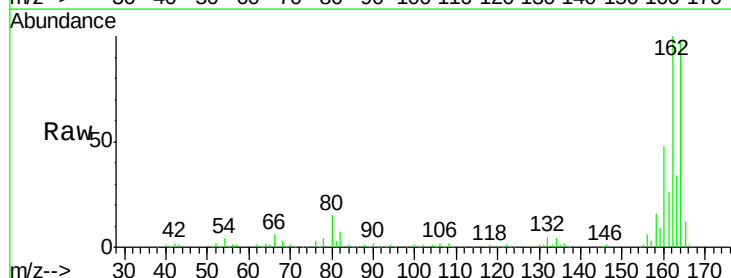

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



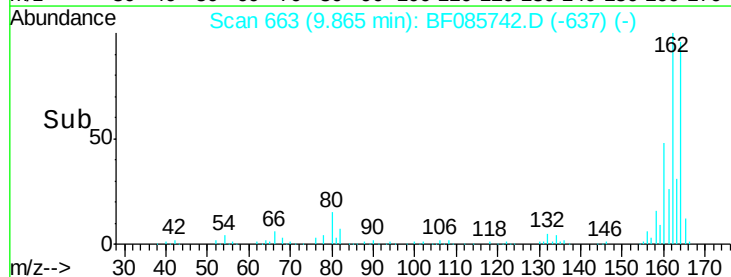
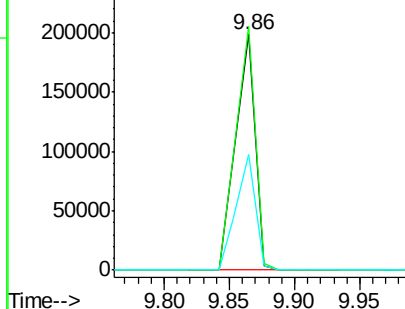


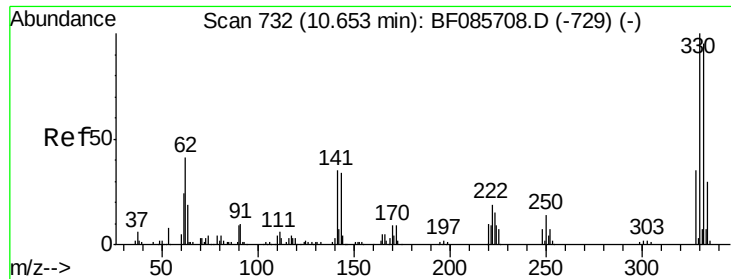

#41
 2,4,6-Tribromophenol
 Concen: 158.43 ng
 RT: 10.65 min Scan# 732
 Delta R.T. -0.00 min
 Lab File: BF085742.D
 Acq: 25 Mar 2016 5:10




Instrument :
 BNA_F
 ClientSampleId :
 GW-01(18-20)


Tgt Ion	Ratio	Lower	Upper
330	100		
332	96.0	78.2	117.2
141	36.2	31.5	47.3

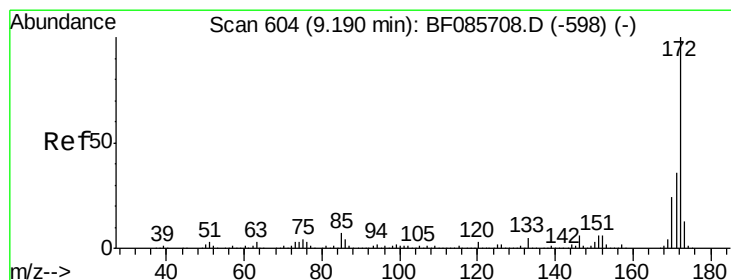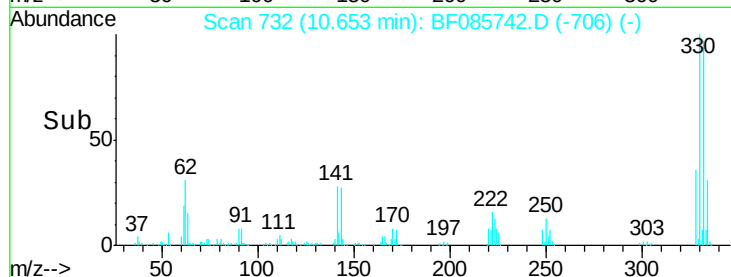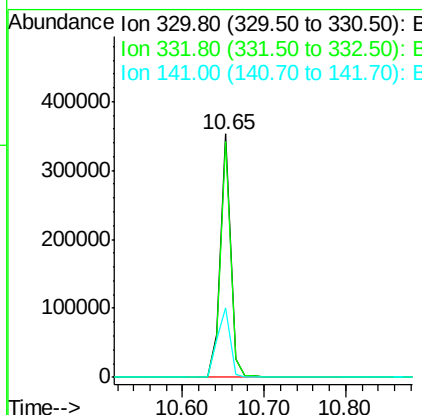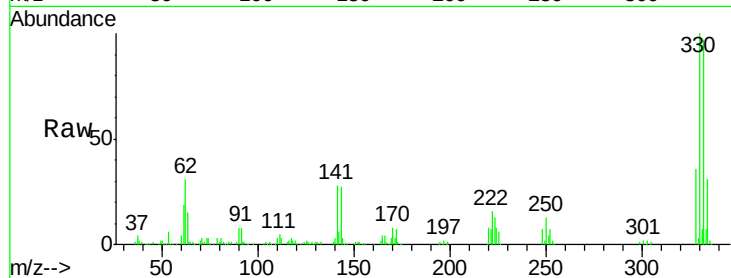

#44
 2-Fluorobiphenyl
 Concen: 97.90 ng
 RT: 9.19 min Scan# 604
 Delta R.T. -0.00 min
 Lab File: BF085742.D
 Acq: 25 Mar 2016 5:10

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.2	29.4	44.2
170	24.2	19.8	29.6

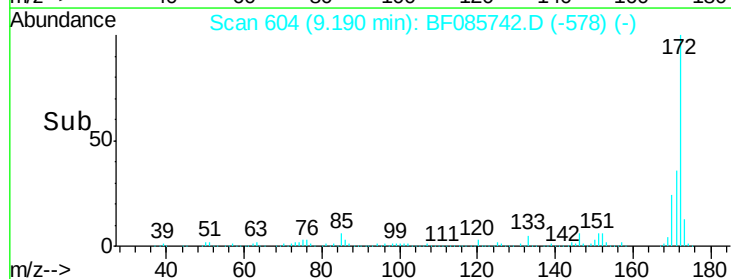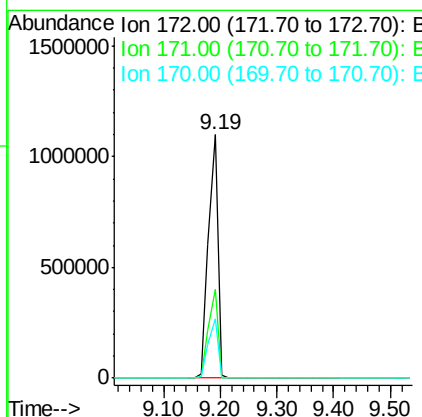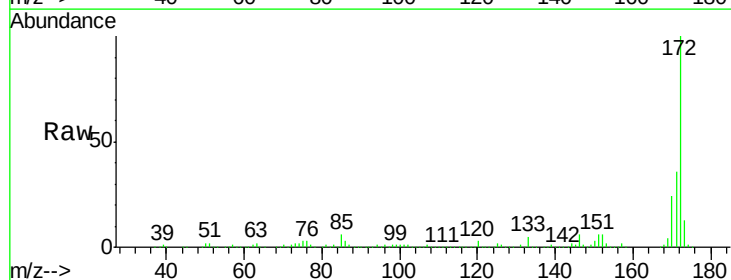

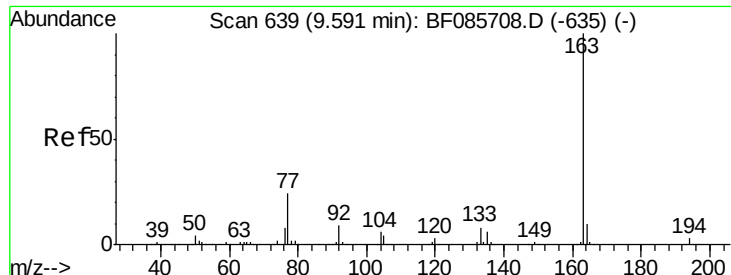

#49

Dimethylphthalate

Concen: 9.94 ng

RT: 9.58 min Scan# 638

Delta R.T. -0.01 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10

Instrument :

BNA_F

ClientSampleId :

GW-01(18-20)


Tgt Ion:163 Resp: 154981

Ion Ratio Lower Upper

163 100

194 3.2 2.9 4.3




164 9.8 8.3 12.5

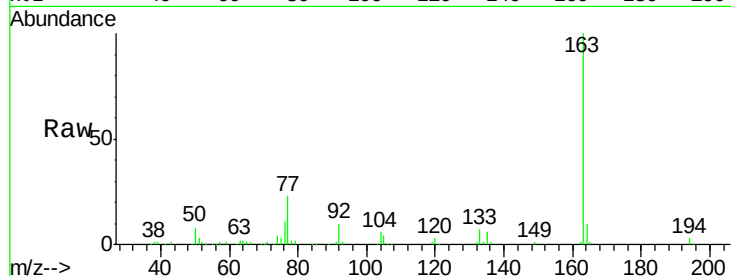

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

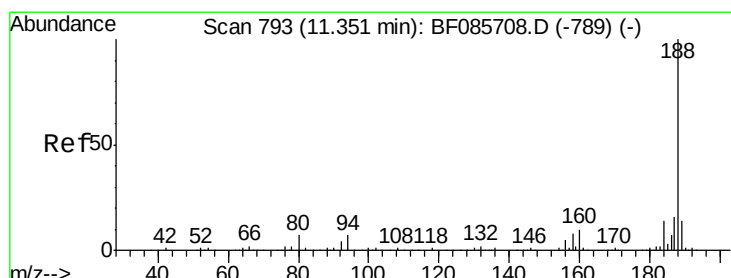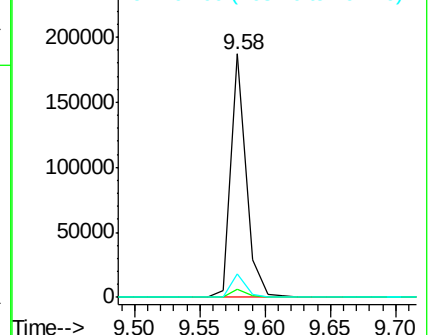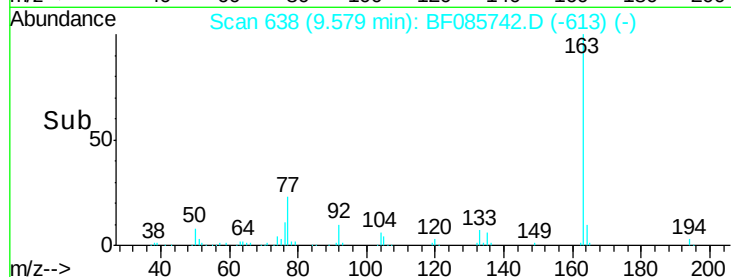

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.34 min Scan# 792

Delta R.T. -0.01 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10


Tgt Ion:188 Resp: 387085

Ion Ratio Lower Upper

188 100

94 13.3 5.4 8.0#



80 14.3 5.5 8.3#

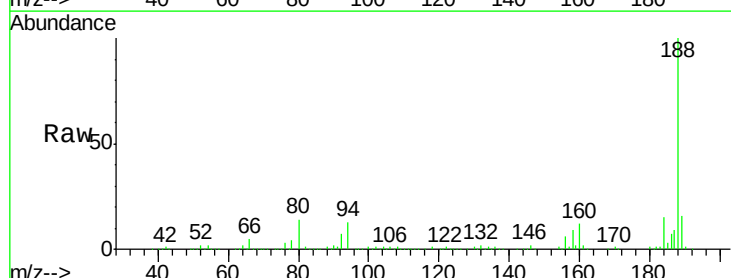


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

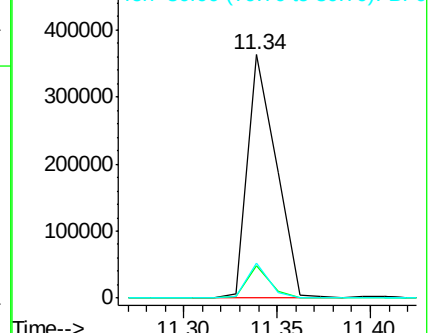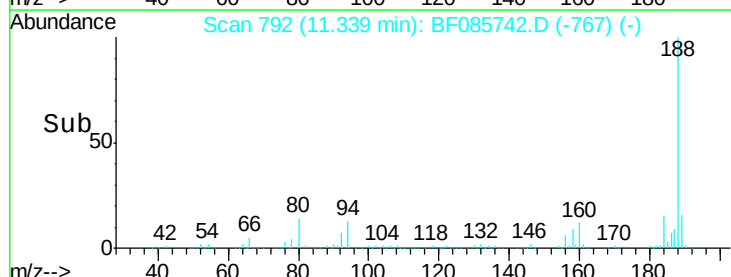

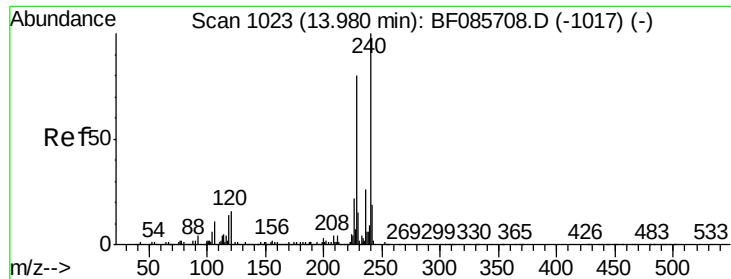

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.98 min Scan# 1023

Delta R.T. -0.00 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10

Instrument :

BNA_F

ClientSampleId :

GW-01(18-20)


Tgt Ion:240 Resp: 274951

Ion Ratio Lower Upper

240 100

120 8.6 13.8 20.8#




236 26.7 20.6 30.8

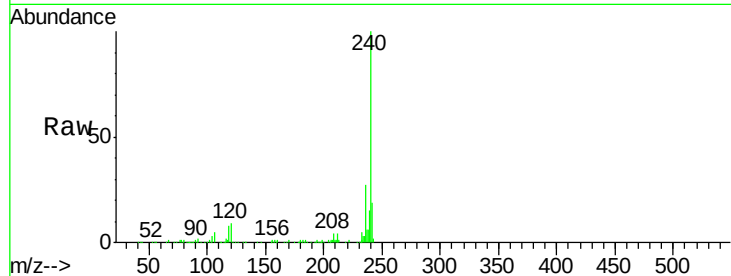

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

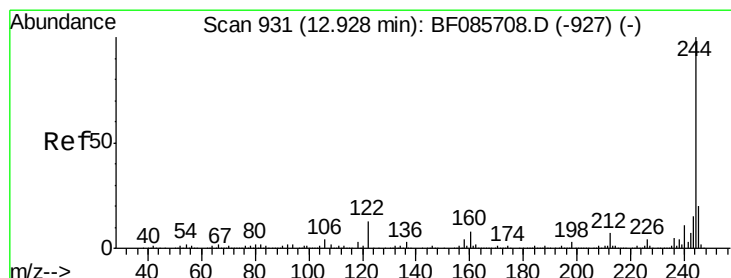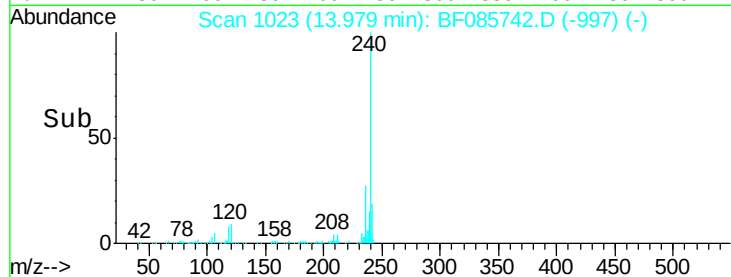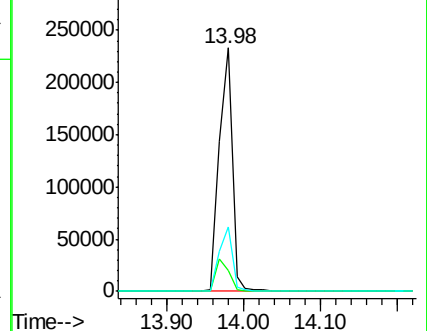

#78

Terphenyl-d14

Concen: 78.24 ng

RT: 12.93 min Scan# 931

Delta R.T. -0.00 min

Lab File: BF085742.D

Acq: 25 Mar 2016 5:10


Tgt Ion:244 Resp: 1046014

Ion Ratio Lower Upper

244 100

212 7.5 6.1 9.1



122 12.8 10.2 15.4

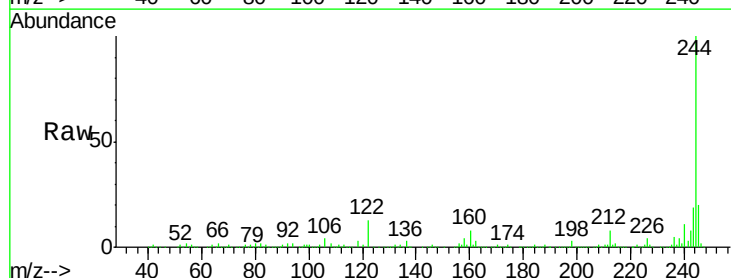


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

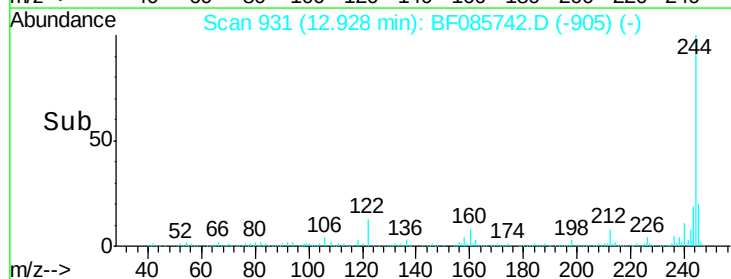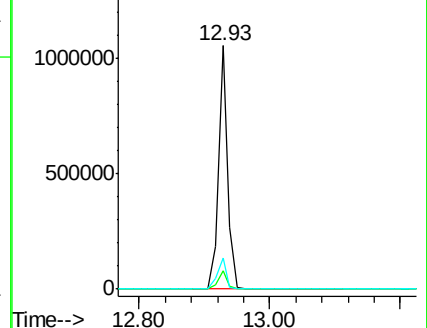


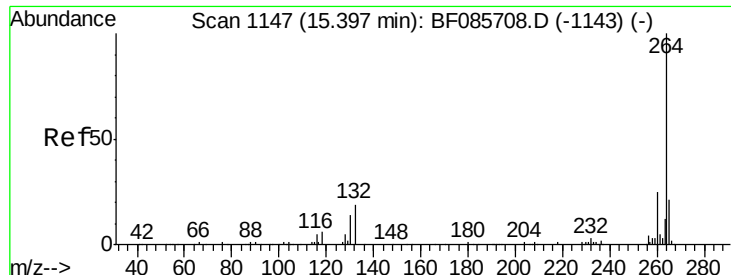

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.40 min Scan# 1147
Delta R.T. -0.00 min
Lab File: BF085742.D
Acq: 25 Mar 2016 5:10

Instrument :
BNA_F
ClientSampleId :
GW-01(18-20)

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.8	19.4	29.2
265	20.7	17.2	25.8

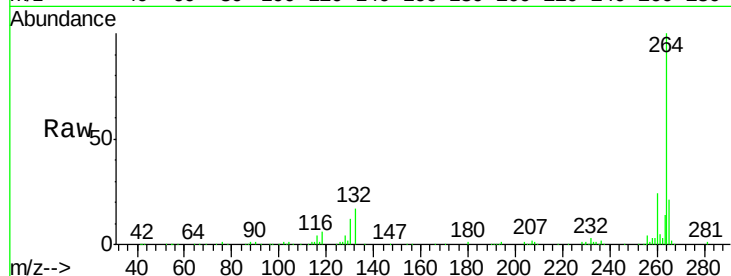

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

