

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
 Data File : BF085716.D
 Acq On : 24 Mar 2016 15:59
 Operator : UM/SJ
 Sample : PB88875BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB88875BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.030	237	240	246	rBV	28320	46157	1.40%	0.188%
2	5.430	272	275	277	rBV	1810669	2586715	78.30%	10.513%
3	6.459	362	365	367	rBV	2374475	2448111	74.10%	9.950%
4	6.596	374	377	379	rBV	1971812	2715743	82.20%	11.038%
5	6.824	394	397	399	rBV	690508	617759	18.70%	2.511%
6	6.973	408	410	413	rBV	1536337	2148236	65.02%	8.731%
7	7.385	443	446	449	rBV	1397560	1604499	48.57%	6.521%
8	8.105	507	509	512	rBV	851405	808863	24.48%	3.287%
9	9.190	601	604	606	rBV	2791549	3303779	100.00%	13.428%
10	9.865	660	663	665	rBV	823862	910757	27.57%	3.702%
11	10.653	729	732	734	rBV	1878022	2060917	62.38%	8.376%
12	11.339	790	792	795	rBV	989290	962151	29.12%	3.910%
13	12.928	928	931	934	rBV	3243002	3117405	94.36%	12.670%
14	13.979	1020	1023	1025	rBV	635805	770244	23.31%	3.131%
15	15.397	1144	1147	1155	rBV	337238	503155	15.23%	2.045%


Sum of corrected areas: 24604491

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
Data File : BF085716.D
Acq On : 24 Mar 2016 15:59
Operator : UM/SJ
Sample : PB88875BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88875BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

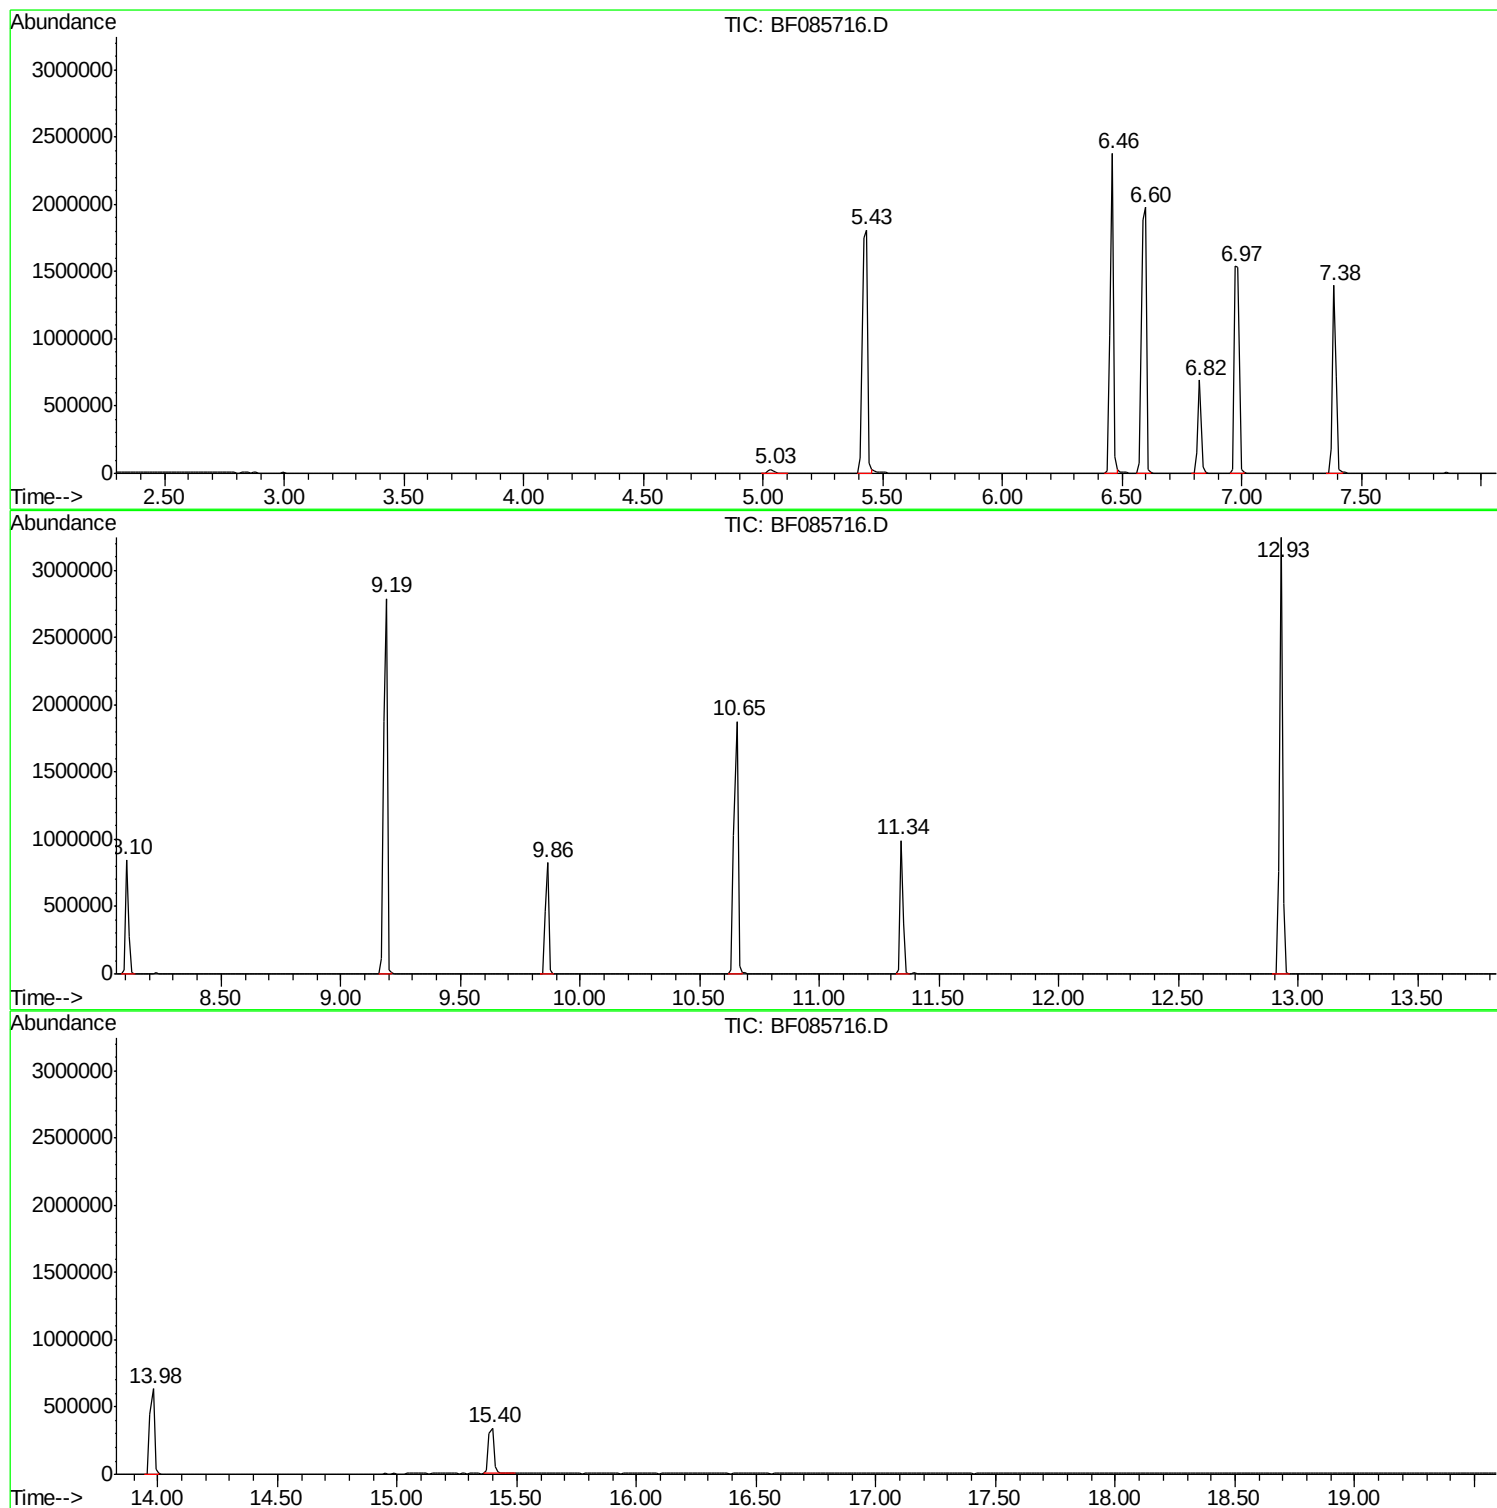

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
Data File : BF085716.D
Acq On : 24 Mar 2016 15:59
Operator : UM/SJ
Sample : PB88875BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88875BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	87.92 ng	2715740	1,4-Dichlorobenzene-d4	6.82

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	38
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	25
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		1H-Benzimidazole, 2-methyl-	132	C8H8N2	000615-15-6	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

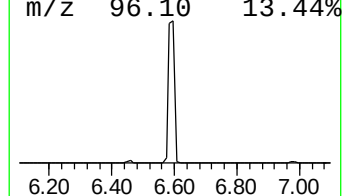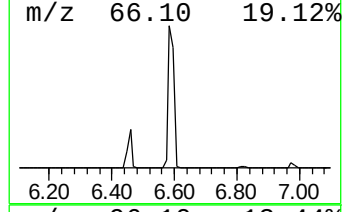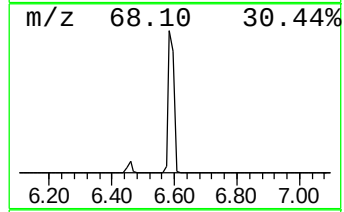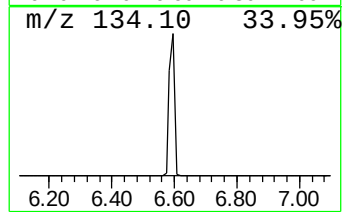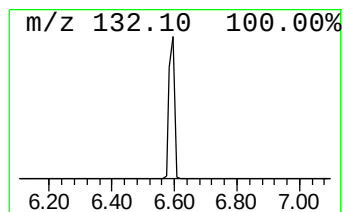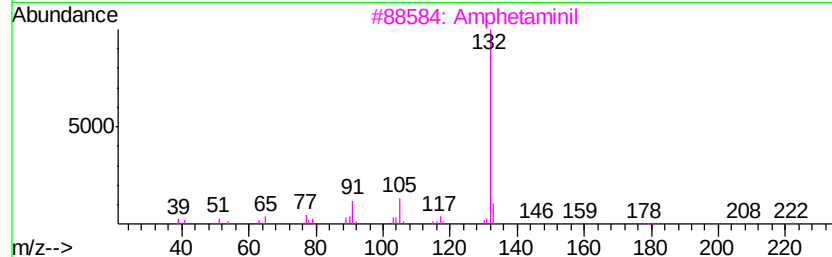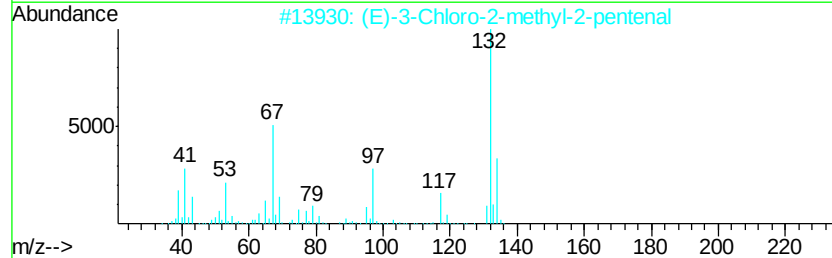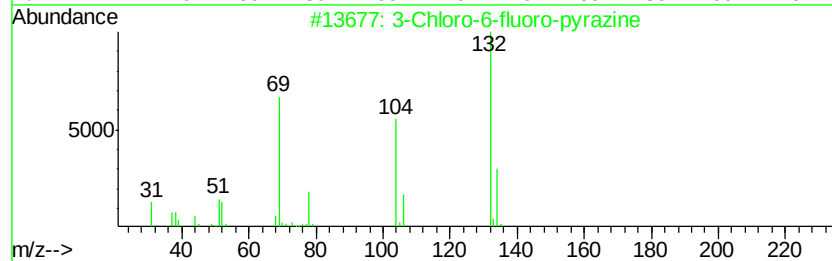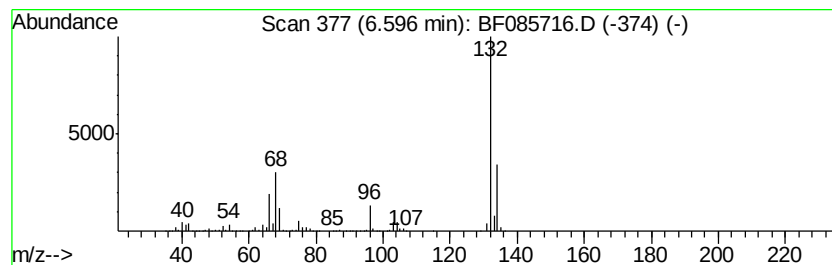

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
Data File : BF085716.D
Acq On : 24 Mar 2016 15:59
Operator : UM/SJ
Sample : PB88875BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB88875BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.60	6.60	87.9	ng	2715740	1	6.82	617759	20.0