


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
 Data File : BF085704.D
 Acq On : 24 Mar 2016 9:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 14:15:39 2016

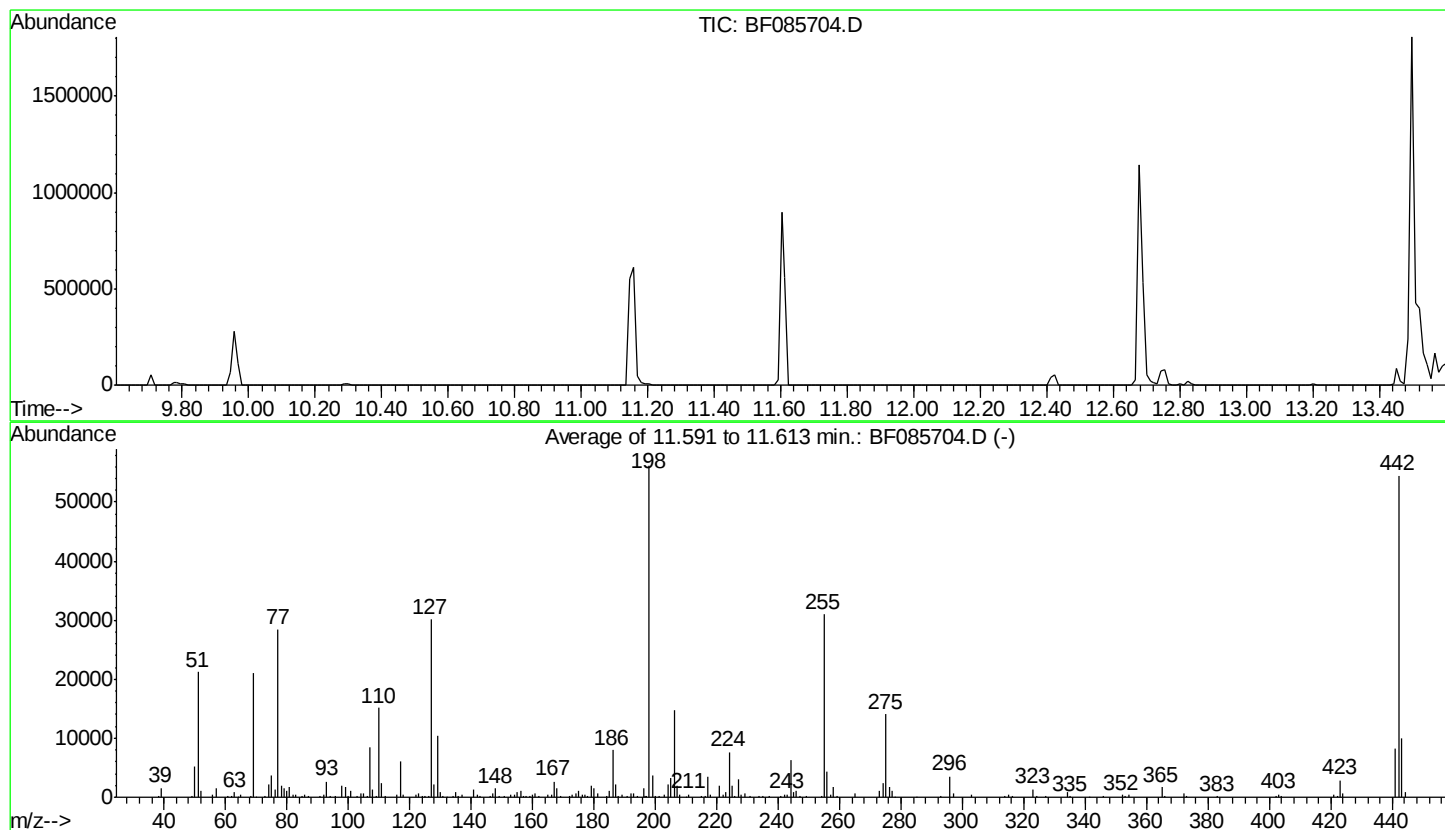

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	21209	PASS
68	69	0.00	2	1.5	305	PASS
69	198	0.00	100	37.4	21018	PASS
70	69	0.00	2	0.5	115	PASS
127	198	10	80	53.6	30115	PASS
197	198	0.00	2	0.4	243	PASS
198	198	100	100	100.0	56179	PASS
199	198	5	9	6.6	3733	PASS
275	198	10	60	24.9	14010	PASS
365	198	1	100	3.1	1728	PASS
441	442	0.01	24	15.3	8325	PASS
442	198	50	100	96.9	54464	PASS
443	442	15	24	18.4	10031	PASS