


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
 Data File : BF085714.D
 Acq On : 24 Mar 2016 15:03
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 14:15:39 2016

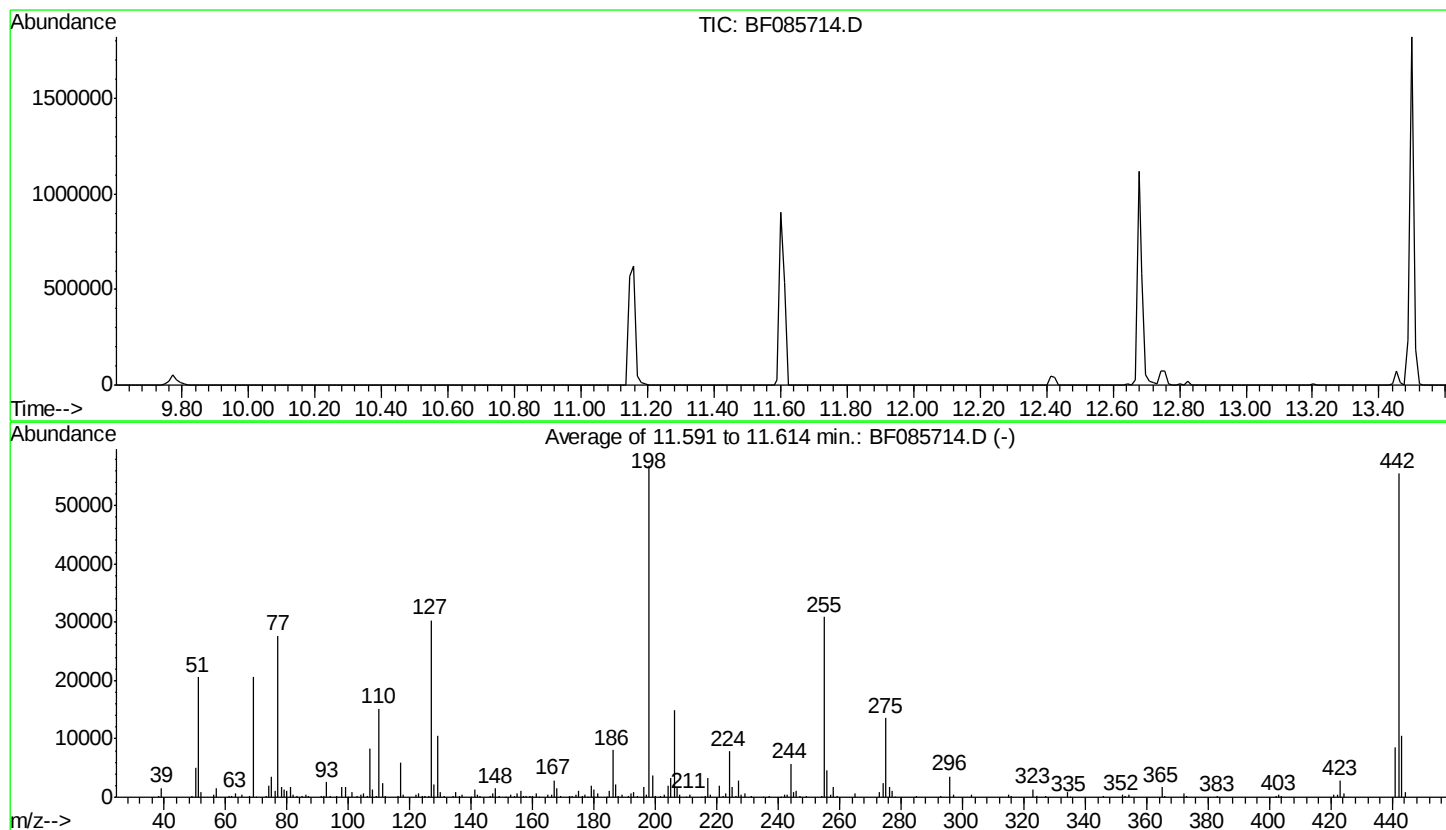

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	20614	PASS
68	69	0.00	2	1.4	298	PASS
69	198	0.00	100	36.4	20693	PASS
70	69	0.00	2	0.5	103	PASS
127	198	10	80	53.3	30306	PASS
197	198	0.00	2	0.8	459	PASS
198	198	100	100	100.0	56818	PASS
199	198	5	9	6.7	3834	PASS
275	198	10	60	23.8	13501	PASS
365	198	1	100	3.0	1697	PASS
441	442	0.01	24	15.3	8470	PASS
442	198	50	100	97.6	55445	PASS
443	442	15	24	18.8	10432	PASS