


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032416\
 Data File : BF085733.D
 Acq On : 25 Mar 2016 00:55
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 24 14:15:39 2016

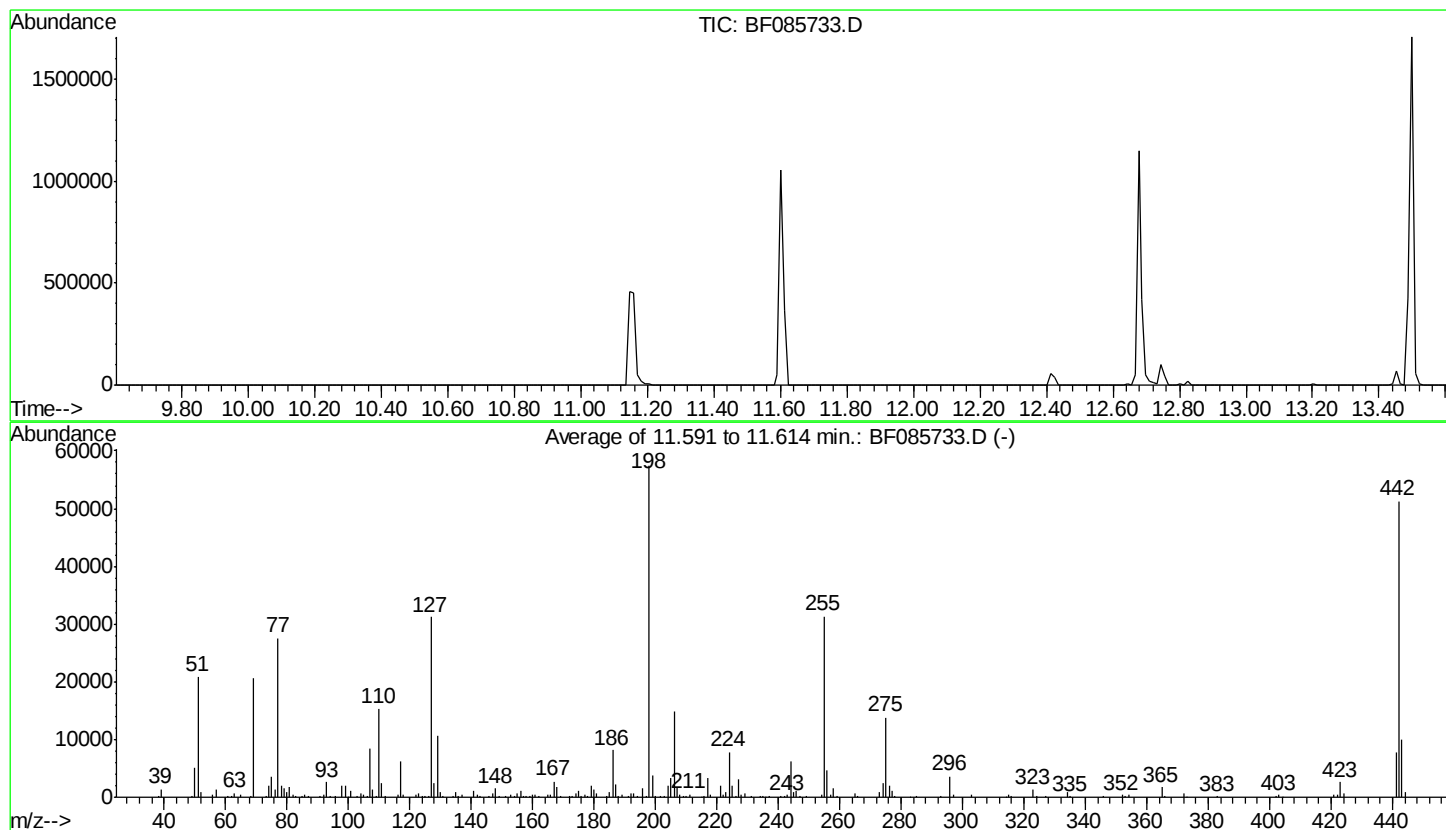

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.5	20959	PASS
68	69	0.00	2	1.5	302	PASS
69	198	0.00	100	35.9	20632	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.3	31185	PASS
197	198	0.00	2	0.6	317	PASS
198	198	100	100	100.0	57443	PASS
199	198	5	9	6.6	3808	PASS
275	198	10	60	24.1	13853	PASS
365	198	1	100	2.9	1690	PASS
441	442	0.01	24	15.3	7861	PASS
442	198	50	100	89.3	51277	PASS
443	442	15	24	19.3	9884	PASS