
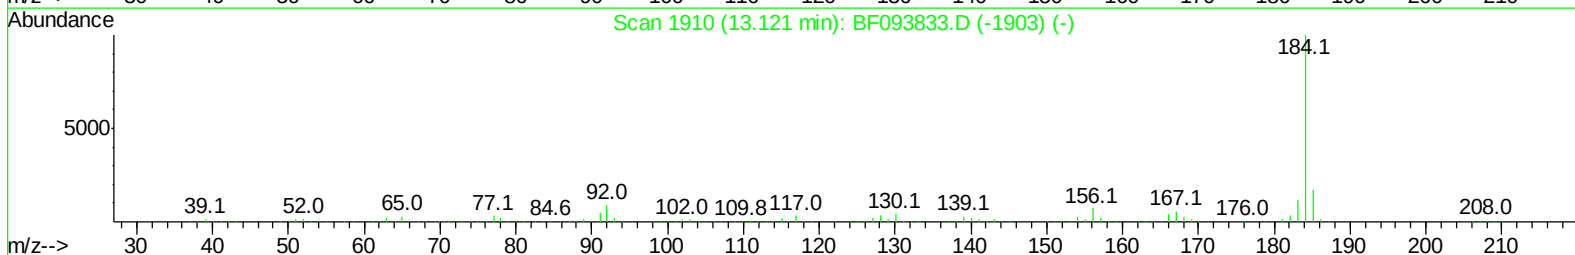
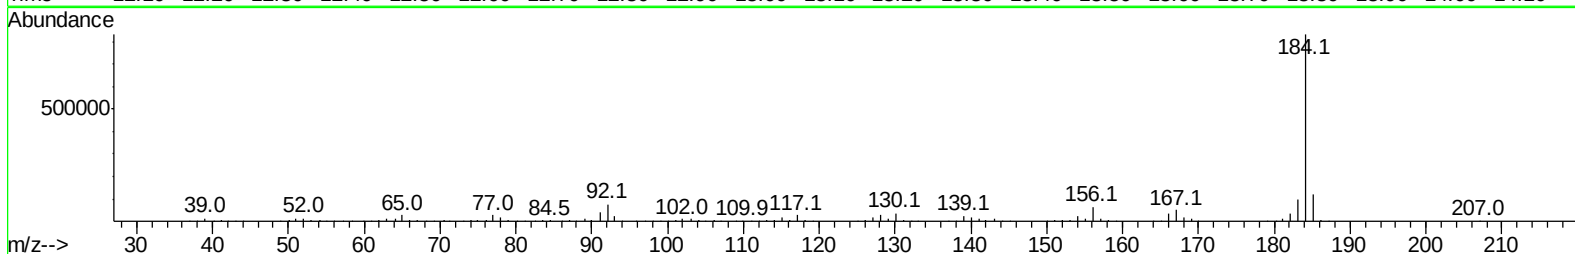


Data Path : Z:\HPCHEM1\BNA F\Data\BF032417\
 Data File : BF093898.D
 Acq On : 24 Mar 2017 10:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 00:38:11 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 23 02:02:22 2017
 Response via : Initial Calibration

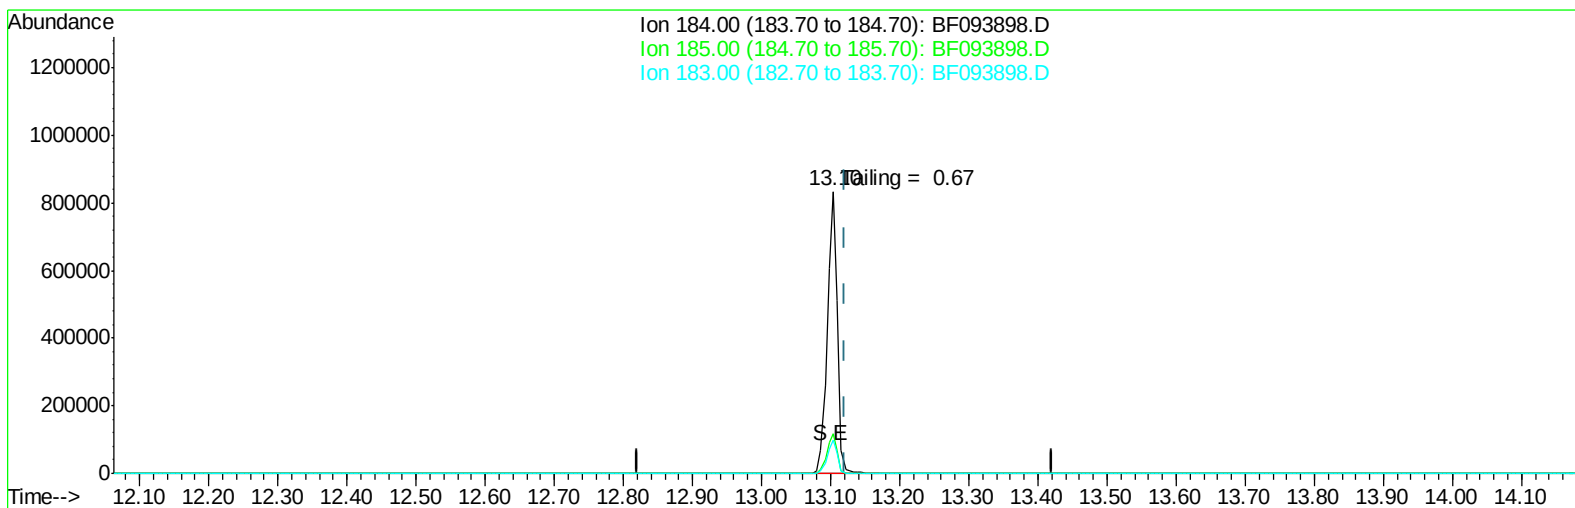

TIC: BF093898.D

(76) Benzidine




13.104min (-0.018) 0.00ng

response 843974

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.22#
183.00	12.20	11.91
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032417\
Data File : BF093898.D
Acq On : 24 Mar 2017 10:18
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 00:38:11 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

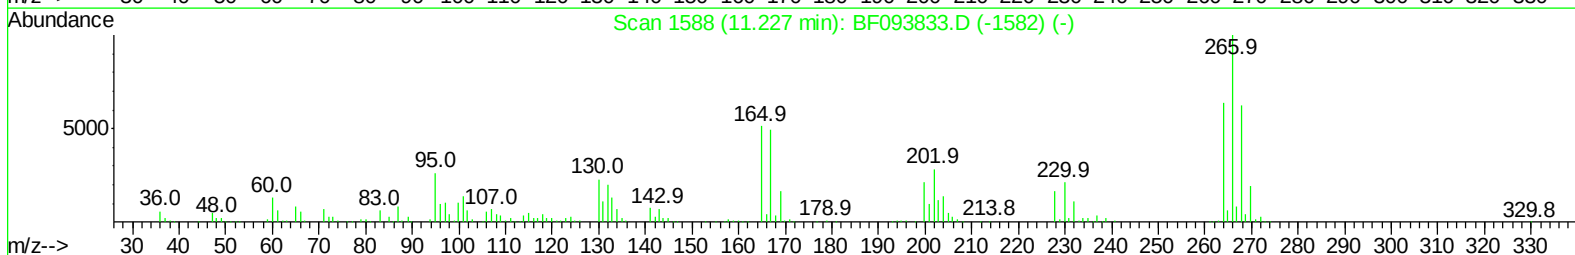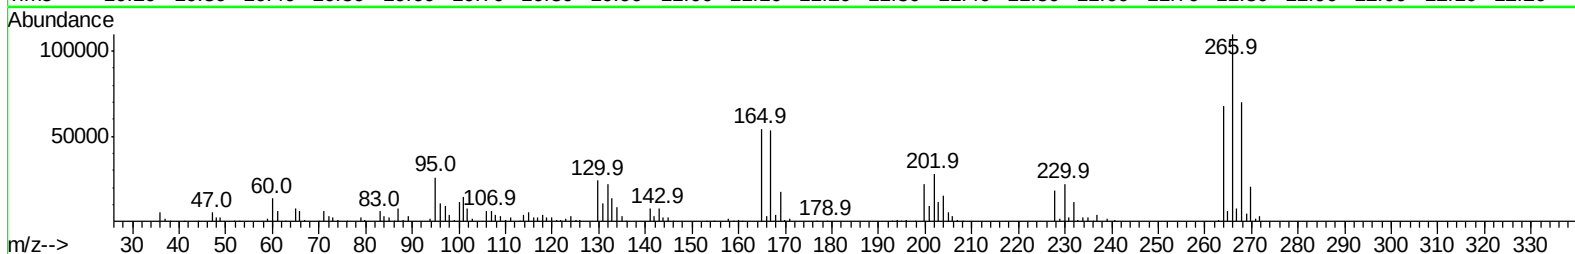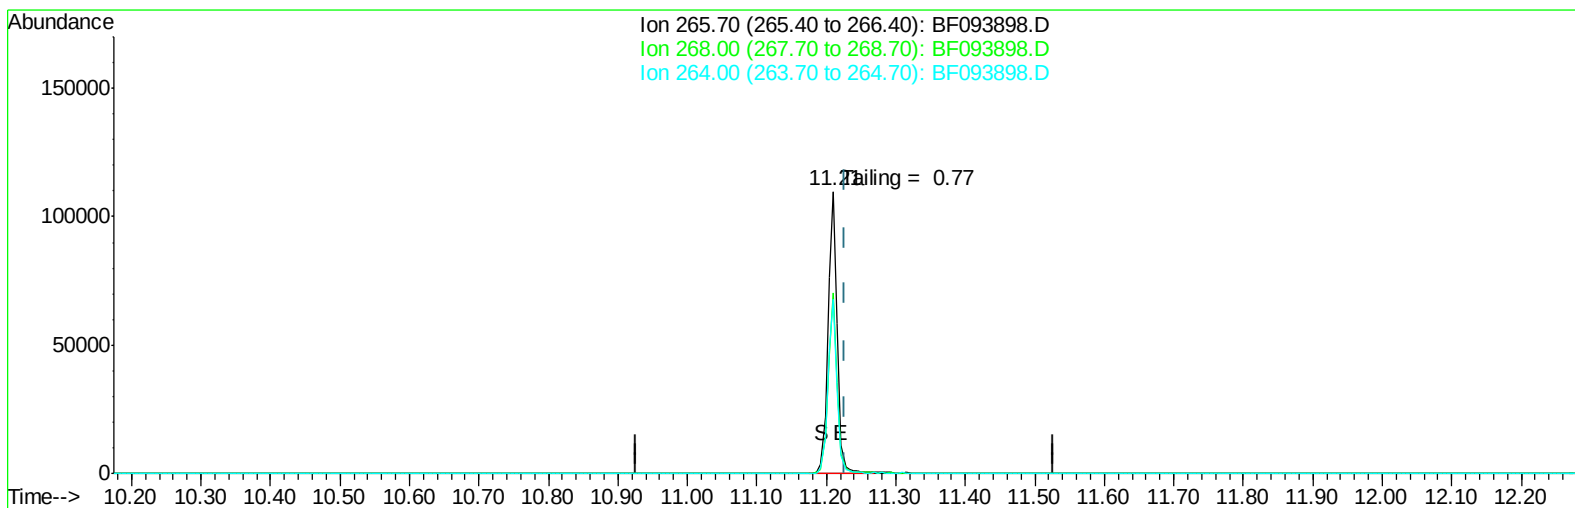

TIC: BF093898.D

(69) Pentachlorophenol (C)

11.210min (-0.018) 0.00ng

response 102044

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.89
264.00	64.60	61.96
0.00	0.00	0.00