
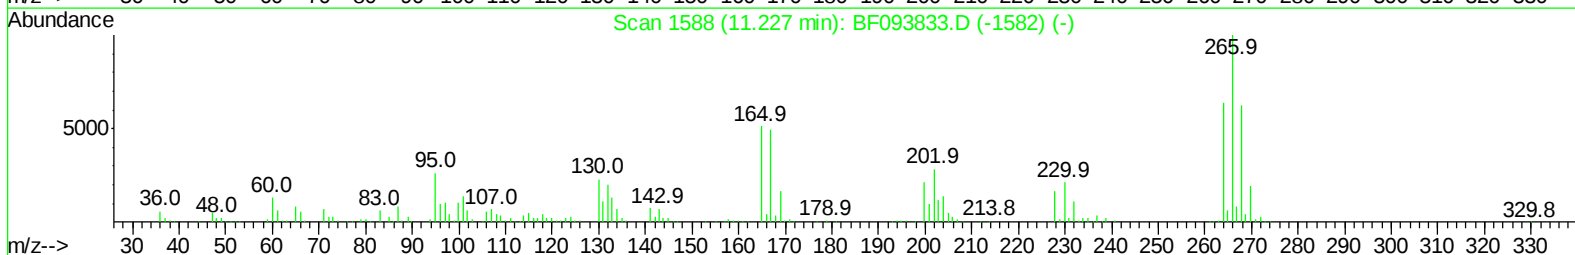
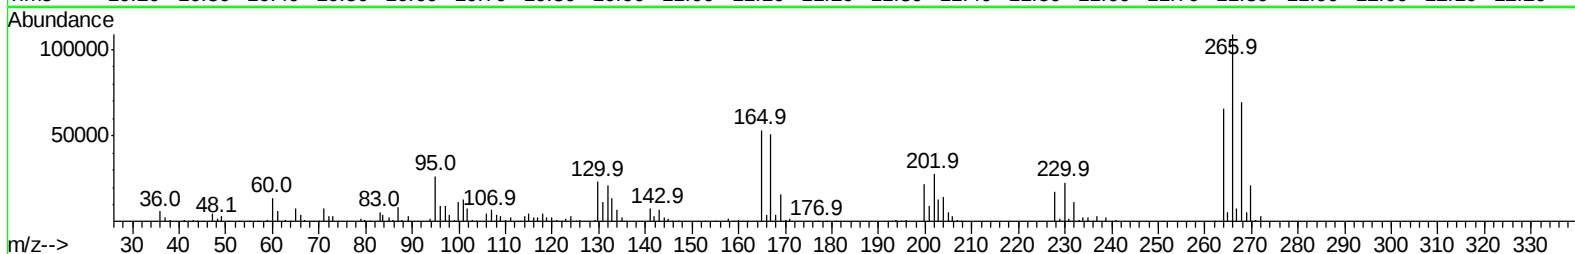


Data Path : Z:\HPCHEM1\BNA F\Data\BF032417\
Data File : BF093911.D
Acq On : 24 Mar 2017 17:19
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 00:38:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

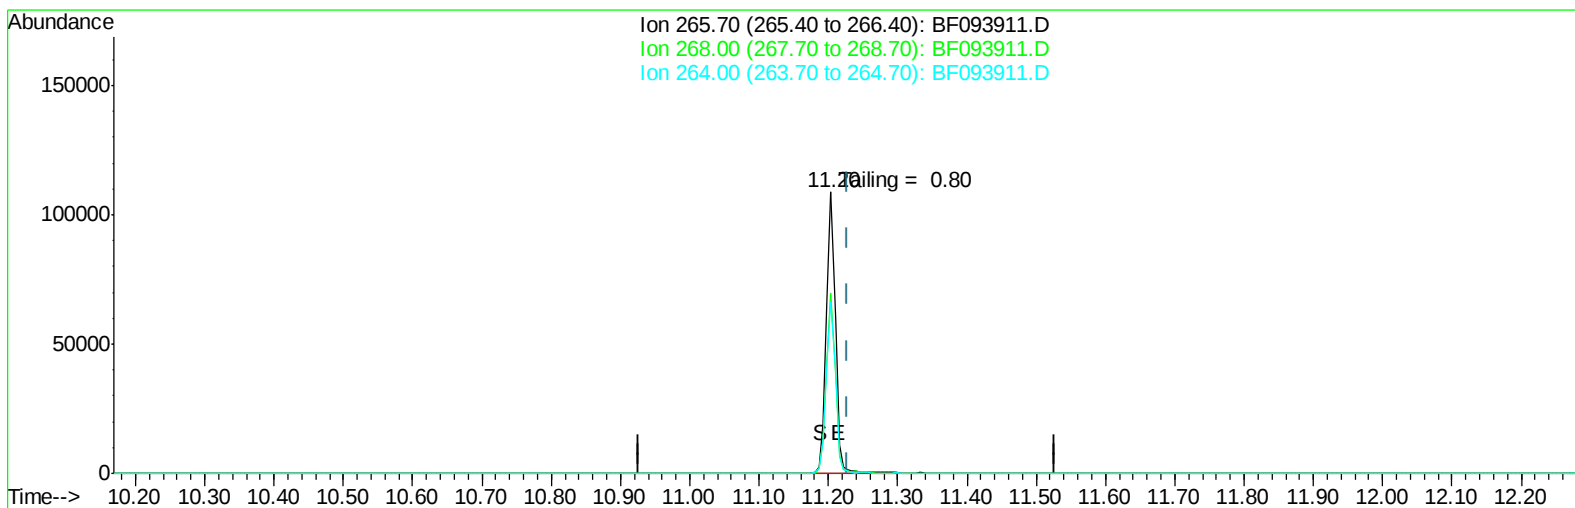

TIC: BF093911.D

(69) Pentachlorophenol (C)




11.204min (-0.023) 0.00ng

response 97333

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.09
264.00	64.60	60.71
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF032417\
Data File : BF093911.D
Acq On : 24 Mar 2017 17:19
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 00:38:59 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 23 02:02:22 2017
Response via : Initial Calibration

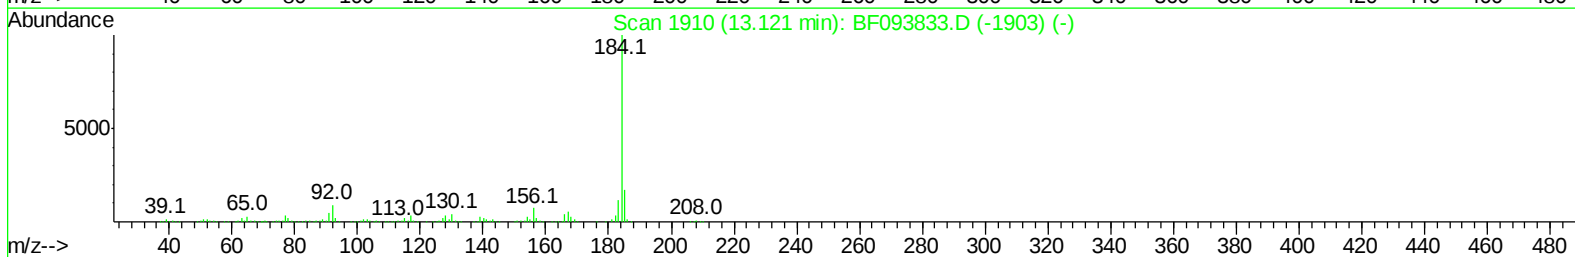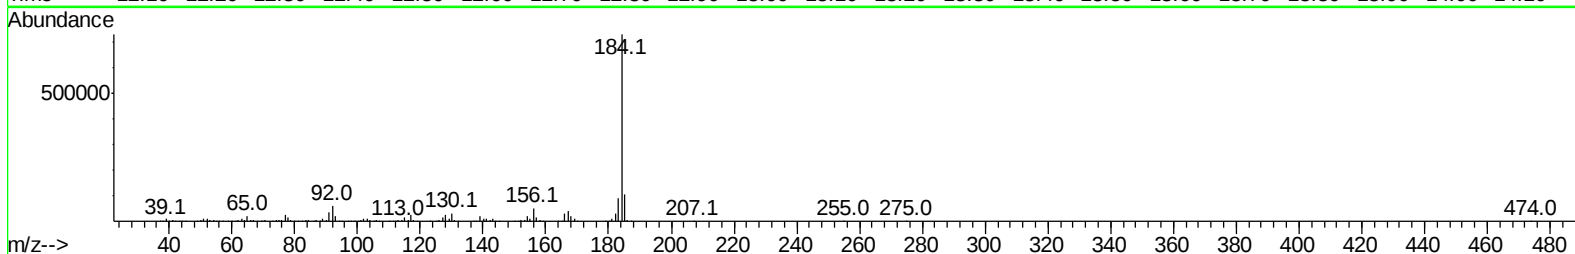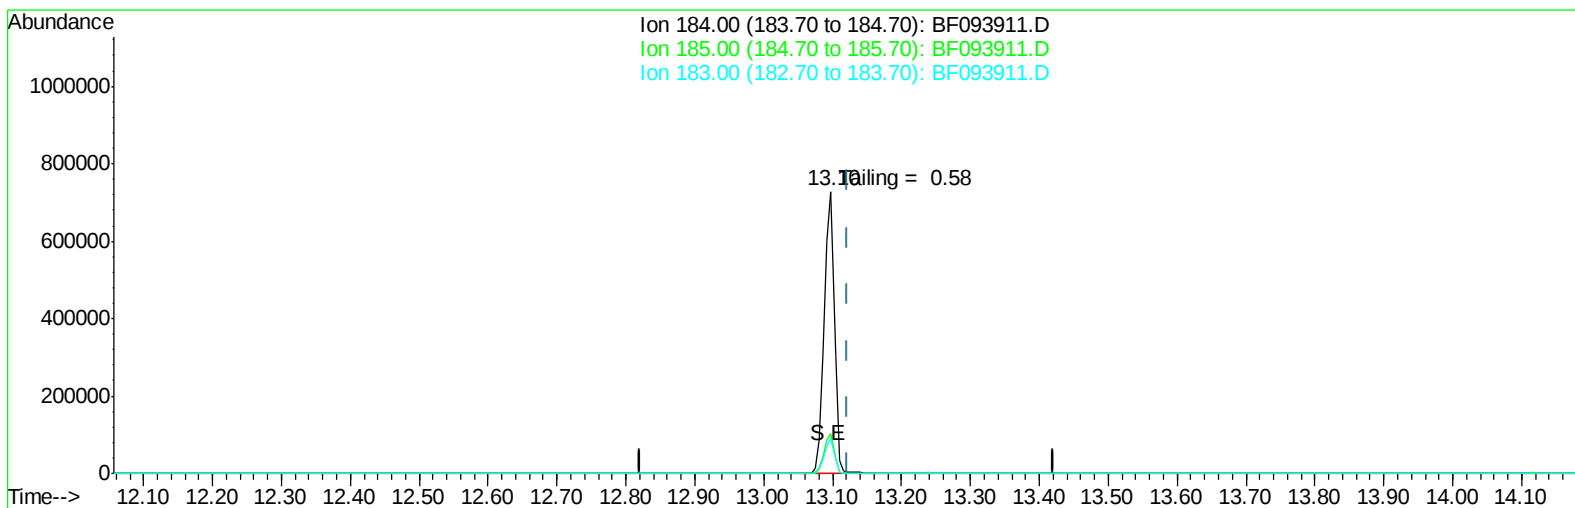

TIC: BF093911.D

(76) Benzidine

13.098min (-0.023) 0.00ng

response 742498

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.26#
183.00	12.20	12.13
0.00	0.00	0.00