


Data Path : Z:\HPCHEM1\BNA F\Data\BF032417\
 Data File : BF093898.D
 Acq On : 24 Mar 2017 10:18
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 23 02:02:22 2017

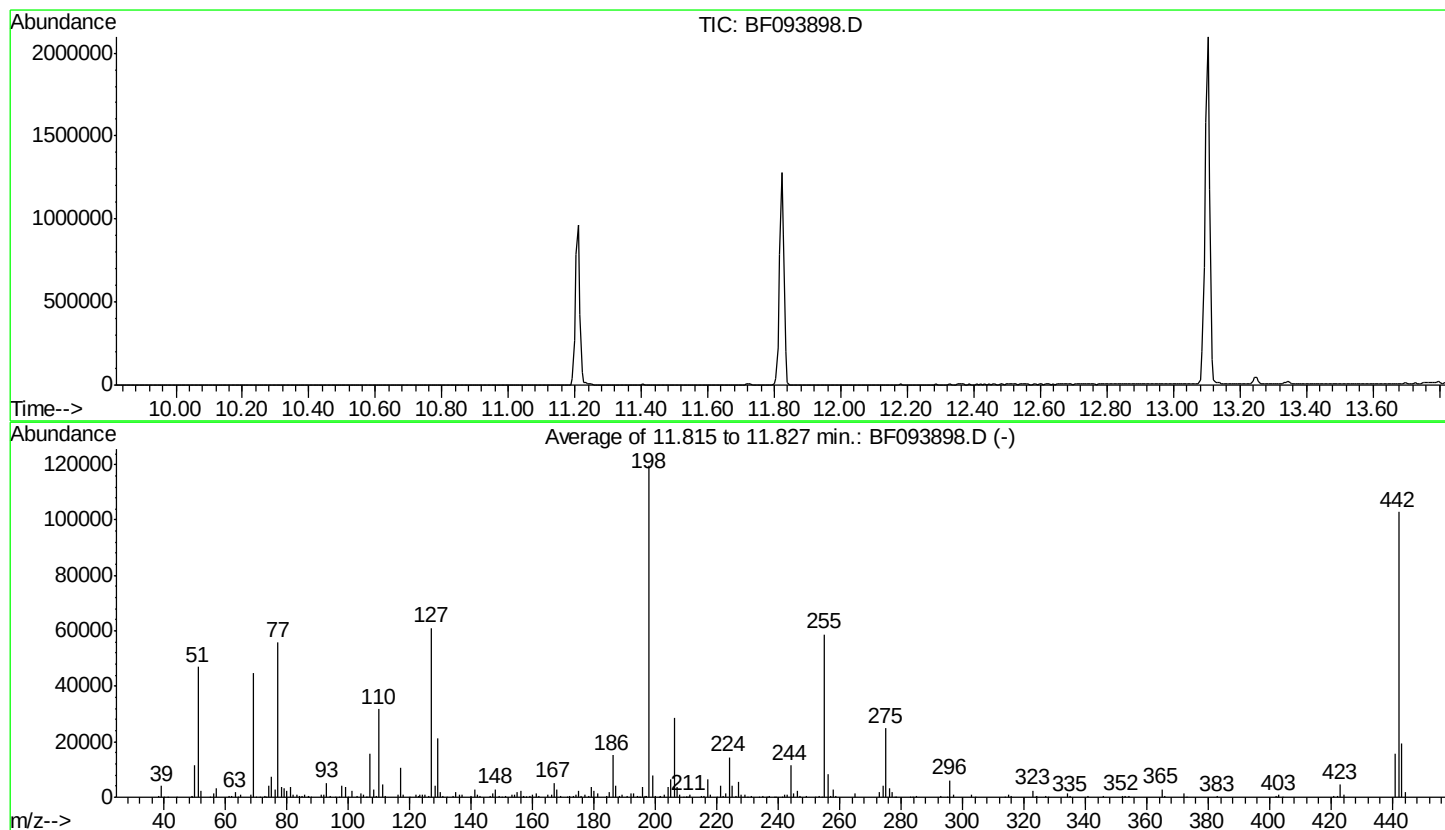

AutoFind: Scans 1688, 1689, 1690; Background Corrected with Scan 1682

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	47090	PASS
68	69	0.00	2	1.8	799	PASS
69	198	0.00	100	37.4	44736	PASS
70	69	0.00	2	0.5	237	PASS
127	198	10	80	51.1	61080	PASS
197	198	0.00	2	0.4	536	PASS
198	198	100	100	100.0	119634	PASS
199	198	5	9	6.7	8004	PASS
275	198	10	60	20.7	24808	PASS
365	198	1	100	2.4	2841	PASS
441	442	0.01	24	15.4	15821	PASS
442	198	50	100	85.9	102824	PASS
443	442	15	24	18.7	19254	PASS