


Data Path : Z:\HPCHEM1\BNA F\Data\BF032417\
 Data File : BF093911.D
 Acq On : 24 Mar 2017 17:19
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 23 02:02:22 2017

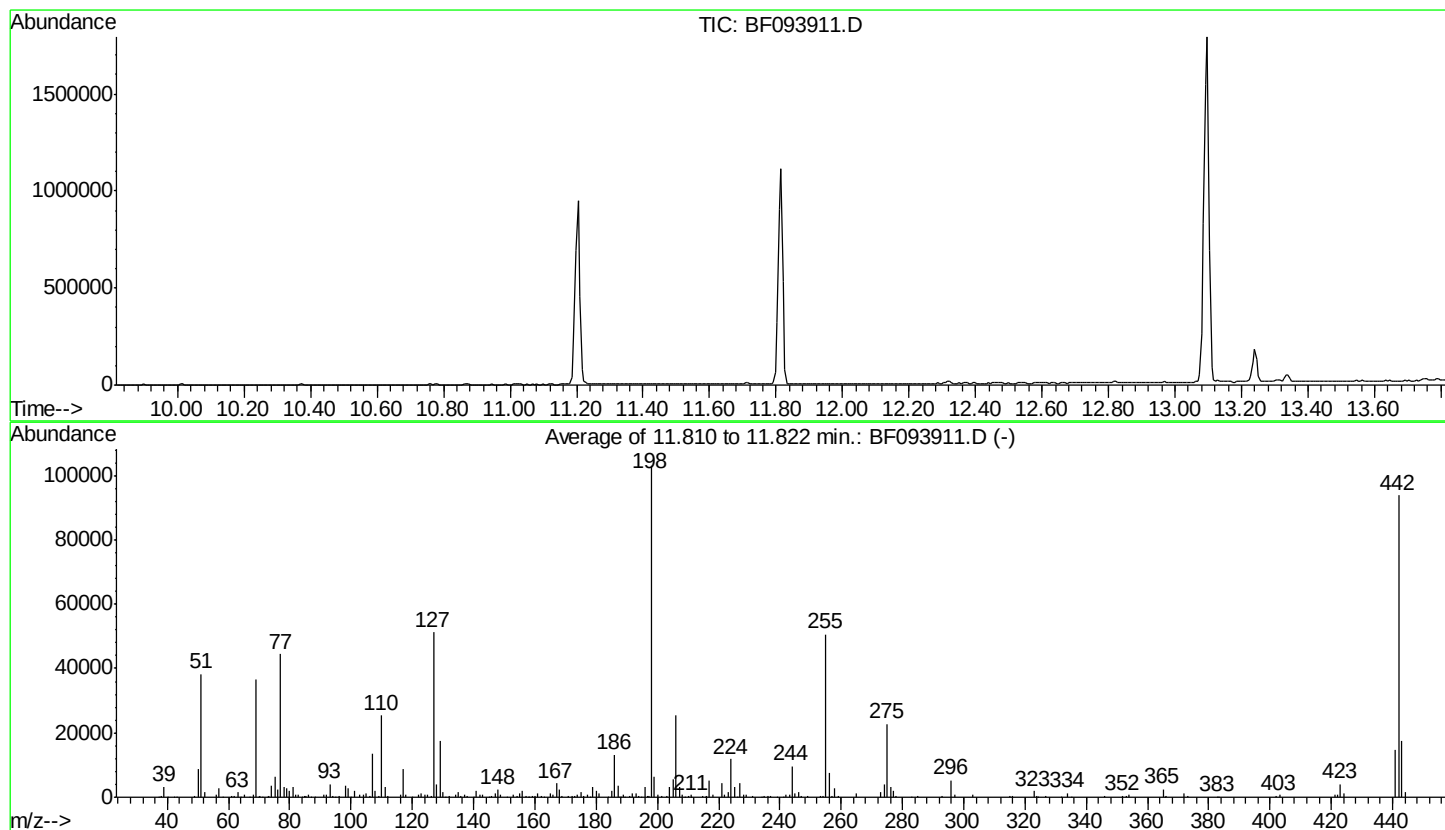

AutoFind: Scans 1687, 1688, 1689; Background Corrected with Scan 1680

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.3	38384	PASS
68	69	0.00	2	1.8	663	PASS
69	198	0.00	100	35.4	36469	PASS
70	69	0.00	2	0.7	259	PASS
127	198	10	80	49.6	51146	PASS
197	198	0.00	2	0.4	371	PASS
198	198	100	100	100.0	103042	PASS
199	198	5	9	6.4	6555	PASS
275	198	10	60	22.1	22749	PASS
365	198	1	100	2.5	2544	PASS
441	442	0.01	24	15.8	14851	PASS
442	198	50	100	91.1	93864	PASS
443	442	15	24	18.6	17474	PASS