


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032419\
 Data File : BF113260.D
 Acq On : 24 Mar 2019 10:43
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF022719.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 13 03:42:55 2019

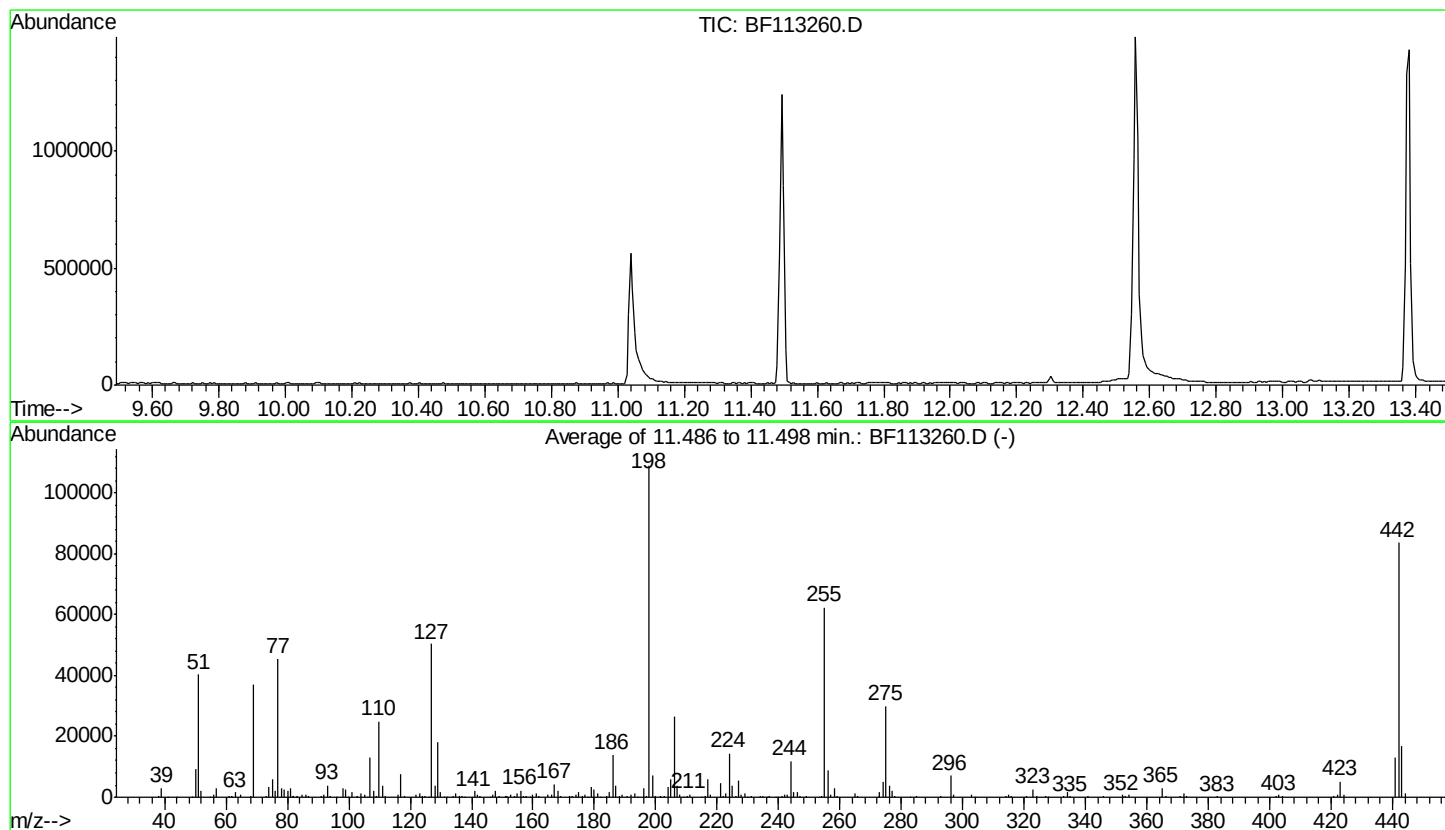

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.9	40176	PASS
68	69	0.00	2	1.6	598	PASS
69	198	0.00	100	33.9	36885	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.2	50357	PASS
197	198	0.00	2	0.4	419	PASS
198	198	100	100	100.0	108938	PASS
199	198	5	9	6.7	7278	PASS
275	198	10	60	27.5	29946	PASS
365	198	1	100	2.9	3158	PASS
441	198	0.01	100	11.9	12930	PASS
442	198	50	100	76.8	83616	PASS
443	442	15	24	19.9	16668	PASS