

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
 Data File : BF127506.D
 Acq On : 24 Mar 2022 16:53
 Operator : CG\JU
 Sample : N2063-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-8-(10-10.5)

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127506.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	476	479	490	rBV	23729	37945	1.26%	0.206%
2	5.475	539	542	568	rBV	2380858	2633322	87.71%	14.282%
3	6.487	710	714	734	rBV	2530833	2756550	91.81%	14.951%
4	6.845	772	775	784	rBV	631877	495893	16.52%	2.690%
5	7.416	868	872	875	rBV	1923801	1786506	59.50%	9.690%
6	8.128	990	993	1004	rBV	759337	643640	21.44%	3.491%
7	9.204	1172	1176	1179	rBV	3478129	3002449	100.00%	16.284%
8	9.886	1288	1292	1304	rVB	839549	743830	24.77%	4.034%
9	10.680	1423	1427	1441	rBV	1944510	1818295	60.56%	9.862%
10	11.374	1542	1545	1554	rBV	849598	728412	24.26%	3.951%
11	12.963	1810	1815	1818	rBV	2815220	2589399	86.24%	14.044%
12	13.804	1953	1958	1961	rBV	34339	45642	1.52%	0.248%
13	13.845	1961	1965	1968	rVV	54312	83282	2.77%	0.452%
14	13.880	1968	1971	1978	rVB	78037	99173	3.30%	0.538%
15	14.021	1992	1995	2004	rVB	505467	490281	16.33%	2.659%
16	15.504	2243	2247	2257	rVB	363519	482884	16.08%	2.619%




Sum of corrected areas: 18437503

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
Data File : BF127506.D
Acq On : 24 Mar 2022 16:53
Operator : CG\JU
Sample : N2063-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-8-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

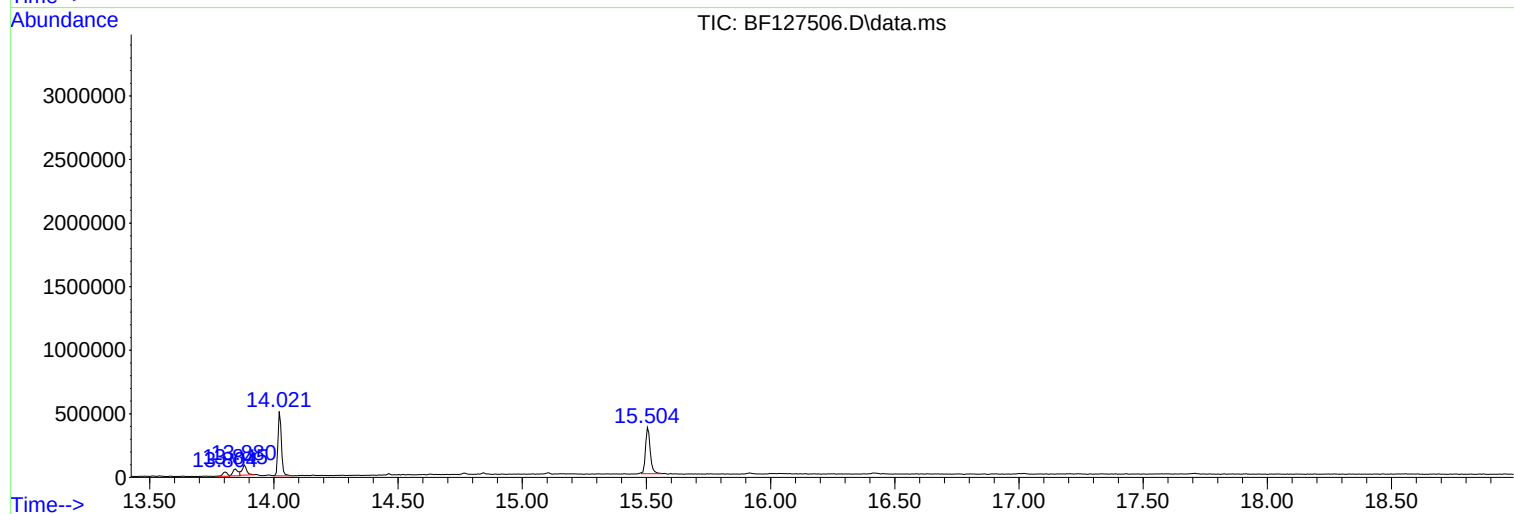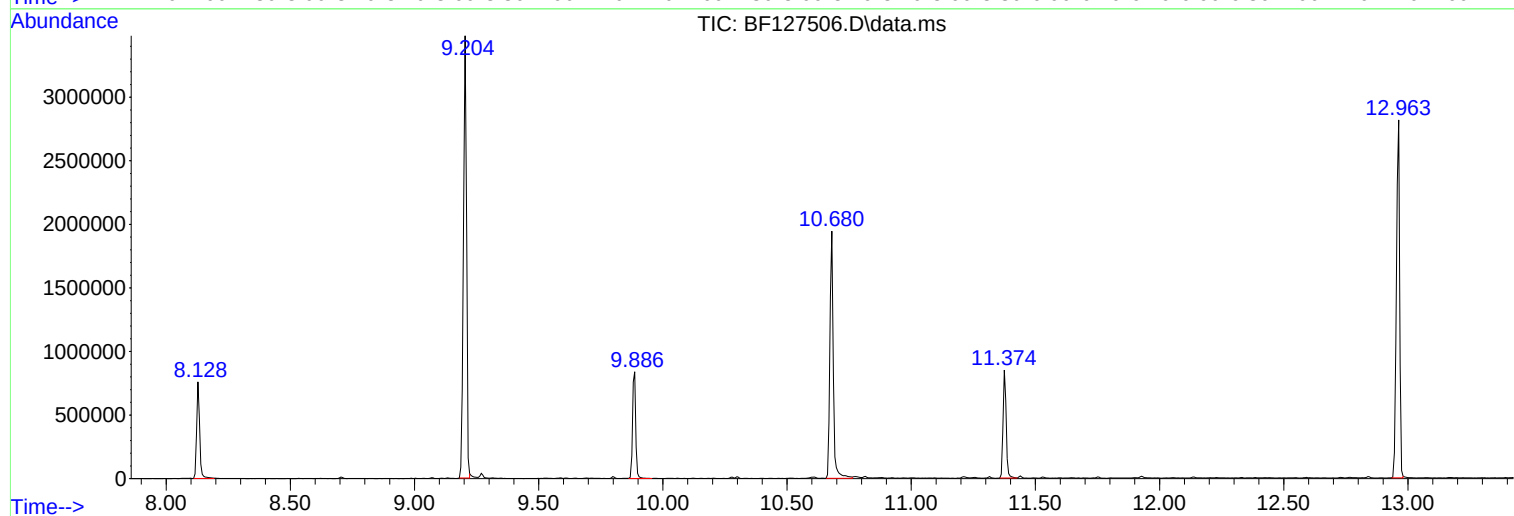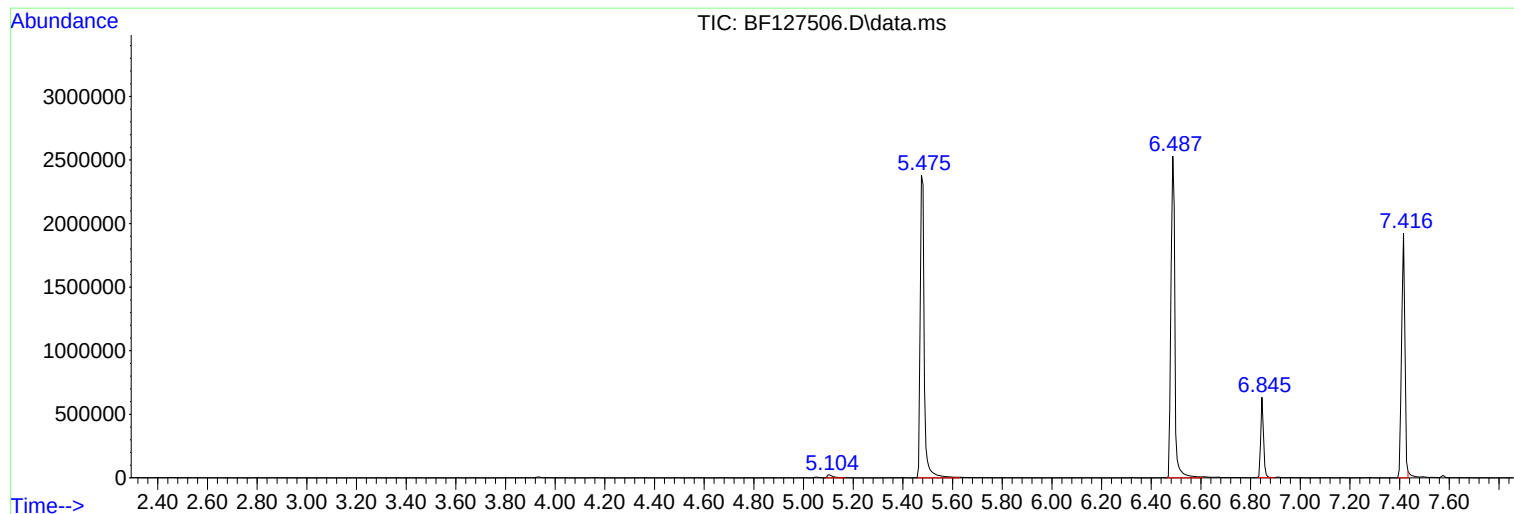

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
Data File : BF127506.D
Acq On : 24 Mar 2022 16:53
Operator : CG\JU
Sample : N2063-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-8-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
Data File : BF127506.D
Acq On : 24 Mar 2022 16:53
Operator : CG\JU
Sample : N2063-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-8-(10-10.5)

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc