


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
 Data File : BF127494.D
 Acq On : 24 Mar 2022 10:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 22 02:16:33 2022

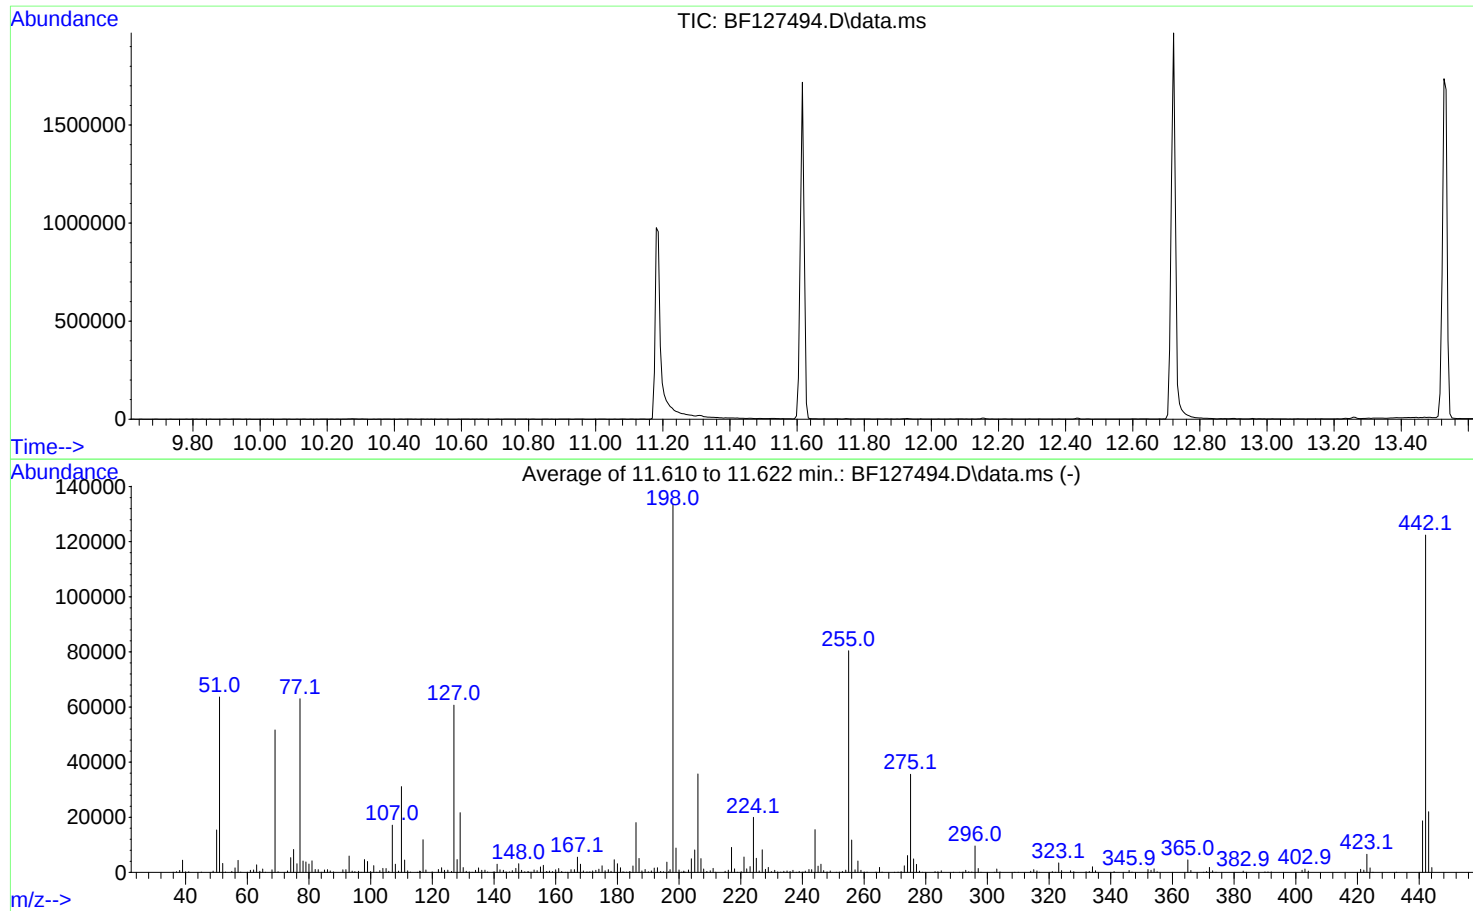




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	63629	PASS
68	69	0.00	2	1.8	917	PASS
69	198	0.00	100	38.7	51664	PASS
70	69	0.00	2	0.5	256	PASS
127	198	10	80	45.5	60696	PASS
197	198	0.00	2	0.8	1006	PASS
198	198	100	100	100.0	133501	PASS
199	198	5	9	6.6	8844	PASS
275	198	10	60	26.7	35616	PASS
365	198	1	100	3.4	4557	PASS
441	198	0.01	100	14.0	18722	PASS
442	442	50	100	100.0	122416	PASS
443	442	15	24	18.0	21999	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
Data File : BF127494.D
Acq On : 24 Mar 2022 10:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 24 15:30:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

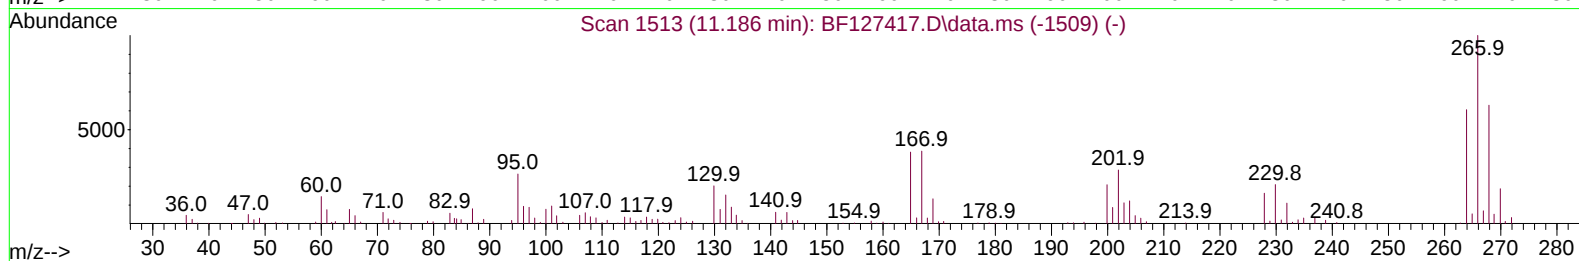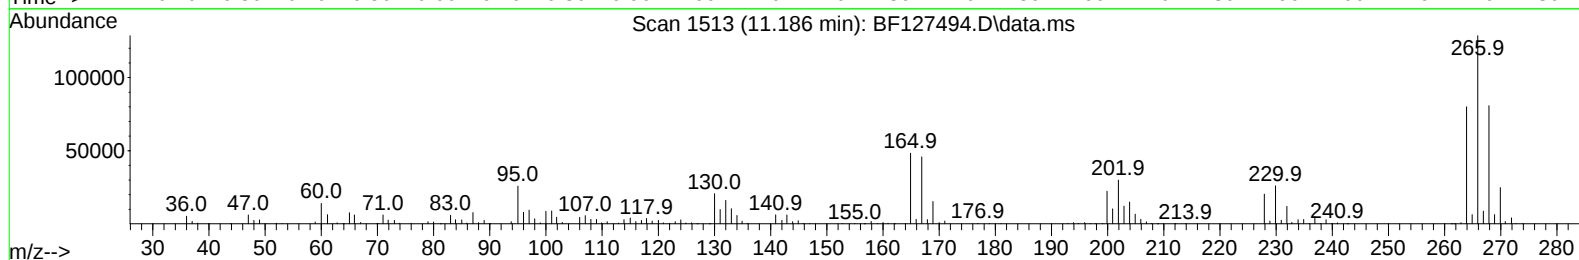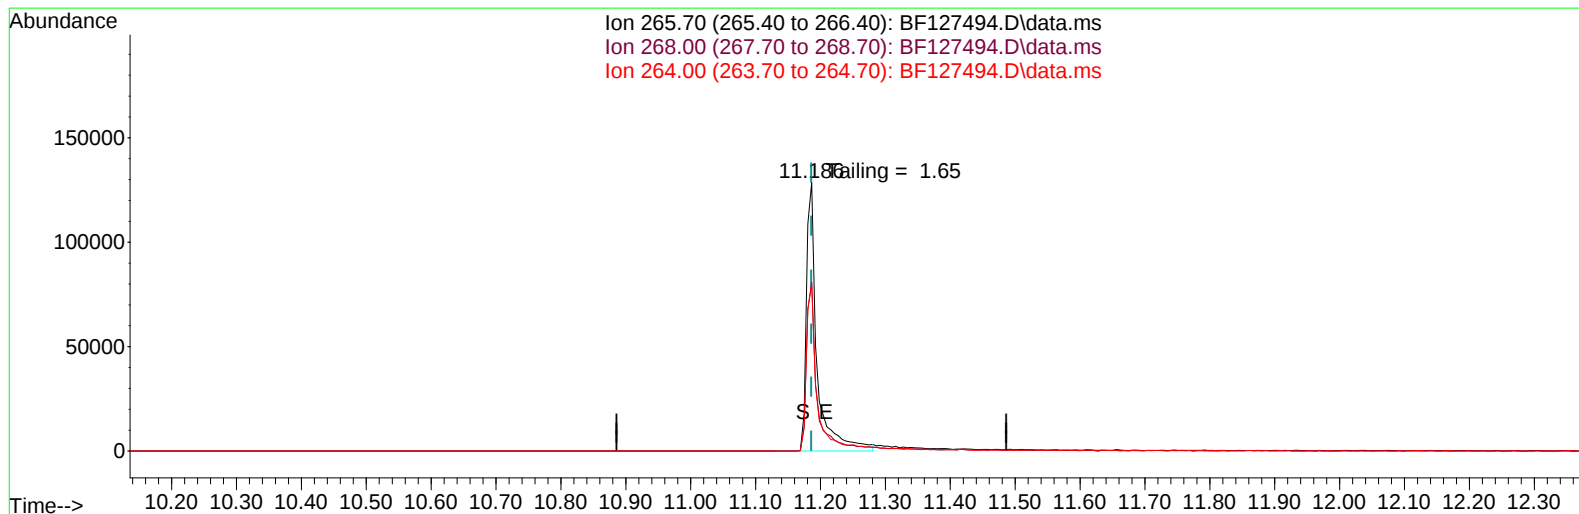

TIC: BF127494.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.000) 54090.30 ng


response 157799

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.87
264.00	60.60	62.24
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032422\
Data File : BF127494.D
Acq On : 24 Mar 2022 10:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 24 15:30:02 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 02:16:33 2022
Response via : Initial Calibration

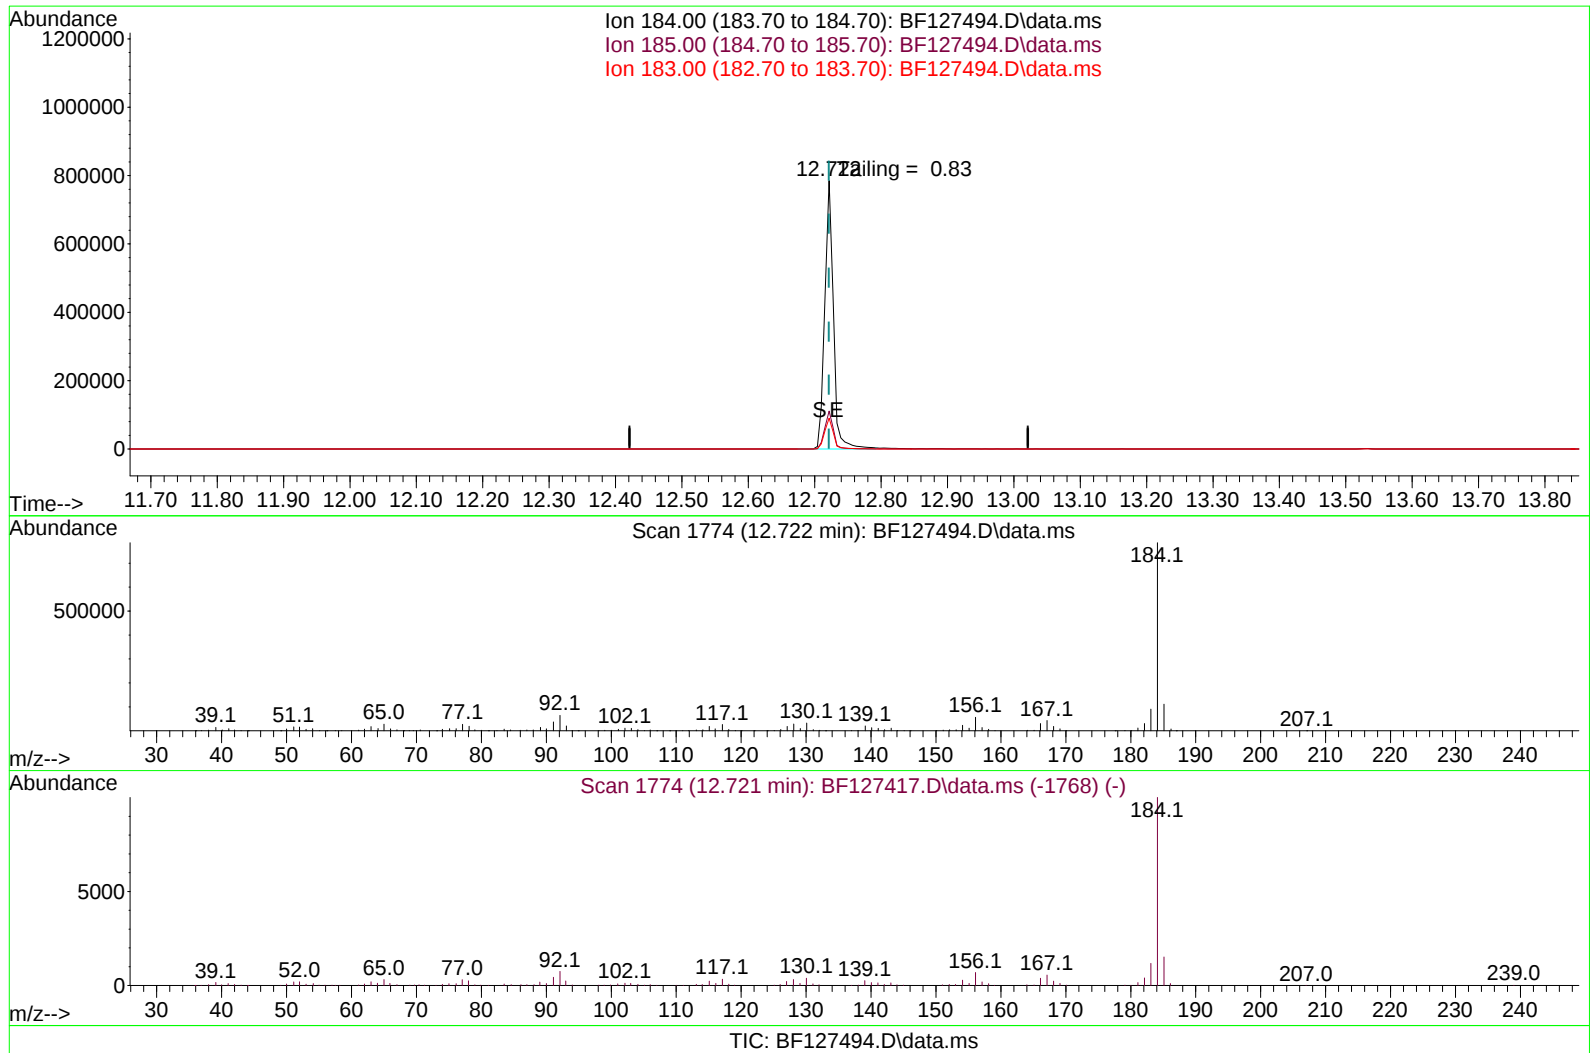

(77) Benzidine

12.722min (+ 0.000) 0.00 ng

response 722623

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.14
183.00	11.70	11.55
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/24/2022	BNA_F	<u>BF127494.D</u>
Compound Name	Response	Retention Time
DDT	337323	13.53
DDD	988	13.23
DDE	872	12.89
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
1860	339183	0.55

Instrument :
BNA_F
ClientSampleId :
DFTPP