


Data Path : T:\svoasrv\HPCHEM1\BNA_F\Data\BF032425\
Data File : BF142044.D
Acq On : 24 Mar 2025 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : T:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

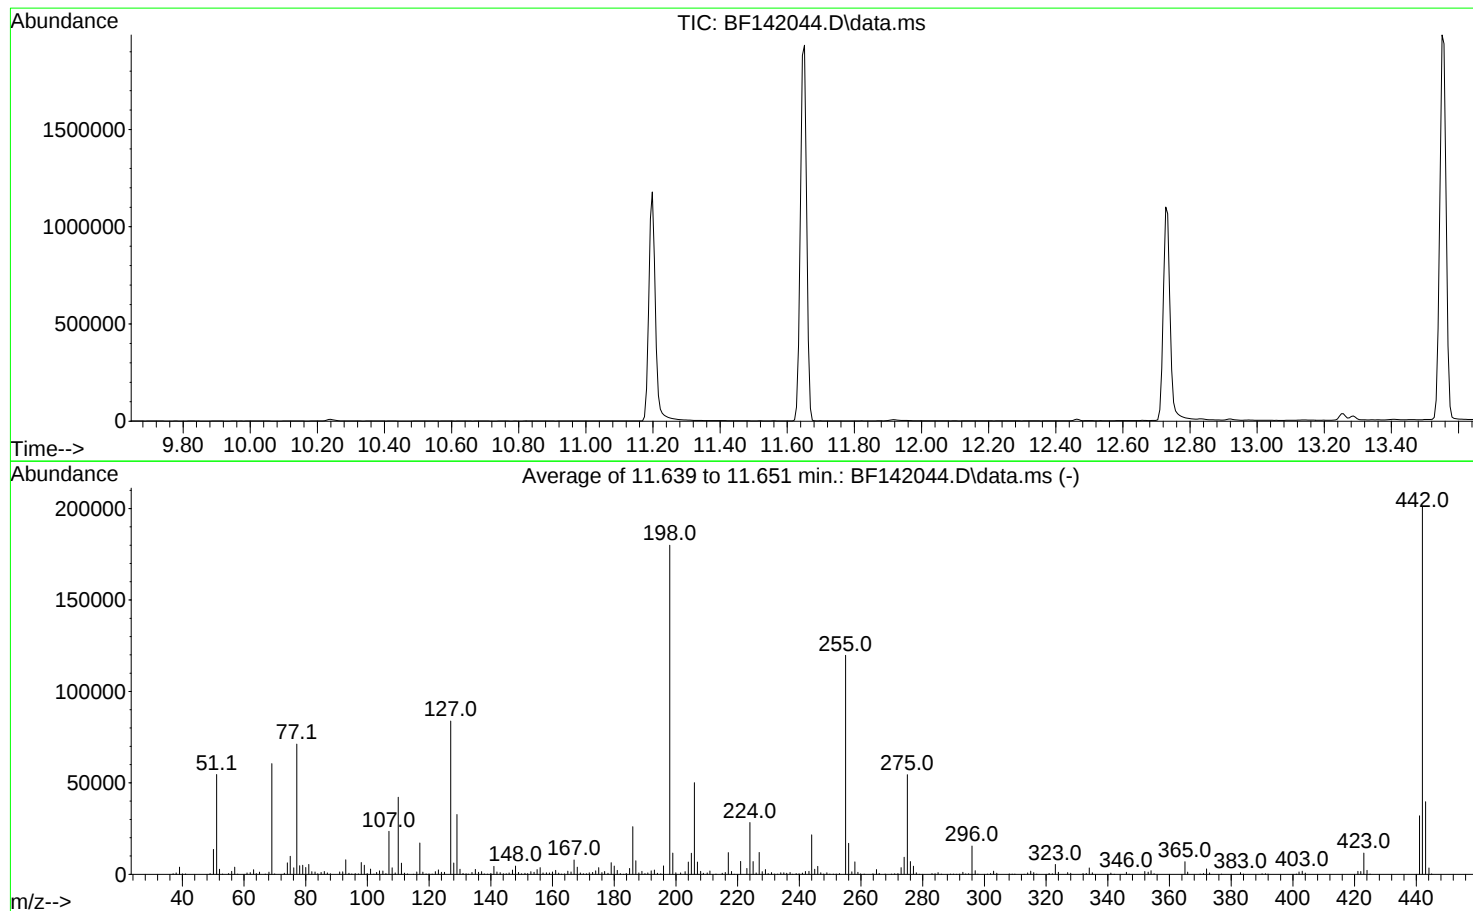




AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.3	54595	PASS
68	69	0.00	2	1.9	1146	PASS
69	198	0.00	100	33.6	60485	PASS
70	69	0.00	2	0.4	267	PASS
127	198	10	80	46.6	83835	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	179944	PASS
199	198	5	9	6.5	11637	PASS
275	198	10	60	30.3	54496	PASS
365	198	1	100	3.8	6912	PASS
441	198	0.01	100	17.8	32003	PASS
442	442	50	100	100.0	201192	PASS
443	442	15	24	19.7	39667	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032425\
Data File : BF142044.D
Acq On : 24 Mar 2025 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 24 11:23:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

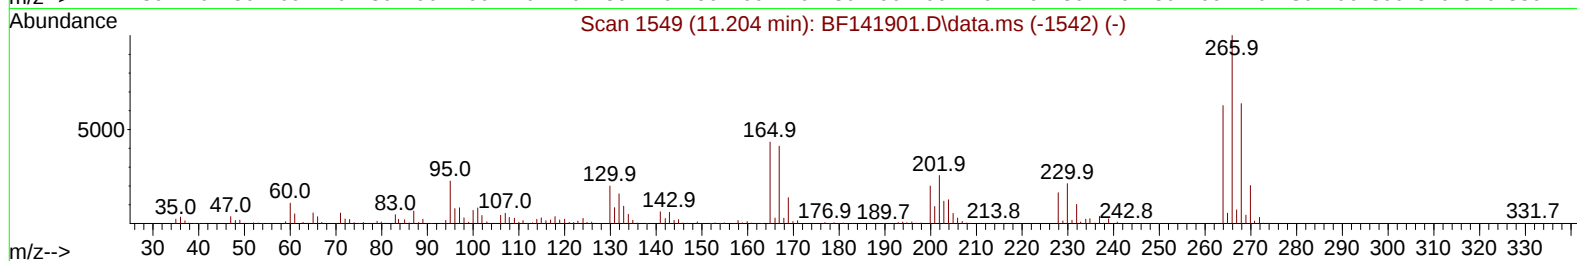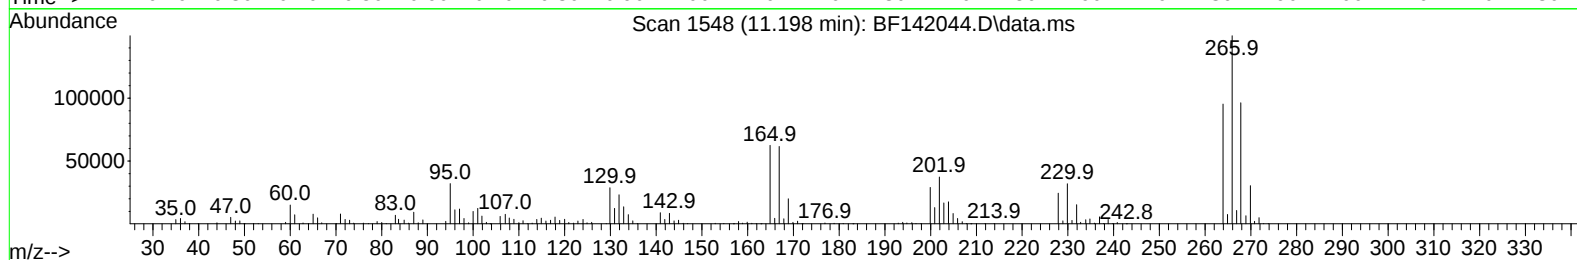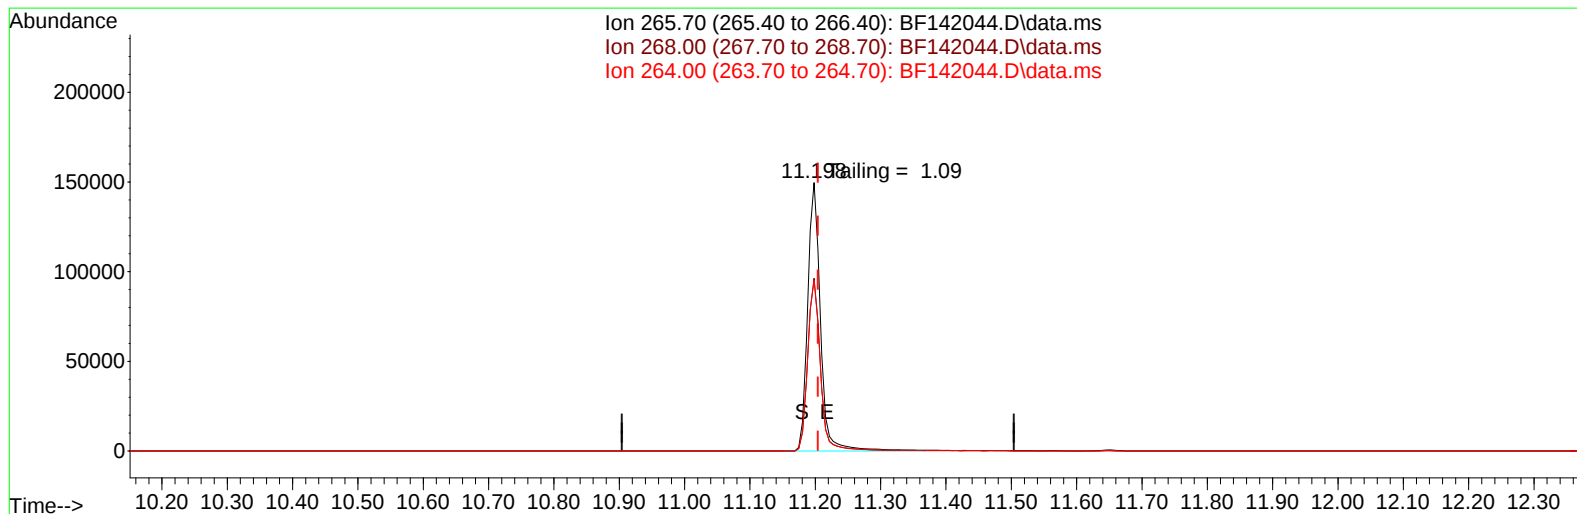

TIC: BF142044.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 409215.86 ng




response 204900

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.35
264.00	62.70	63.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032425\
Data File : BF142044.D
Acq On : 24 Mar 2025 09:43
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 24 11:23:26 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

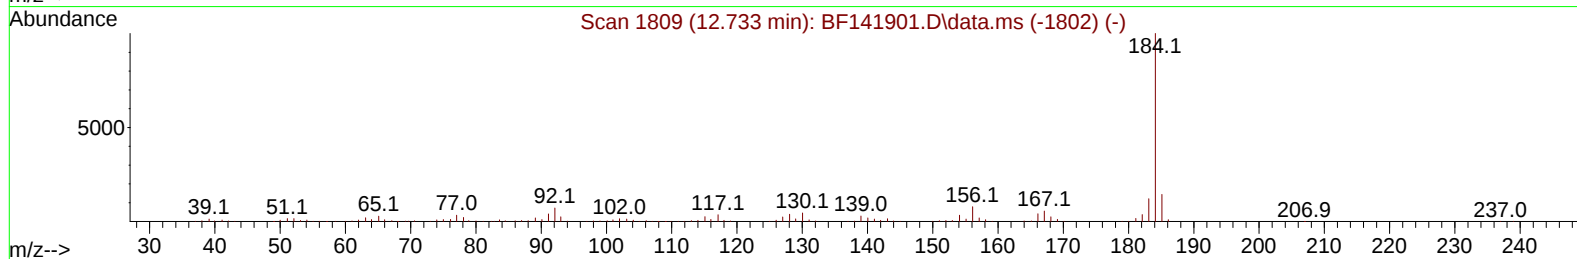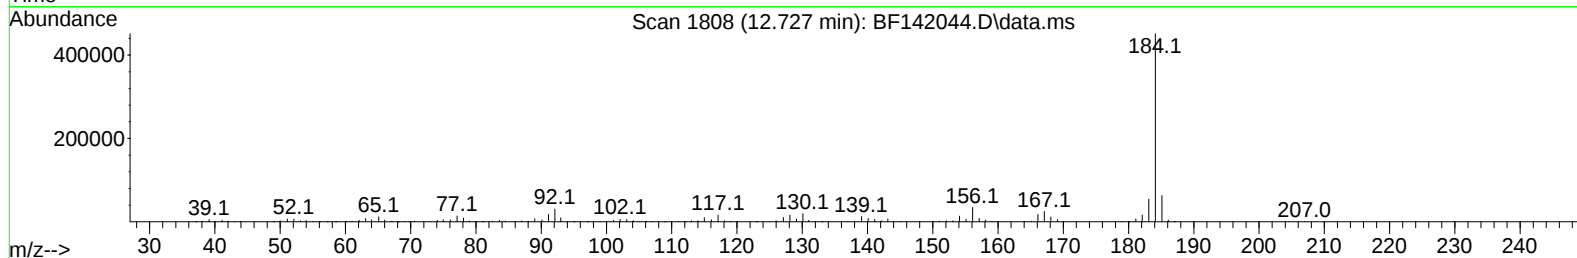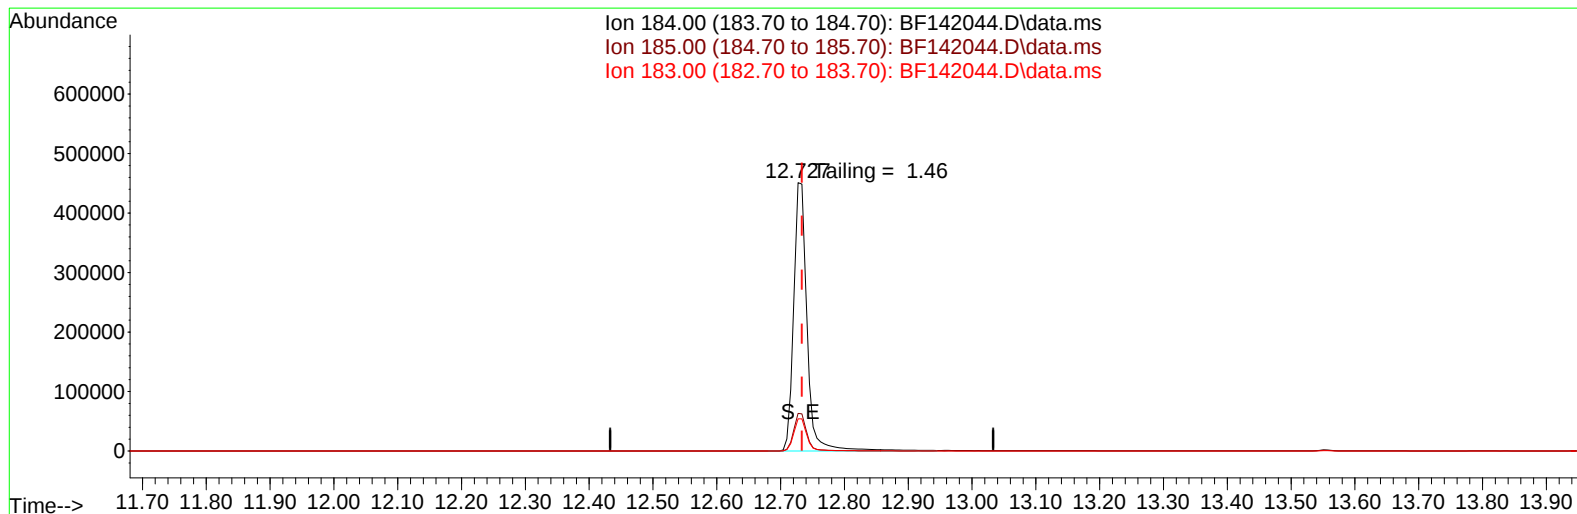

TIC: BF142044.D\data.ms

(77) Benzidine

12.727min (-0.006) 0.00 ng

response 662362

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.01
183.00	12.10	12.02
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/24/2025	BNA_F	<u>BF142044.D</u>
Compound Name	Response	Retention Time
DDT	529950	13.557
DDD	16020	13.257
DDE	2069	12.922
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18089	548039	3.30

Instrument :
BNA_F
ClientSampleId :
DFTPP