

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032515\
 Data File : BF077974.D
 Acq On : 26 Mar 2015 3:06
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 26 03:05:04 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 26 00:45:24 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	0.00	152	0	0.00	ng	-7.09
21) Naphthalene-d8	0.00	136	0	0.00	ng	-8.67
38) Acenaphthene-d10	0.00	164	0	0.00	ng	-10.84
63) Phenanthrene-d10	0.00	188	0	0.00	ng	-12.68
75) Chrysene-d12	0.00	240	0	0.00	ng	-15.97
86) Perylene-d12	0.00	264	0	0.00	ng	-17.75
System Monitoring Compounds						
5) 2-Fluorophenol	0.00	112	0	0.00	ng	
7) Phenol-d6	0.00	99	0	0.00	ng	
23) Nitrobenzene-d5	0.00	82	0	0.00	ng	
41) 2,4,6-Tribromophenol	0.00	330	0	0.00	ng	
44) 2-Fluorobiphenyl	0.00	172	0	0.00	ng	
78) Terphenyl-d14	0.00	244	0	0.00	ng	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032515\
Data File : BF077974.D
Acq On : 26 Mar 2015 3:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 26 03:05:04 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 00:45:24 2015
Response via : Initial Calibration

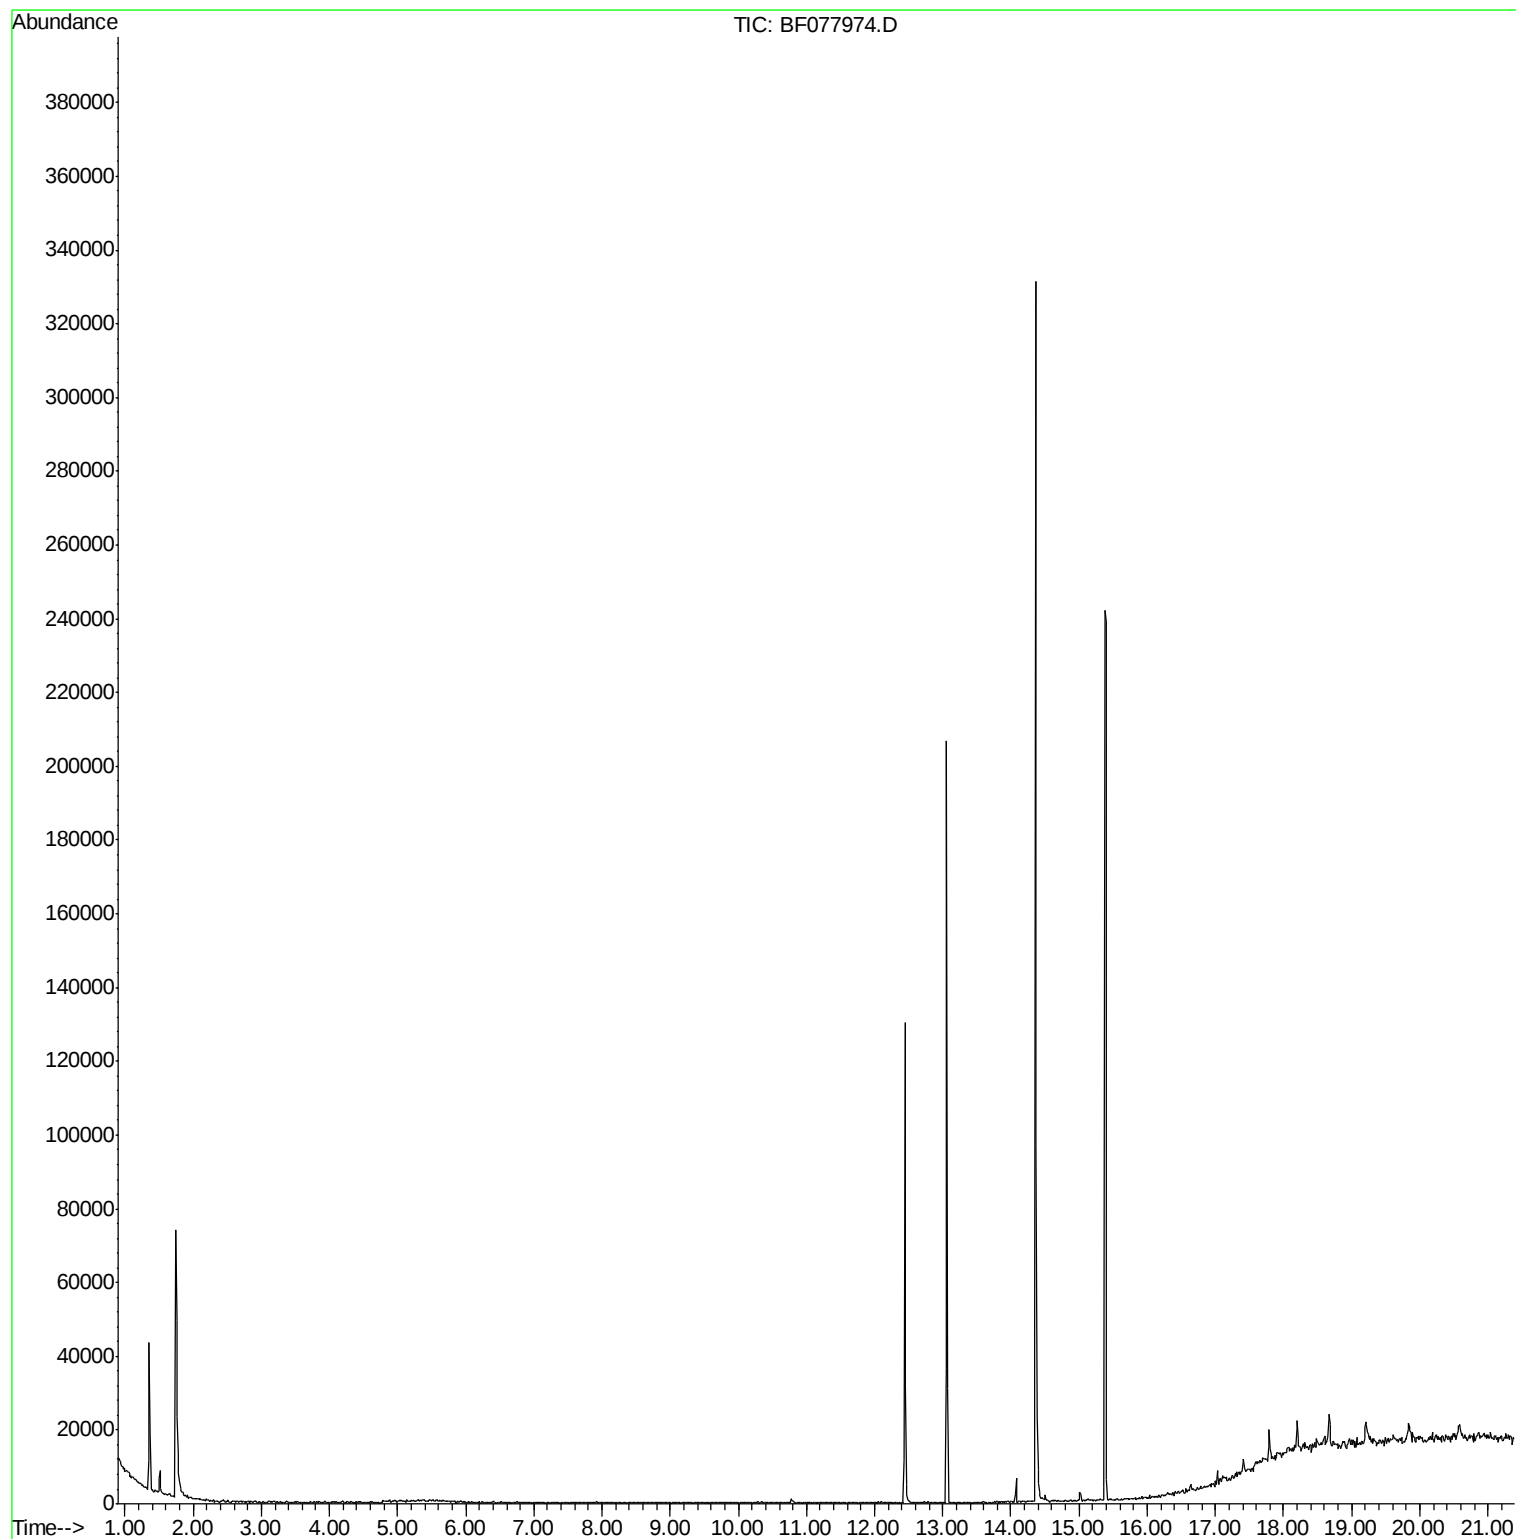

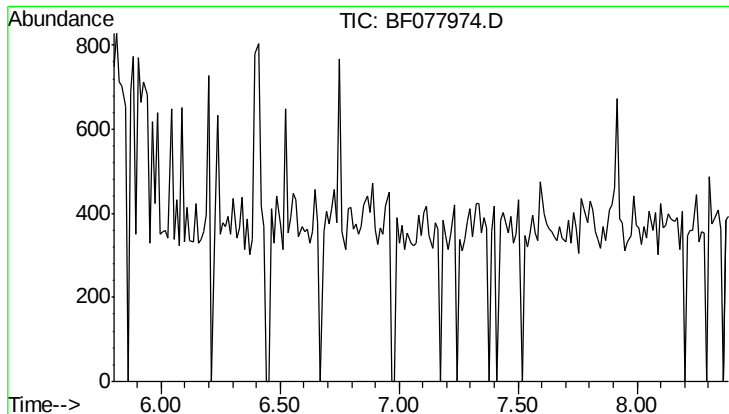

#1

1,4-Dichlorobenzene-d4

Concen: 0.00 ng

Expected RT: 7.09 min

Lab File: BF077974.D

Acq: 26 Mar 2015 3:06

Instrument :

BNA_F

ClientSampleId :

DFTPP



Tgt Ion: 152

Sig Exp Ratio

152 100

150 149.4

115 53.7

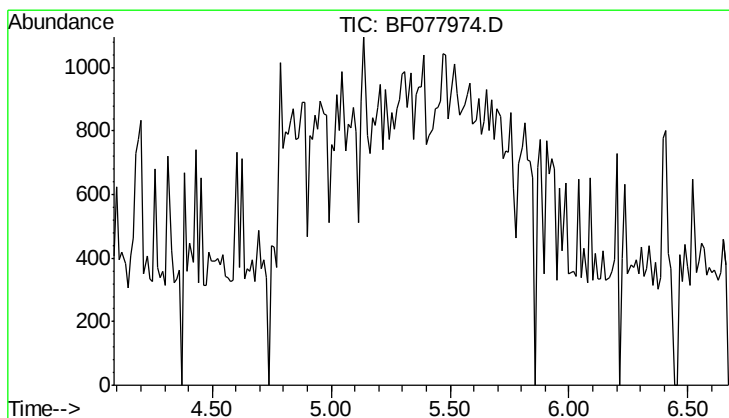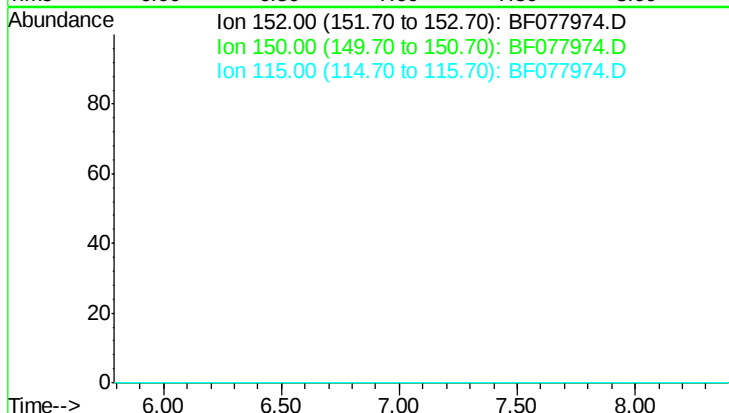

#5

2-Fluorophenol

Concen: 0.00 ng

Expected RT: 5.38 min

Lab File: BF077974.D

Acq: 26 Mar 2015 3:06


Tgt Ion: 112


Sig Exp Ratio

112 100

64 48.2

63 24.1

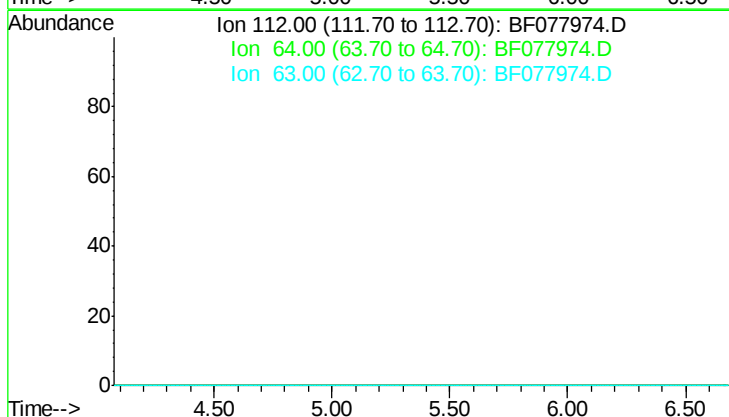

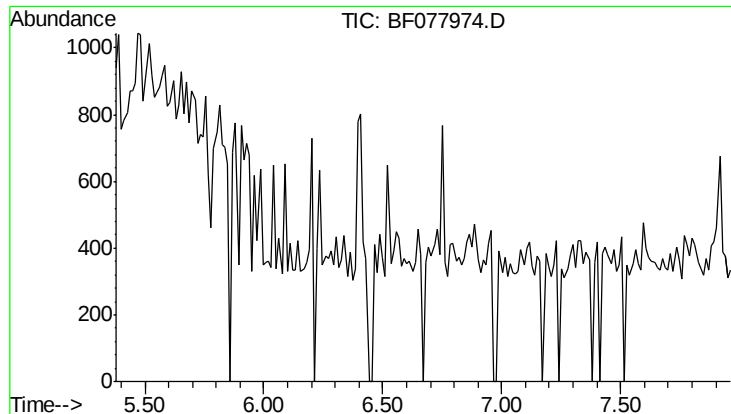

#7

Phenol-d6

Concen: 0.00 ng

Expected RT: 6.67 min

Lab File: BF077974.D

Acq: 26 Mar 2015 3:06

Instrument :

BNA_F

ClientSampleId :

DFTPP



Tgt Ion: 99

Sig Exp Ratio

99 100

42 13.7

71 29.3

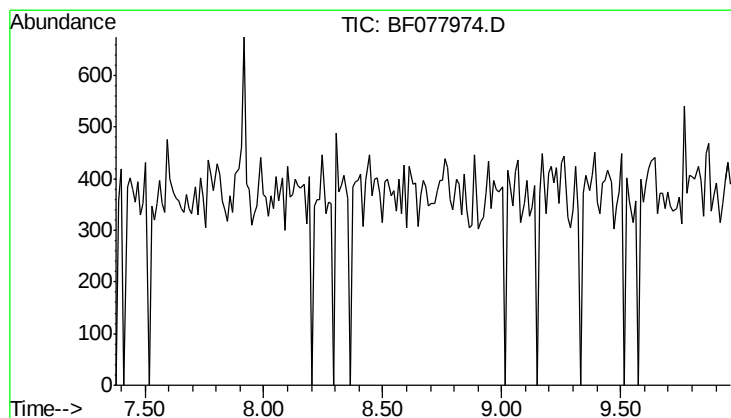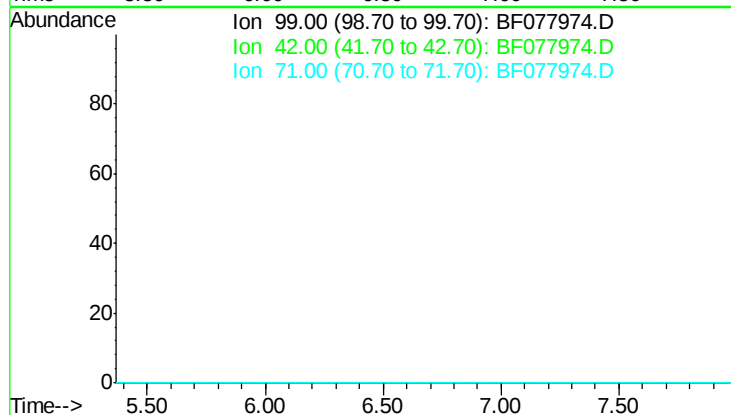

#21

Naphthalene-d8

Concen: 0.00 ng

Expected RT: 8.67 min

Lab File: BF077974.D

Acq: 26 Mar 2015 3:06

Tgt Ion: 136


Sig Exp Ratio


136 100

137 10.9

54 5.7

68 4.6


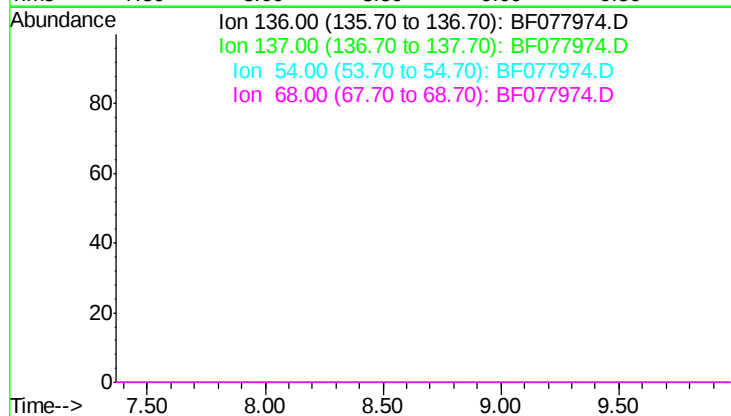


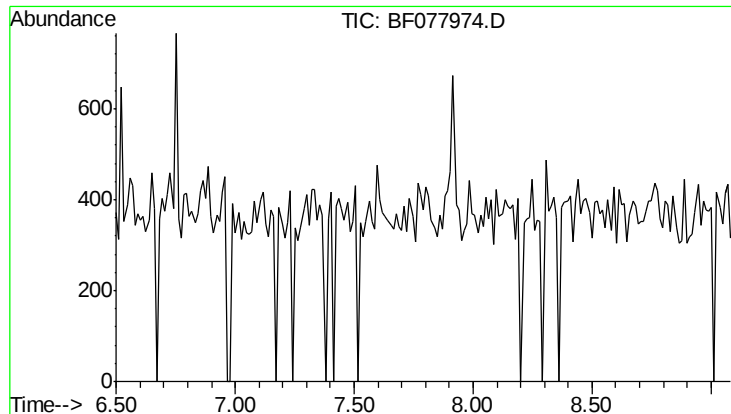

#23
 Nitrobenzene-d5
 Concen: 0.00 ng
 Expected RT: 7.79 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06


Instrument :
 BNA_F
 ClientSampleId :
 DFTPP


Tgt Ion	Exp Ratio
82	100
128	41.0
54	50.7

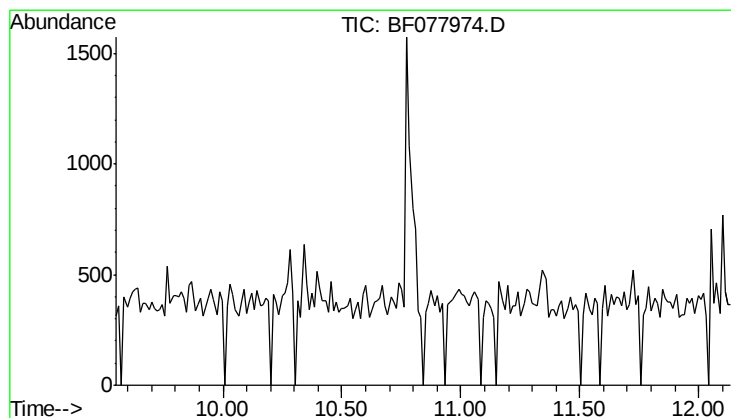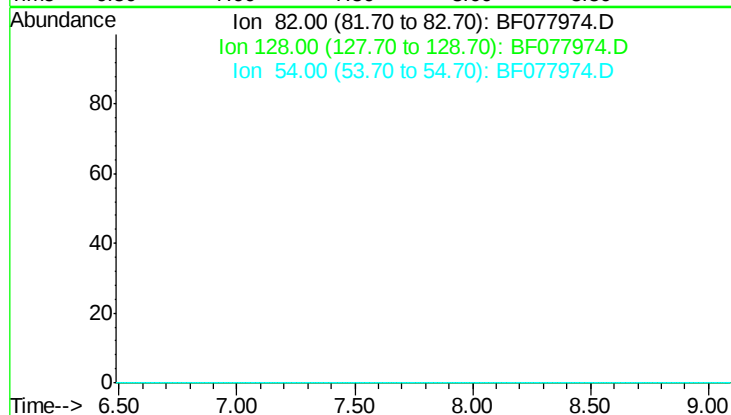

#38
 Acenaphthene-d10
 Concen: 0.00 ng
 Expected RT: 10.84 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06

Tgt Ion	Exp Ratio
164	100
162	103.0
160	44.7


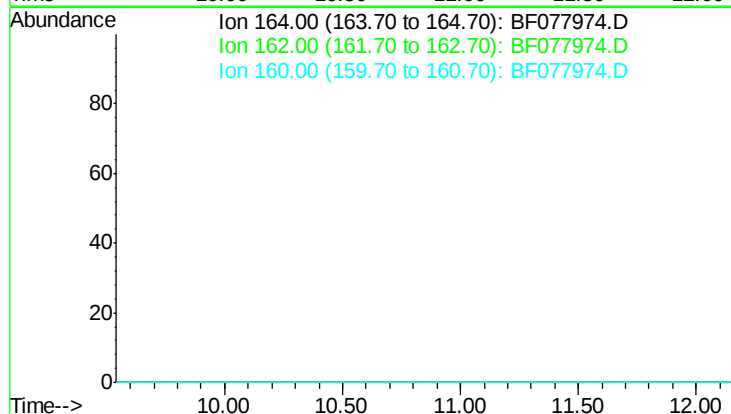


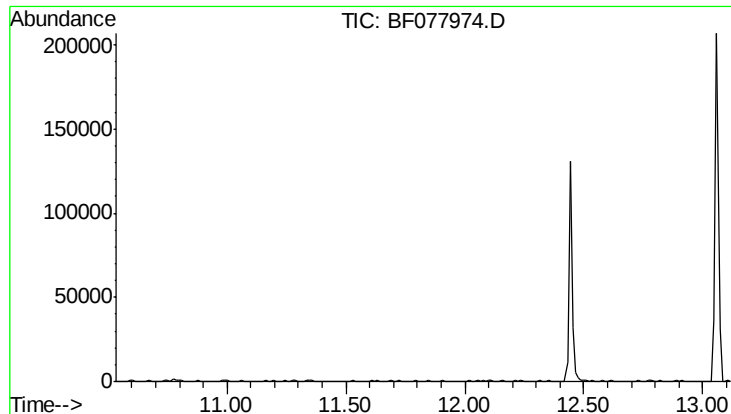

#41
 2,4,6-Tribromophenol
 Concen: 0.00 ng
 Expected RT: 11.82 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06


Instrument :
 BNA_F
 ClientSampleId :
 DFTPP


Tgt Ion: 330
 Sig Exp Ratio
 330 100
 332 0.0
 141 0.0

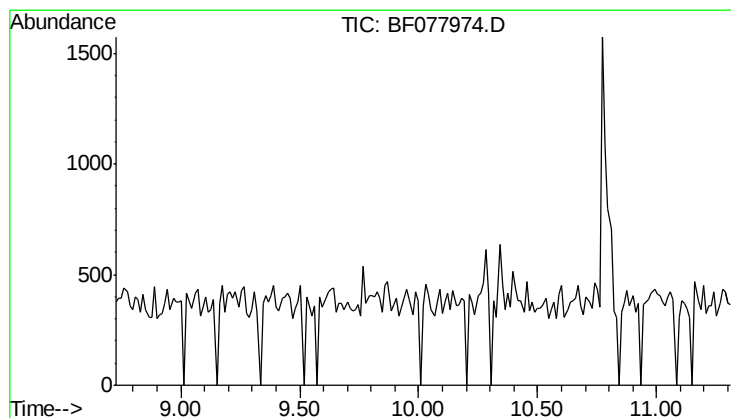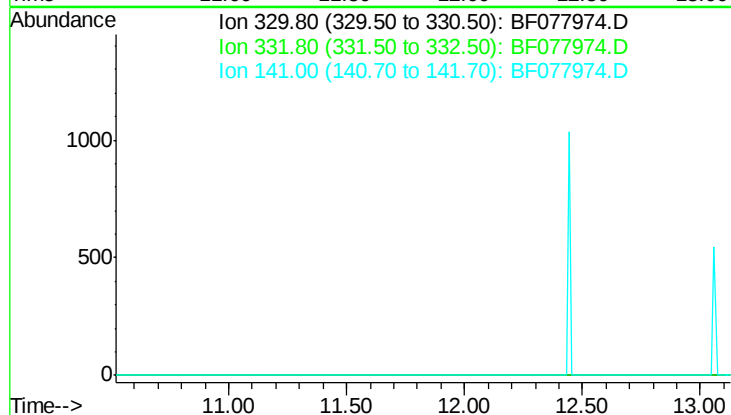

#44
 2-Fluorobiphenyl
 Concen: 0.00 ng
 Expected RT: 10.02 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06

Tgt Ion: 172
 Sig Exp Ratio
 172 100
 171 35.6
 170 23.5


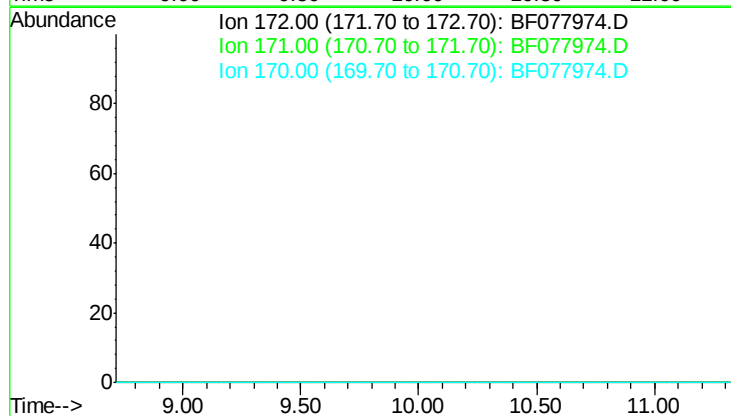


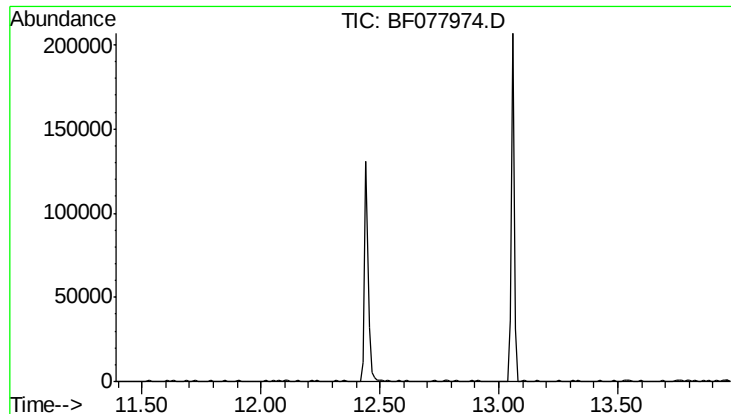

#63
 Phenanthrene-d10
 Concen: 0.00 ng
 Expected RT: 12.68 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06


Instrument :
 BNA_F
 ClientSampleId :
 DFTPP


Tgt Ion: 188
 Sig Exp Ratio
 188 100
 94 10.9
 80 11.6

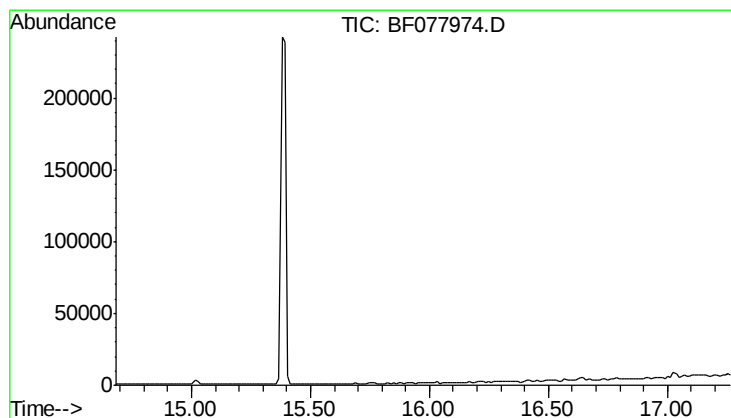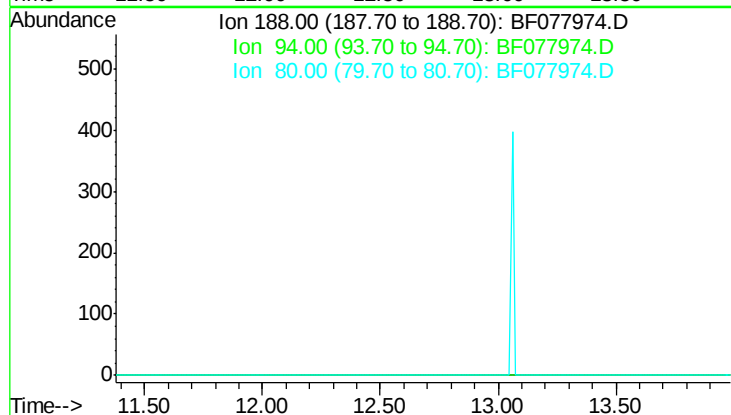

#75
 Chrysene-d12
 Concen: 0.00 ng
 Expected RT: 15.97 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06

Tgt Ion: 240
 Sig Exp Ratio
 240 100
 120 10.2
 236 25.0


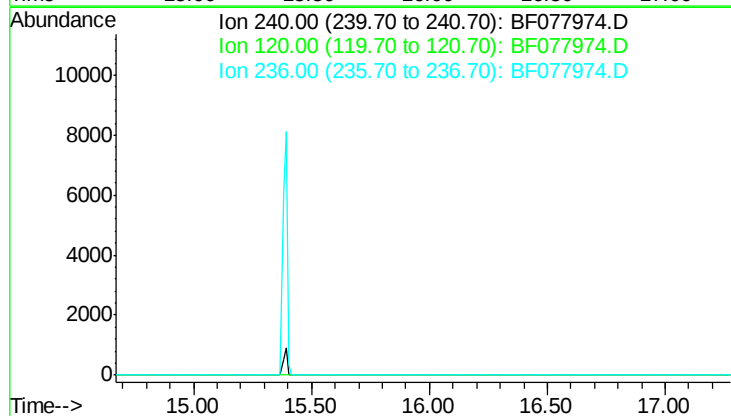


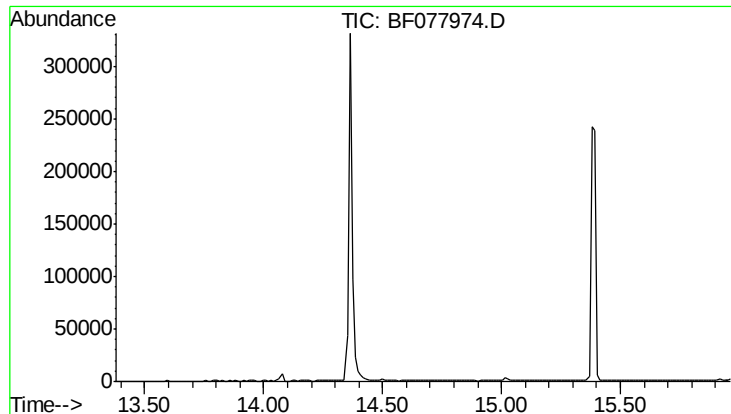

#78
 Terphenyl-d14
 Concen: 0.00 ng
 Expected RT: 14.67 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Tgt Ion: 244
 Sig Exp Ratio
 244 100
 212 6.1
 122 7.8

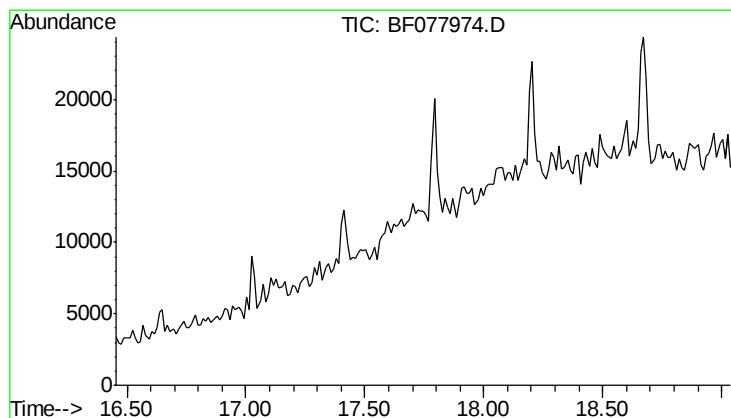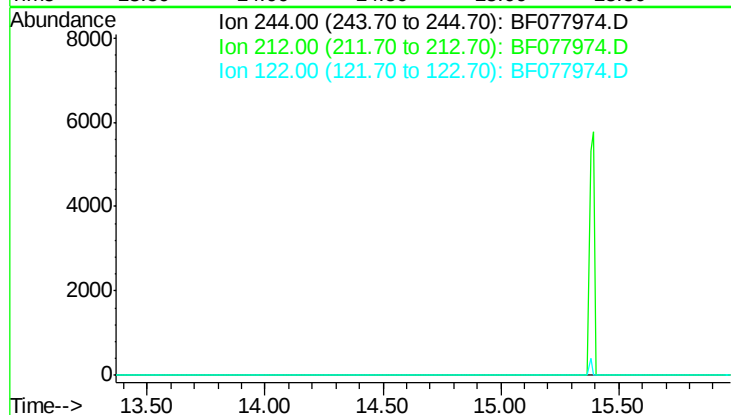

#86
 Perylene-d12
 Concen: 0.00 ng
 Expected RT: 17.75 min
 Lab File: BF077974.D
 Acq: 26 Mar 2015 3:06

Tgt Ion: 264
 Sig Exp Ratio
 264 100
 260 23.2
 265 21.6

