
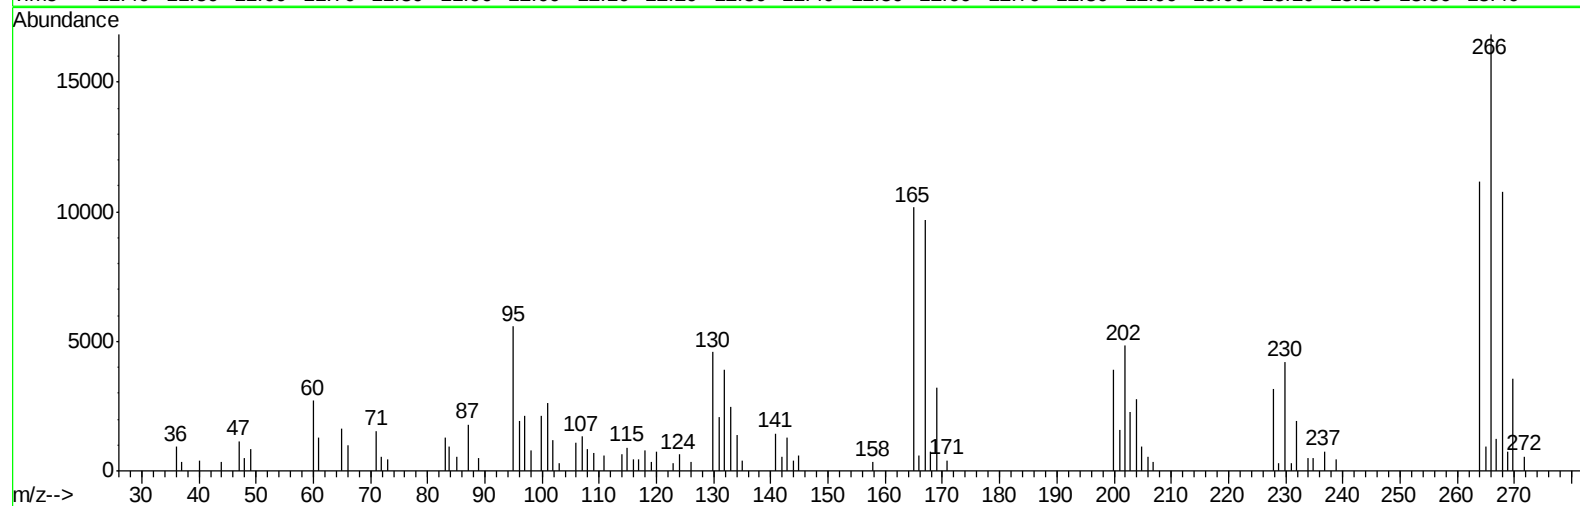


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032515\
Data File : BF077952.D
Acq On : 25 Mar 2015 15:14
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:12:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 00:45:24 2015
Response via : Initial Calibration

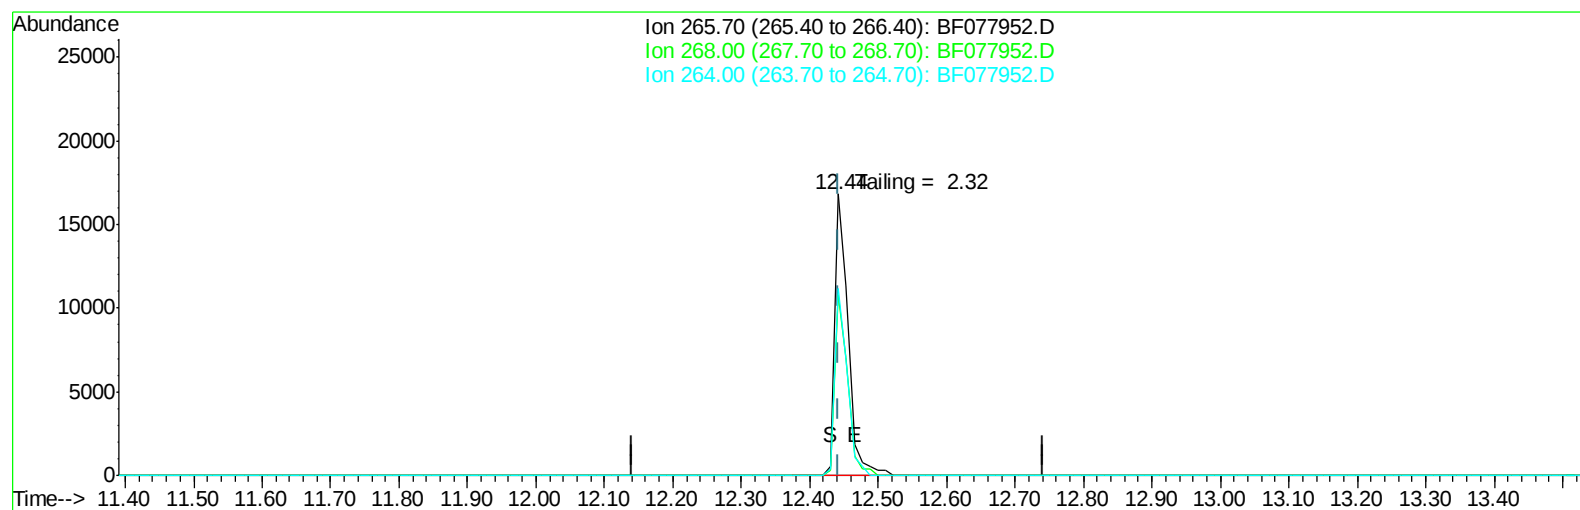

TIC: BF077952.D

(69) Pentachlorophenol (C)



12.442min (+0.000) 0.00ng

response 22264

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.97
264.00	61.20	66.37
0.00	0.00	0.00

```
Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032515\  
Data File : BF077952.D  
Acq On    : 25 Mar 2015   15:14  
Operator  : TP/IZ  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1      Sample Multiplier: 1
```

Quant Time: Mar 26 08:12:32 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 00:45:24 2015
Response via : Initial Calibration

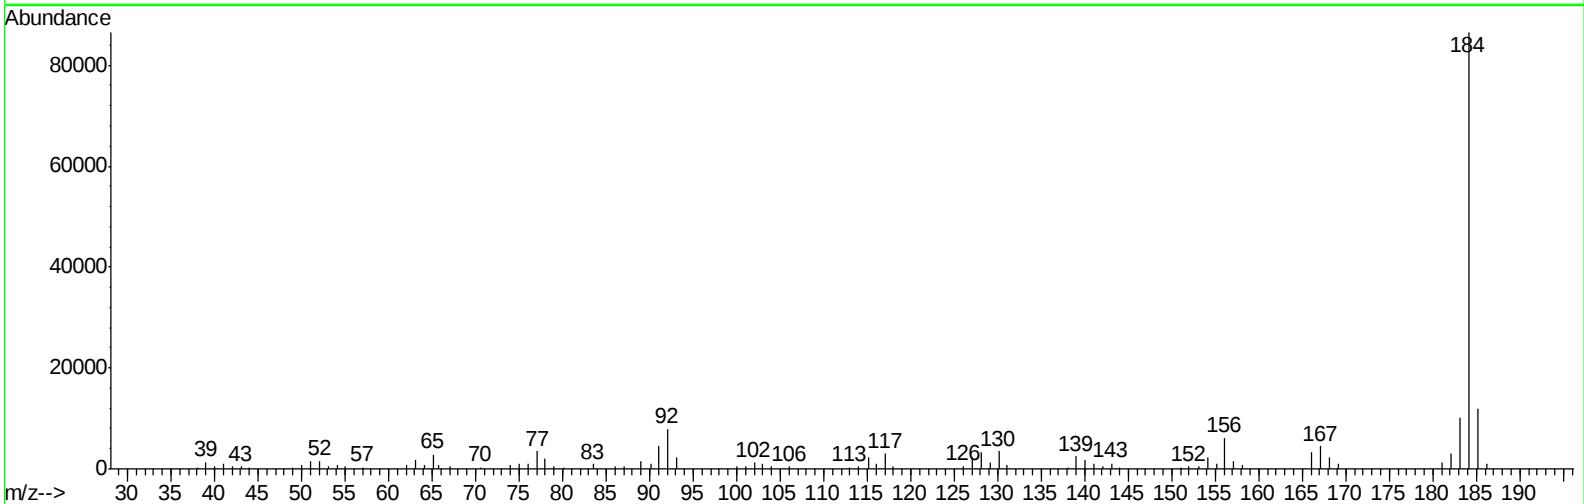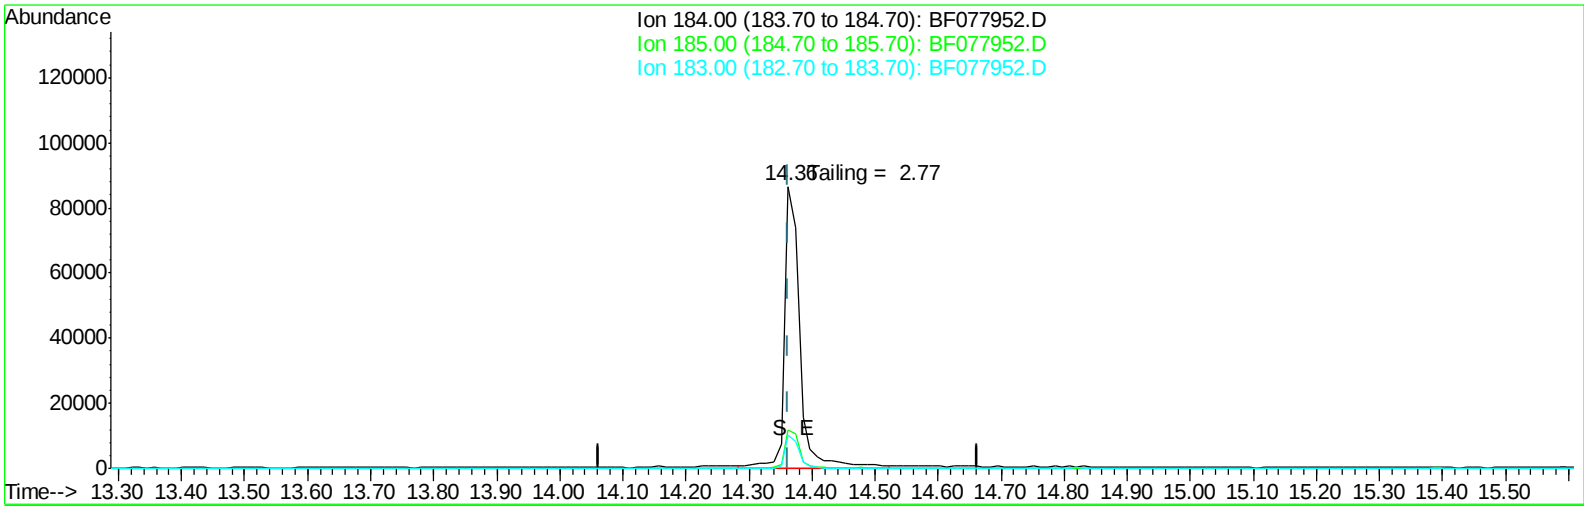

TIC: BF077952.D

(76) Benzidine

14.362min (+0.000) 0.00ng

response 140750

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.70
183.00	11.10	11.85
0.00	0.00	0.00