
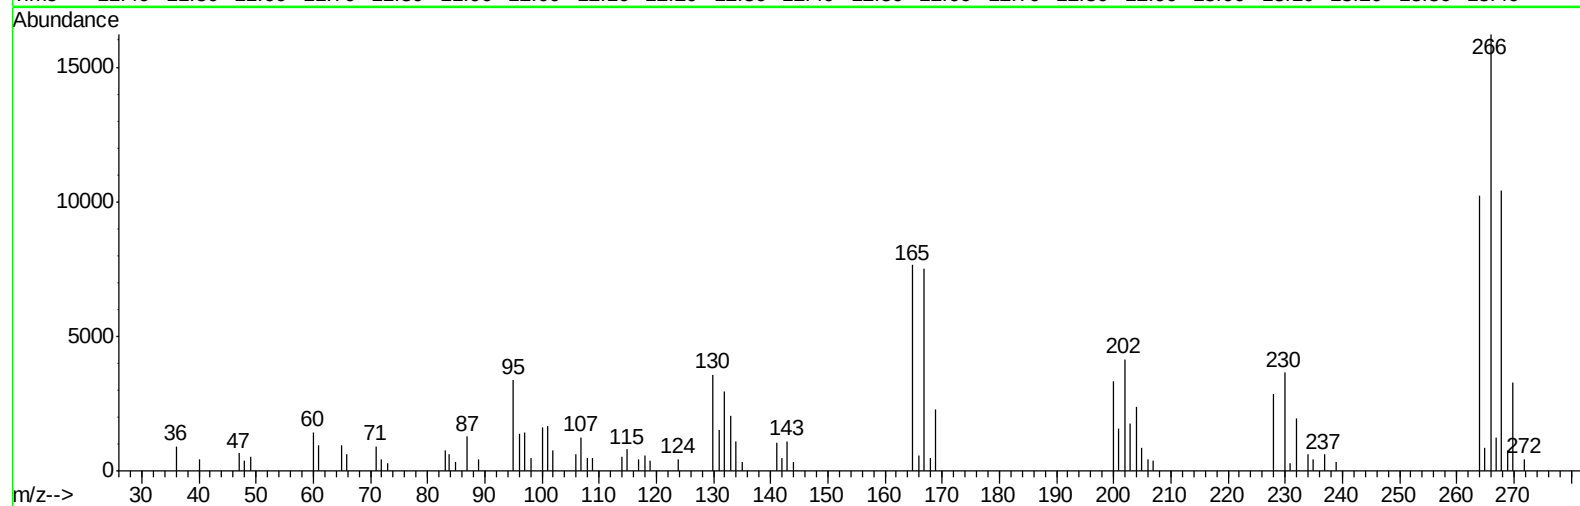


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032515\
Data File : BF077974.D
Acq On : 26 Mar 2015 3:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:15:36 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 00:45:24 2015
Response via : Initial Calibration

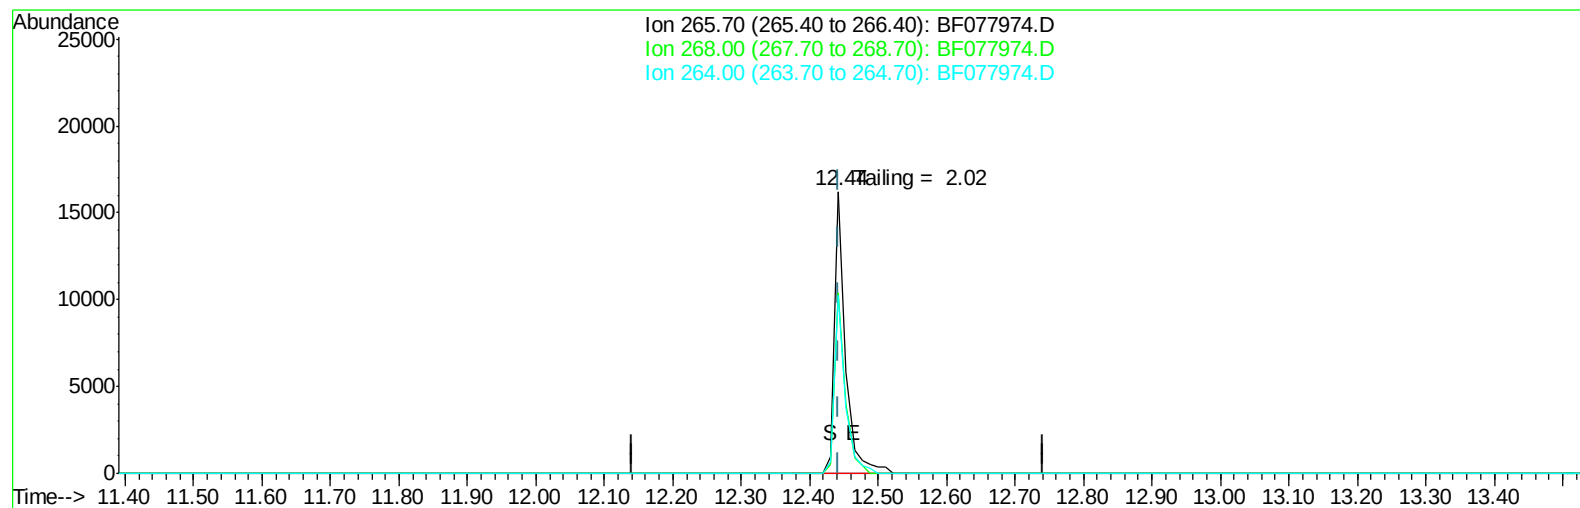

TIC: BF077974.D

(69) Pentachlorophenol (C)



12.442min (+0.000) 0.00ng

response 17992

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	64.23
264.00	61.20	63.16
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032515\
Data File : BF077974.D
Acq On : 26 Mar 2015 3:06
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 08:15:36 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 26 00:45:24 2015
Response via : Initial Calibration

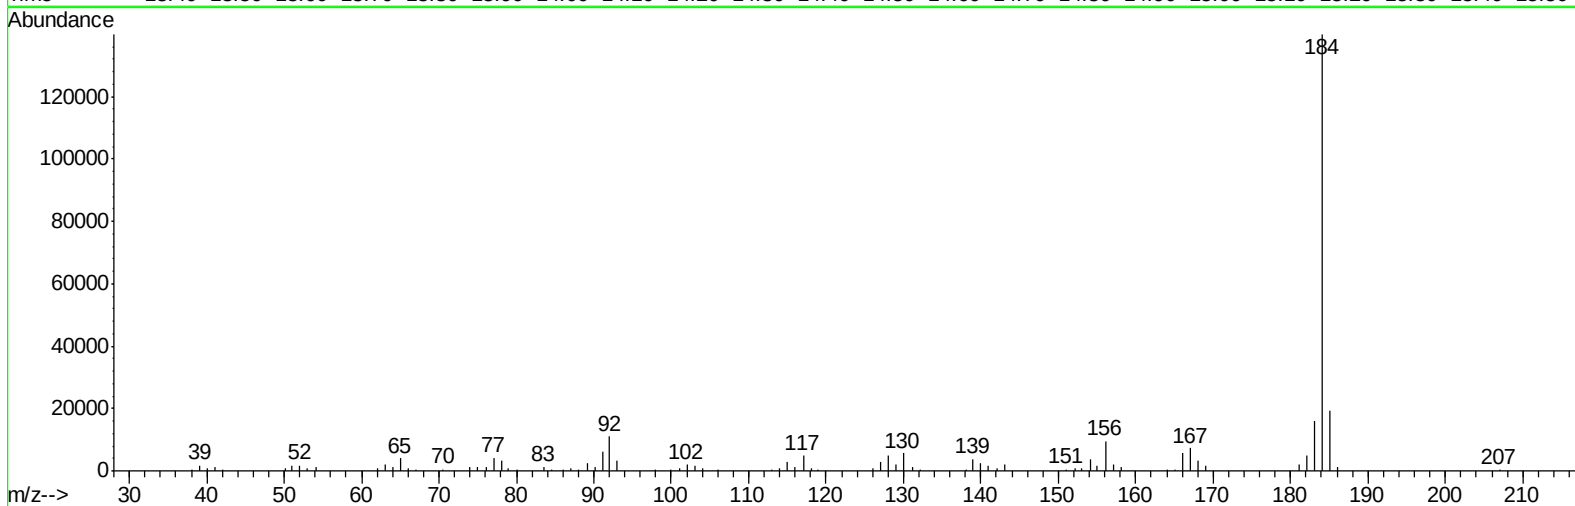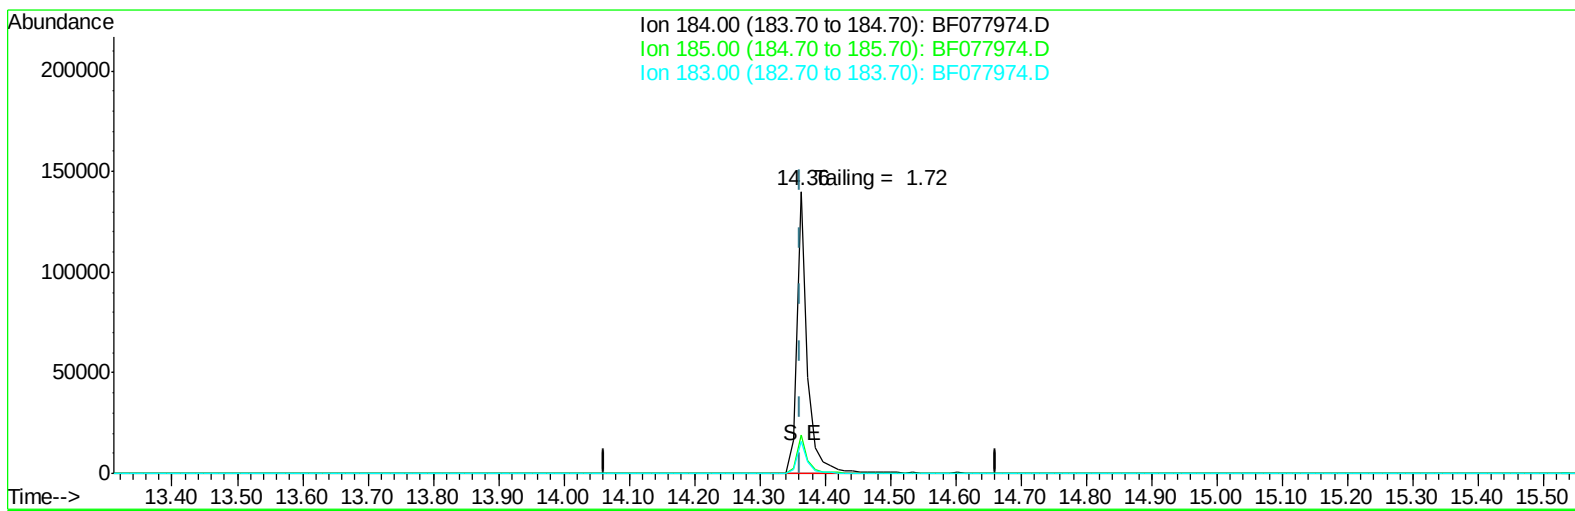

TIC: BF077974.D

(76) Benzidine

14.362min (+0.000) 0.00ng

response 160922

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.76
183.00	11.10	11.52
0.00	0.00	0.00