


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032516\
 Data File : BF085785.D
 Acq On : 26 Mar 2016 2:28
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 28 15:50:38 2016

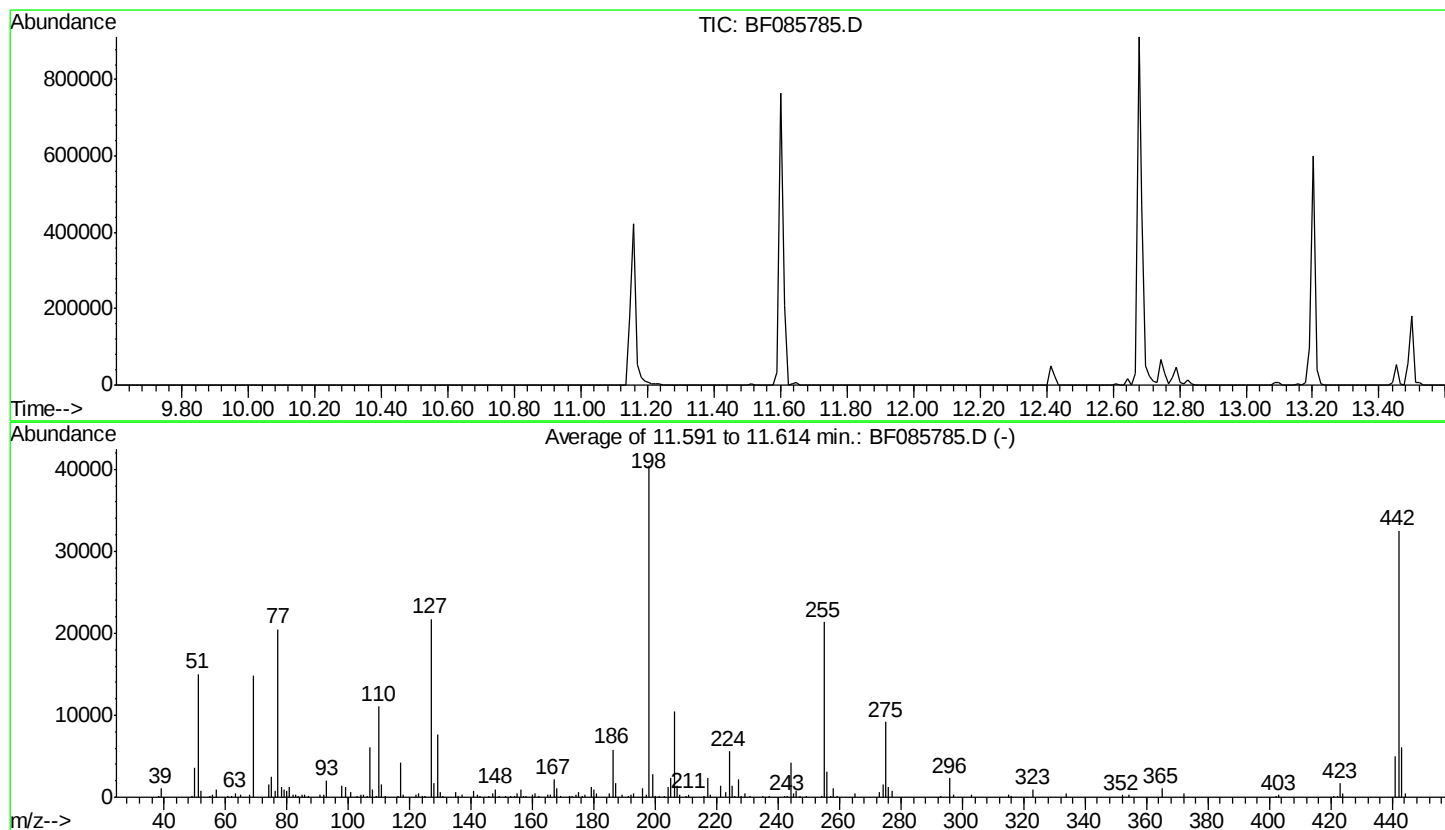

AutoFind: Scans 814, 815, 816; Background Corrected with Scan 811

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	15043	PASS
68	69	0.00	2	1.6	242	PASS
69	198	0.00	100	36.7	14845	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	21761	PASS
197	198	0.00	2	0.7	268	PASS
198	198	100	100	100.0	40433	PASS
199	198	5	9	7.0	2829	PASS
275	198	10	60	22.7	9173	PASS
365	198	1	100	2.6	1060	PASS
441	442	0.01	24	15.5	5032	PASS
442	198	50	100	80.4	32488	PASS
443	442	15	24	18.6	6057	PASS