
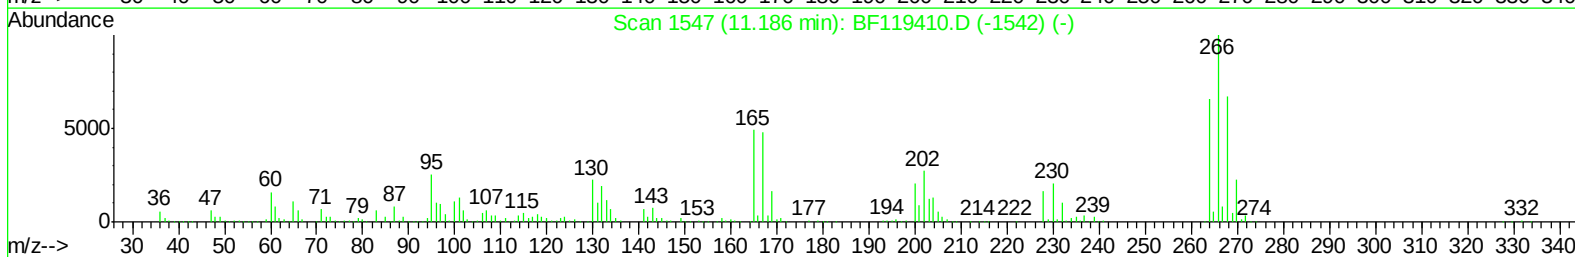
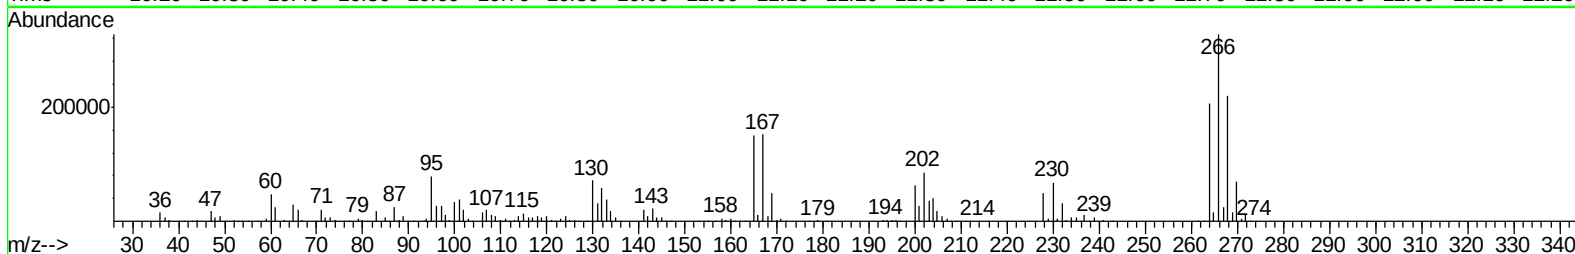


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032520\
 Data File : BF119499.D
 Acq On : 25 Mar 2020 11:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 01:49:47 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 18 15:11:18 2020
 Response via : Initial Calibration

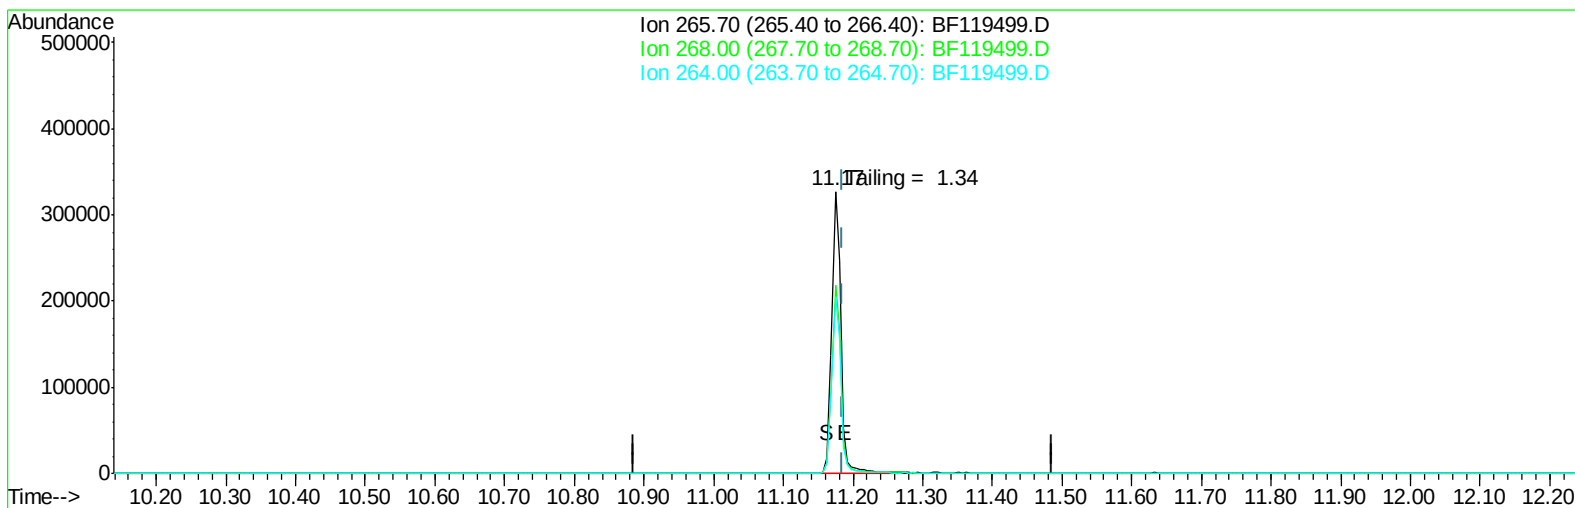

TIC: BF119499.D

(70) Pentachlorophenol (C)




11.174min (-0.012) 186278.40ng

response 291549

Ion	Exp%	Act%
265.70	100	100
268.00	67.10	66.90
264.00	65.60	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032520\
Data File : BF119499.D
Acq On : 25 Mar 2020 11:16
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 01:49:47 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 18 15:11:18 2020
Response via : Initial Calibration

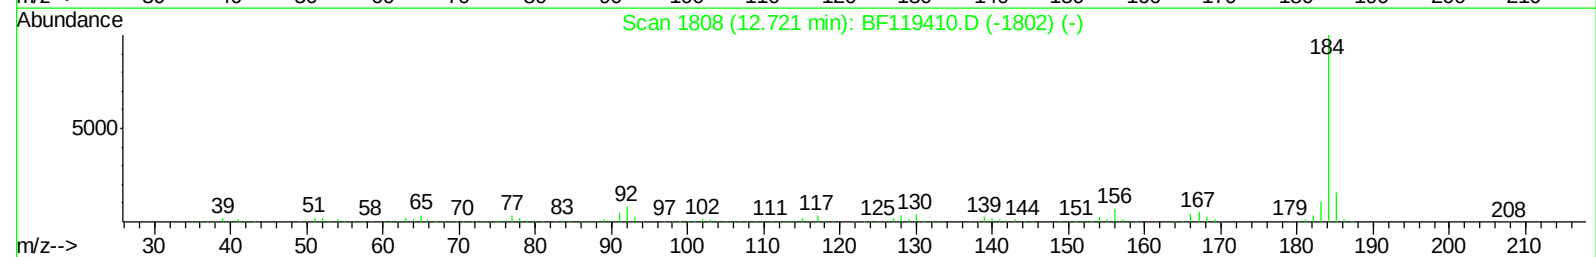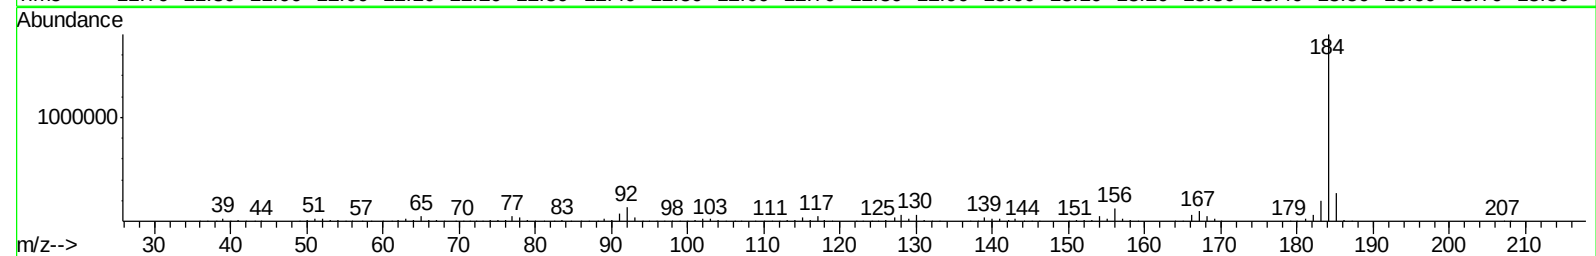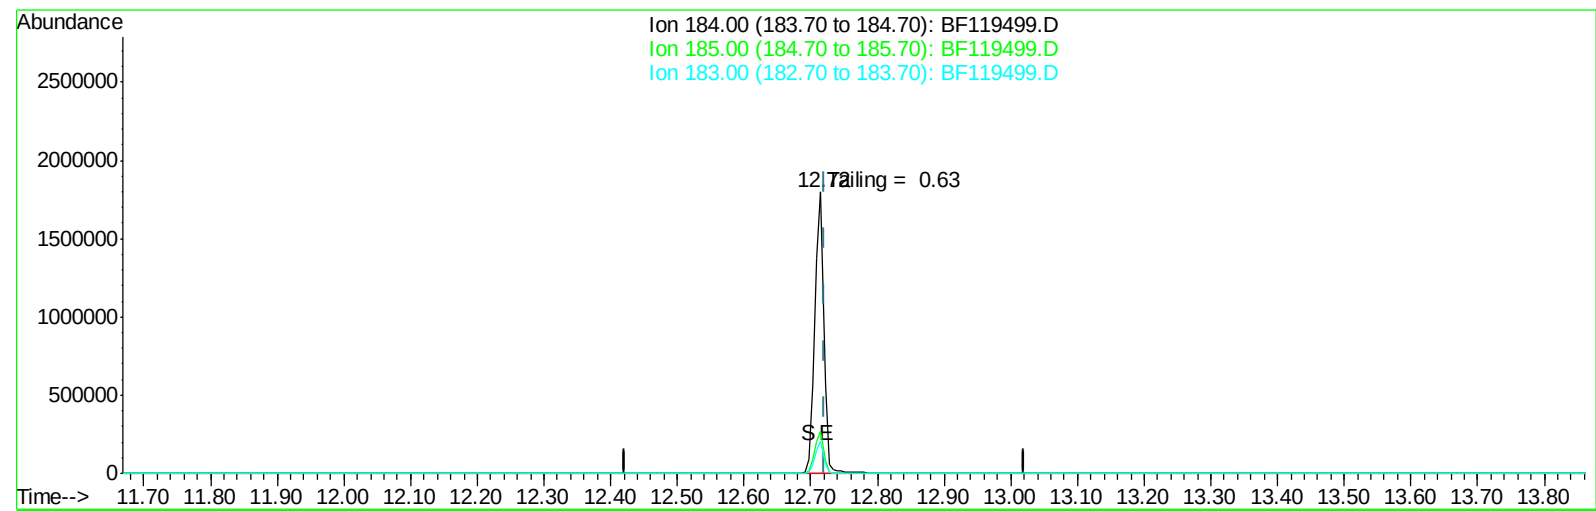

TIC: BF119499.D

(77) Benzidine

12.715min (-0.006) 42932.62ng

response 1622508

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.79
183.00	11.20	11.23
0.00	0.00	0.00