
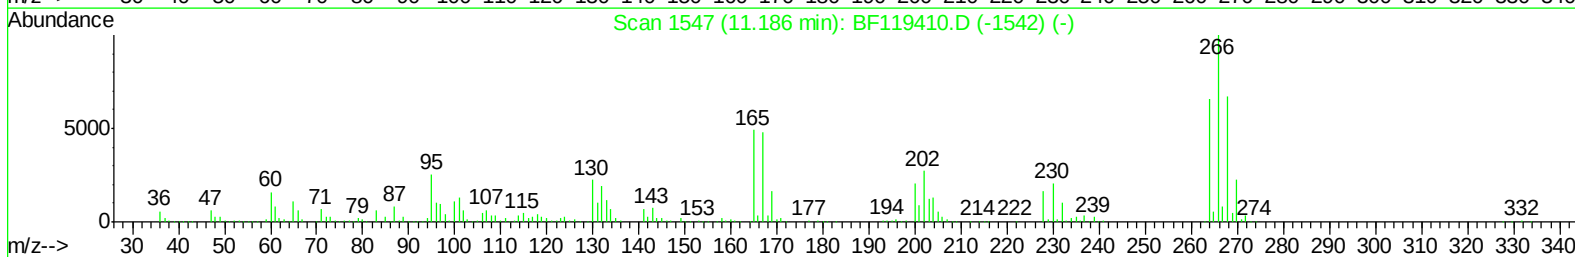
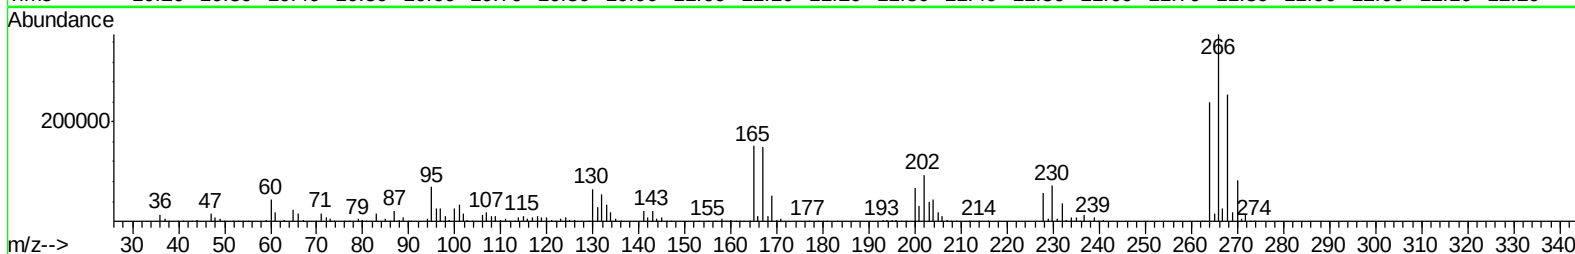


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032520\
Data File : BF119518.D
Acq On : 25 Mar 2020 22:48
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 01:41:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 18 15:11:18 2020
Response via : Initial Calibration

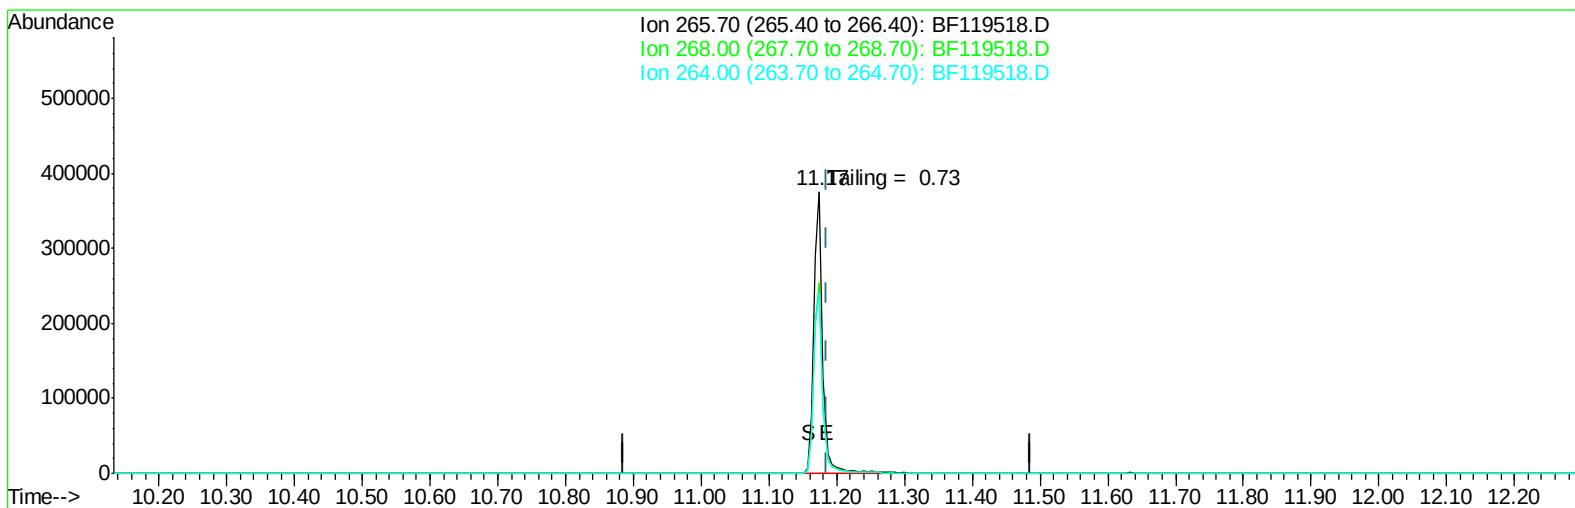

TIC: BF119518.D

(70) Pentachlorophenol (C)




11.175min (-0.012) 30820.30ng

response 340823

Ion	Exp%	Act%
265.70	100	100
268.00	67.10	67.75
264.00	65.60	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032520\
 Data File : BF119518.D
 Acq On : 25 Mar 2020 22:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 01:41:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 18 15:11:18 2020
 Response via : Initial Calibration

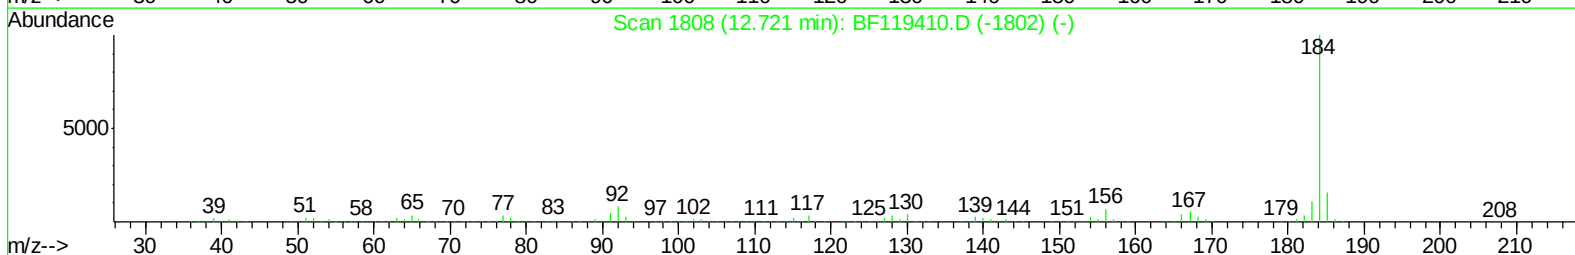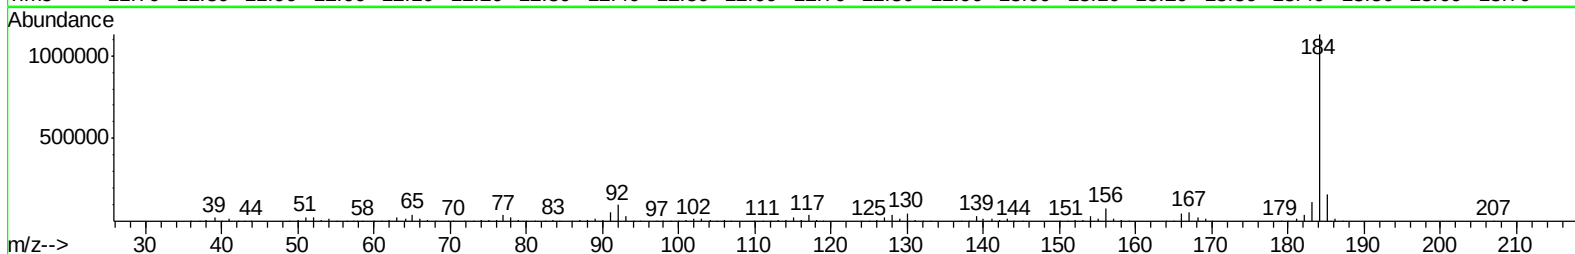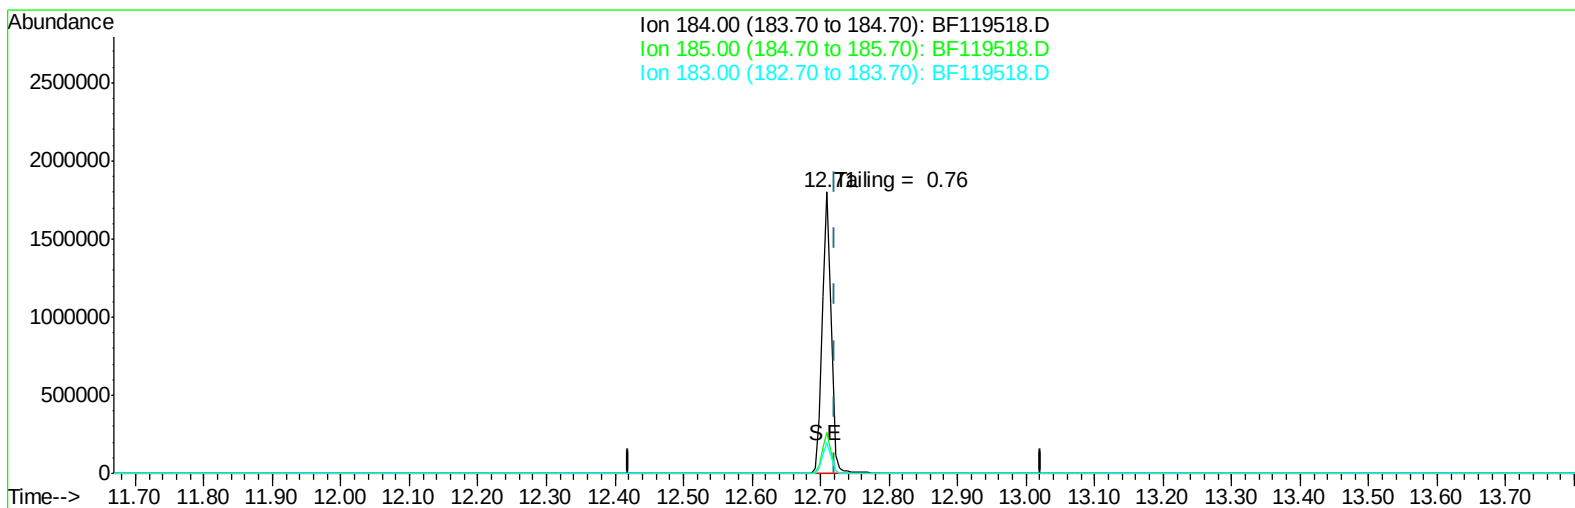

TIC: BF119518.D

(77) Benzidine

12.710min (-0.012) 0.00ng

response 1640566

Ion	Exp%	Act%
184.00	100	100
185.00	16.10	14.46
183.00	11.20	10.89
0.00	0.00	0.00