

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032520\
 Data File : BF119505.D
 Acq On : 25 Mar 2020 15:04
 Operator : CG/JU
 Sample : PB127799BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB127799BL

Quant Time: Mar 25 17:40:51 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 25 14:07:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.84	152	332272	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	1275188	20.00	ng	0.00
39) Acenaphthene-d10	9.89	164	679028	20.00	ng	0.00
64) Phenanthrene-d10	11.37	188	1339111	20.00	ng	0.00
76) Chrysene-d12	14.02	240	1054271	20.00	ng	-0.01
87) Perylene-d12	15.48	264	859884	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.46	112	2531447	121.28	ng	0.01
7) Phenol-d6	6.47	99	3129666	117.38	ng	0.00
23) Nitrobenzene-d5	7.40	82	2037897	86.85	ng	-0.01
42) 2,4,6-Tribromophenol	10.68	330	974183	139.06	ng	0.00
45) 2-Fluorobiphenyl	9.21	172	3773310	82.32	ng	0.00
79) Terphenyl-d14	12.97	244	4562856	84.79	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF032520\
Data File : BF119505.D
Acq On : 25 Mar 2020 15:04
Operator : CG/JU
Sample : PB127799BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB127799BL

Quant Time: Mar 25 17:40:51 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF031820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 25 14:07:20 2020
Response via : Initial Calibration

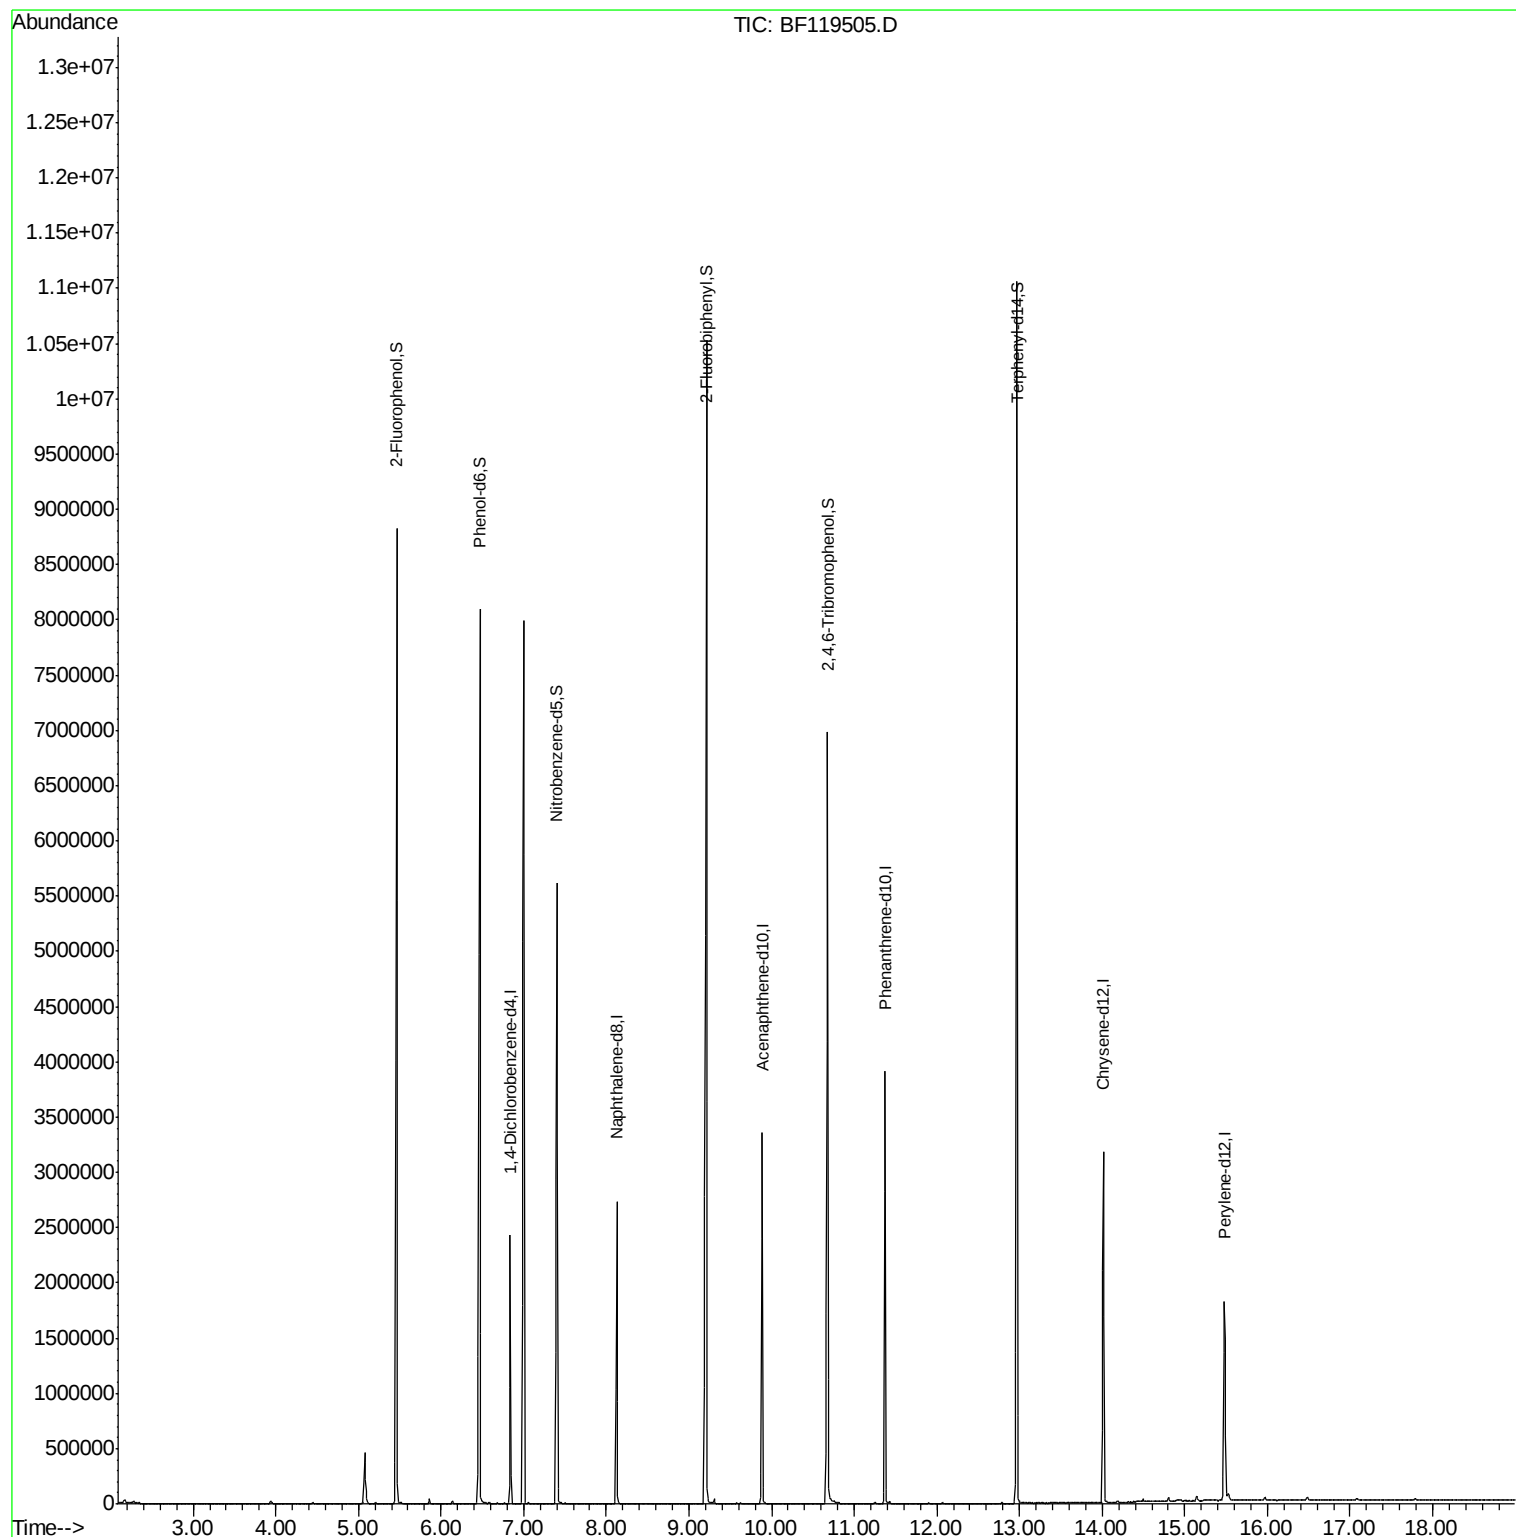

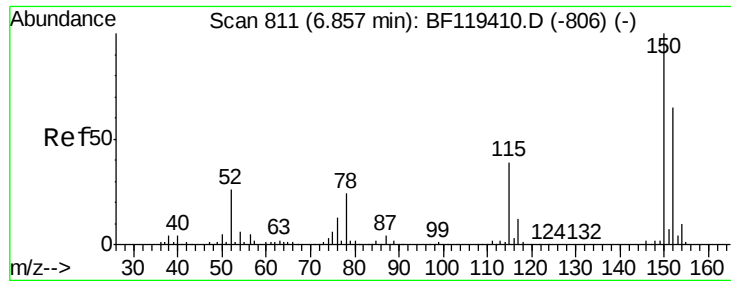


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.84 min Scan# 808
Delta R.T. -0.01 min
Lab File: BF119505.D
Acq: 25 Mar 2020 15:04

Instrument :
BNA_F
ClientSampleId :
PB127799BL

Tot Ion:152 Resp: 332272
Ion Ratio Lower Upper
152 100
150 155.9 123.9 185.9
115 62.4 47.8 71.6

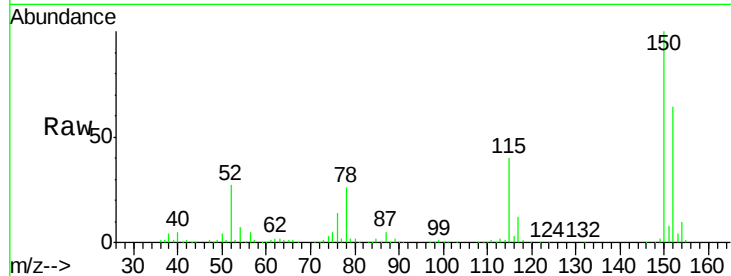


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

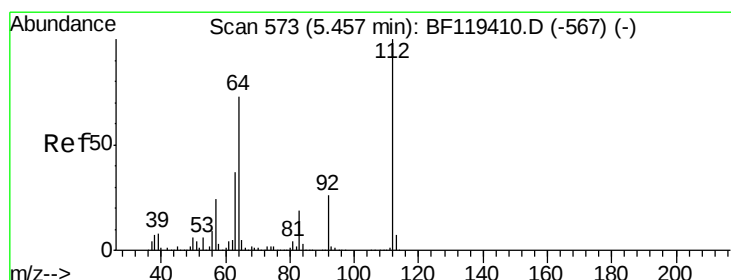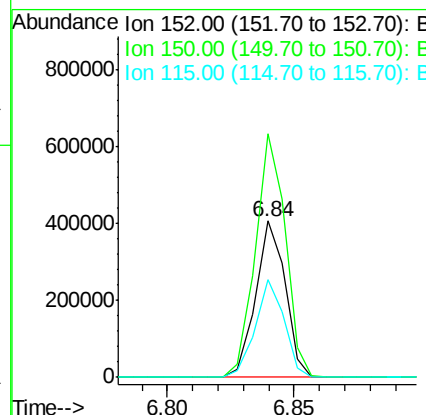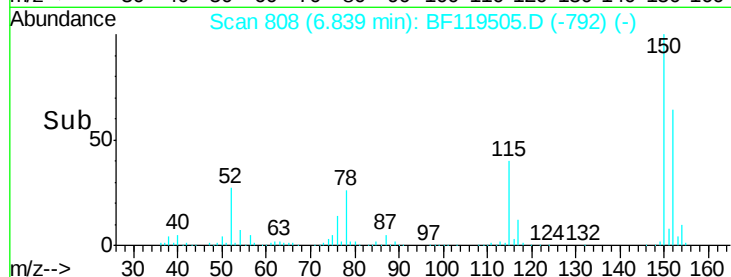



#5


2-Fluorophenol
Concen: 121.281 ng
RT: 5.46 min Scan# 574
Delta R.T. 0.01 min
Lab File: BF119505.D
Acq: 25 Mar 2020 15:04

Tgt Ion:112 Resp: 2531447
Ion Ratio Lower Upper
112 100
64 73.2 58.1 87.1
63 38.5 29.7 44.5

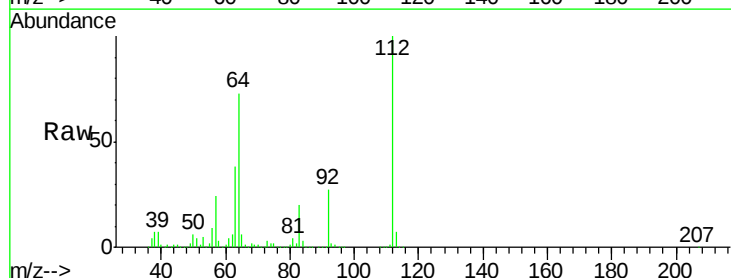

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

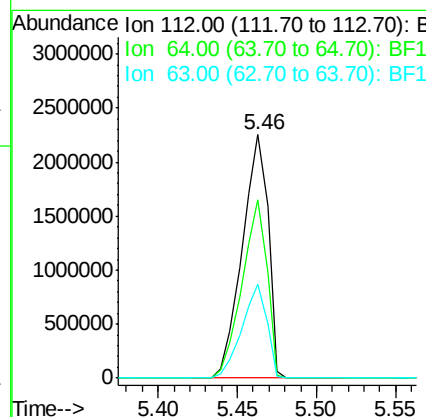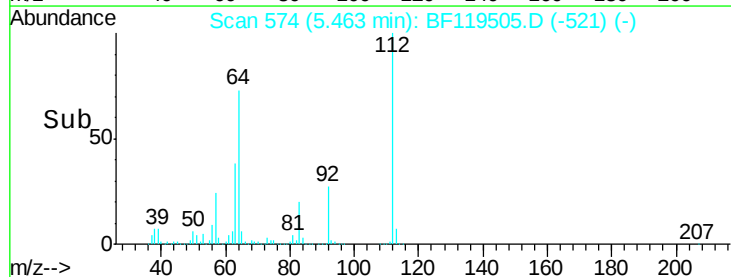

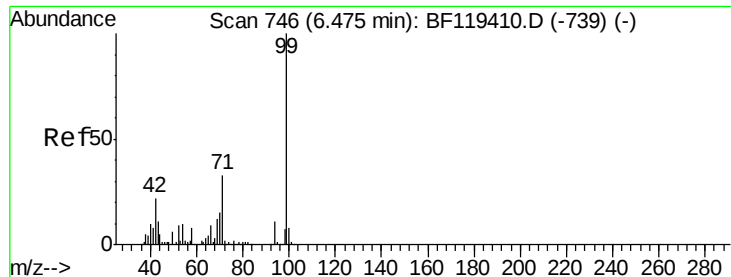

#7

Phenol-d6

Concen: 117.377 ng

RT: 6.47 min Scan# 745

Delta R.T. -0.01 min

Lab File: BF119505.D

Acq: 25 Mar 2020 15:04

Instrument :

BNA_F

ClientSampleId :

PB127799BL


Tot Ion: 99 Resp: 3129666

Ion Ratio Lower Upper

99 100

42 21.2 17.8 26.6




71 34.6 26.0 39.0

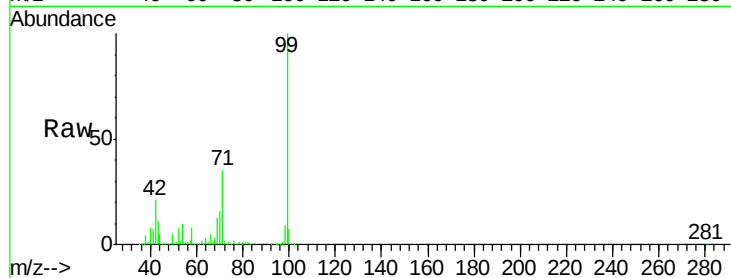

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

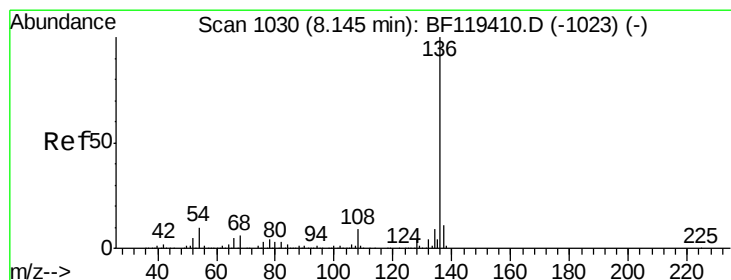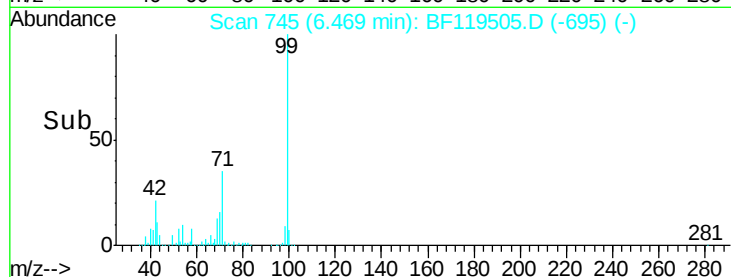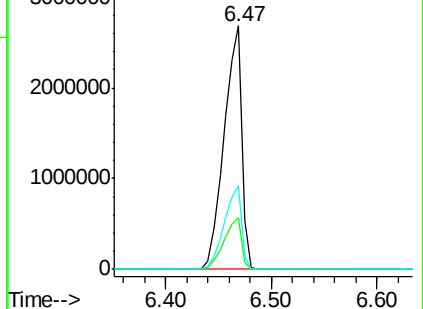

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.13 min Scan# 1027

Delta R.T. -0.01 min

Lab File: BF119505.D

Acq: 25 Mar 2020 15:04

Tgt Ion: 136 Resp: 1275188


Ion Ratio Lower Upper

136 100

137 10.8 8.4 12.6

54 9.9 8.3 12.5

68 5.6 4.9 7.3


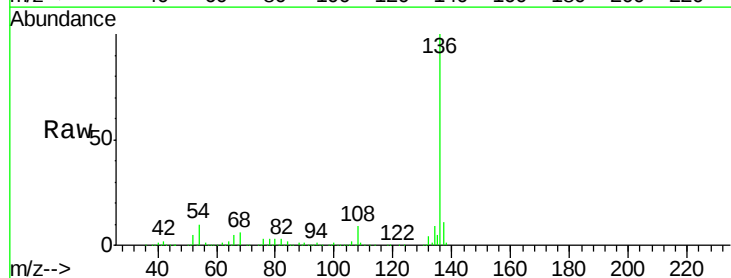



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

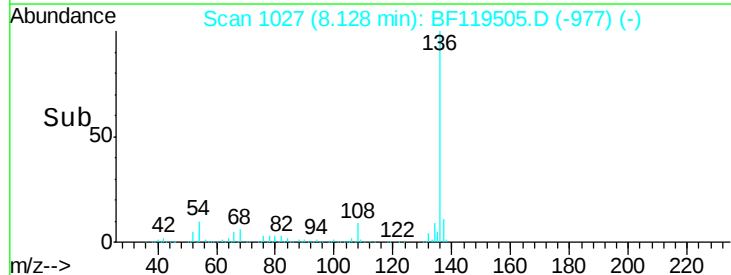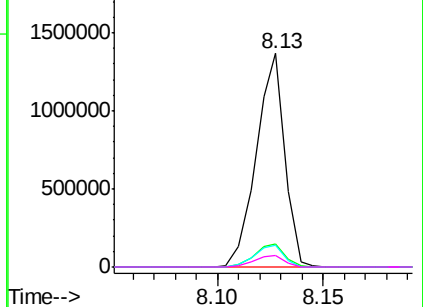


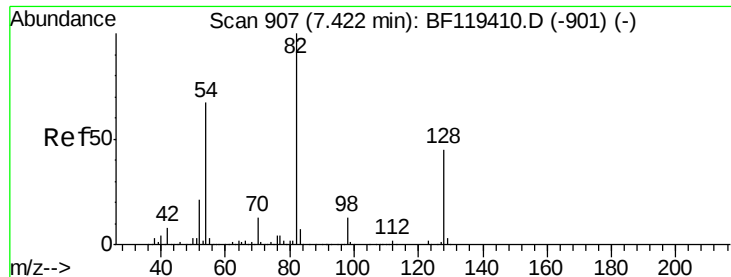




#23
Nitrobenzene-d5
Concen: 86.854 ng
RT: 7.40 min Scan# 904
Delta R.T. -0.01 min
Lab File: BF119505.D
Acq: 25 Mar 2020 15:04

Instrument :
BNA_F
ClientSampleId :
PB127799BL

Tot Ion: 82 Resp: 2037897
Ion Ratio Lower Upper
82 100
128 45.6 35.8 53.8
54 65.4 53.4 80.0

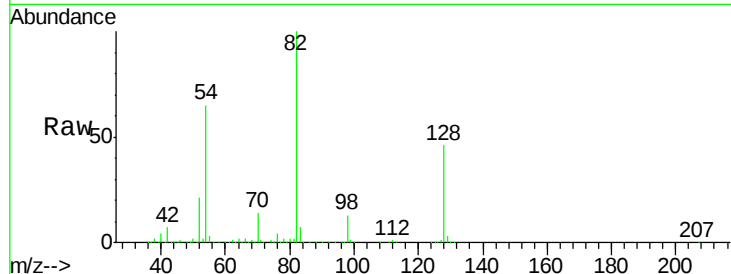


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

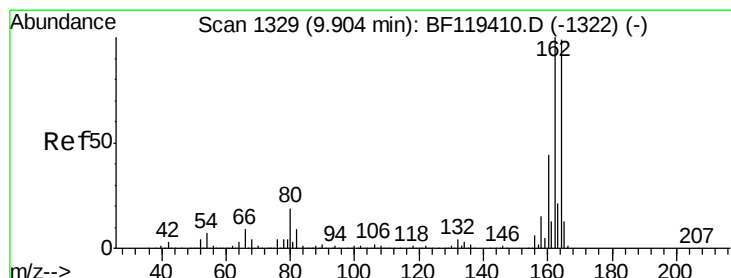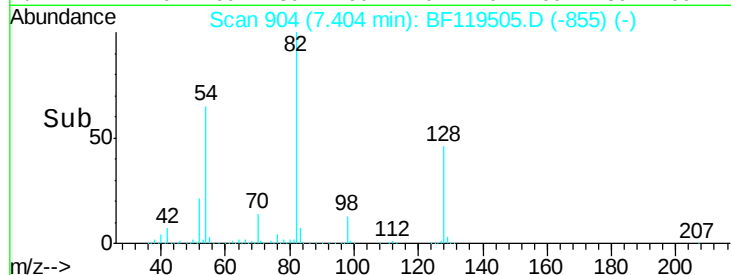
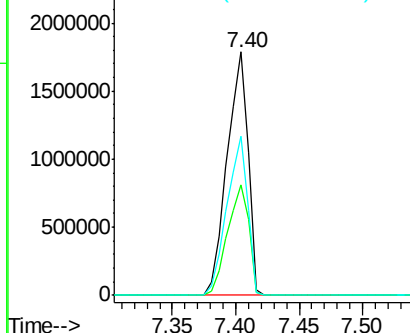


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.89 min Scan# 1326
Delta R.T. -0.01 min
Lab File: BF119505.D
Acq: 25 Mar 2020 15:04

Tgt Ion:164 Resp: 679028
Ion Ratio Lower Upper
164 100
162 102.4 80.7 121.1
160 47.8 35.5 53.3

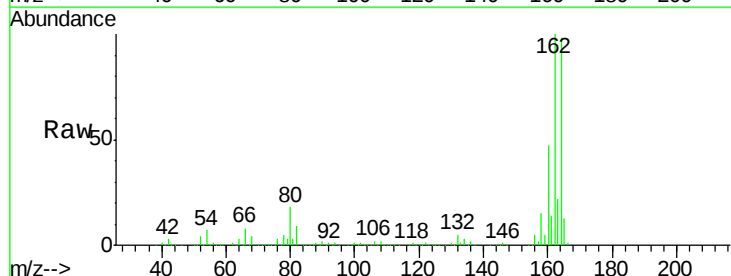

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

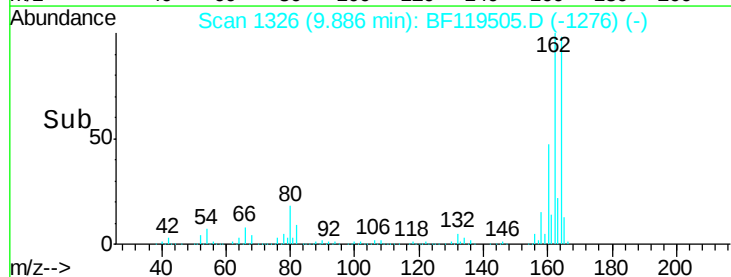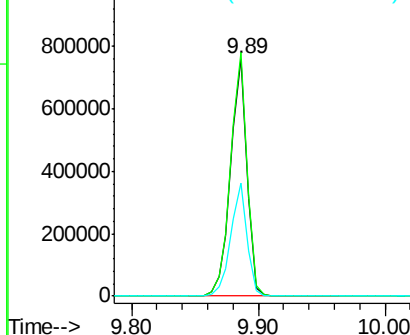







#42
 2,4,6-Tribromophenol
 Concen: 139.064 ng
 RT: 10.68 min Scan# 1461
 Delta R.T. -0.00 min
 Lab File: BF119505.D
 Acq: 25 Mar 2020 15:04

Instrument :
 BNA_F
 ClientSampleId :
 PB127799BL

Tot Ion:330 Resp: 974183
 Ion Ratio Lower Upper
 330 100
 332 97.7 77.6 116.4
 141 32.7 26.6 40.0

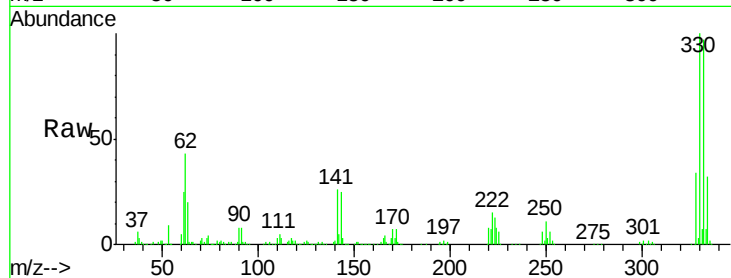


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

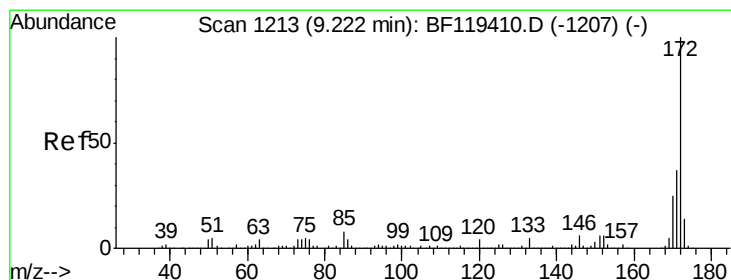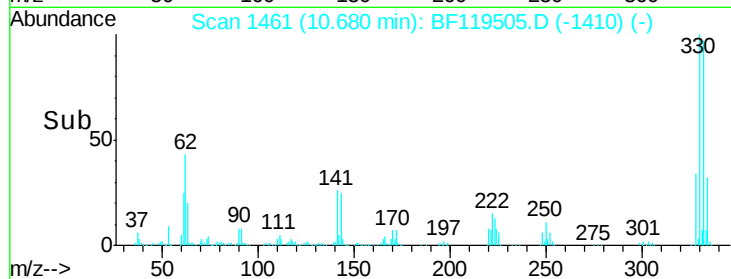
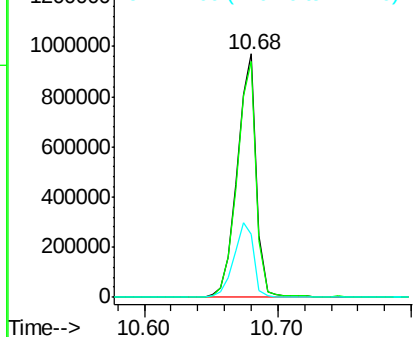



#45
 2-Fluorobiphenyl
 Concen: 82.324 ng
 RT: 9.21 min Scan# 1211
 Delta R.T. -0.01 min
 Lab File: BF119505.D
 Acq: 25 Mar 2020 15:04

Tgt Ion:172 Resp: 3773310
 Ion Ratio Lower Upper
 172 100
 171 38.3 29.9 44.9
 170 26.1 20.1 30.1

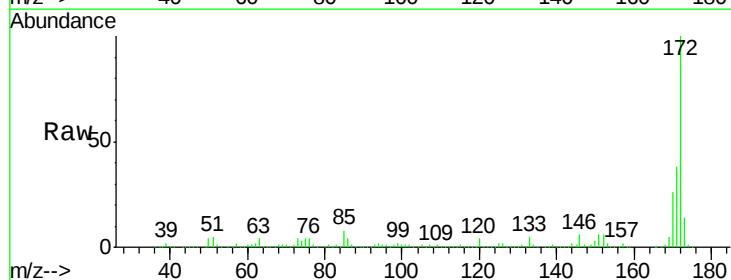

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



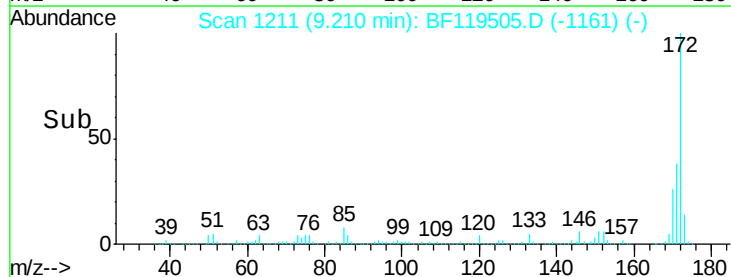
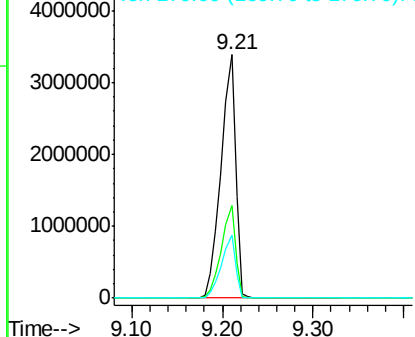


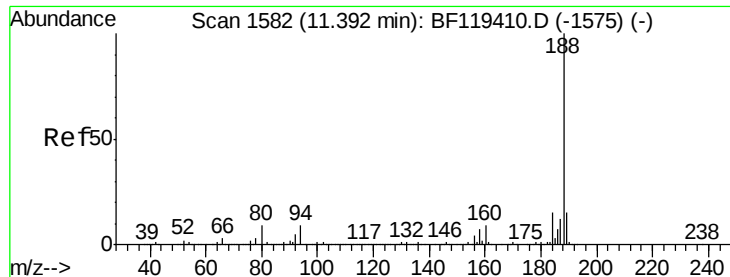

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.37 min Scan# 1579
Delta R.T. -0.01 min
Lab File: BF119505.D
Acq: 25 Mar 2020 15:04




Instrument :
BNA_F
ClientSampleId :
PB127799BL


Tot Ion:188 Resp: 1339111
Ion Ratio Lower Upper
188 100
94 9.4 7.1 10.7
80 9.9 7.5 11.3

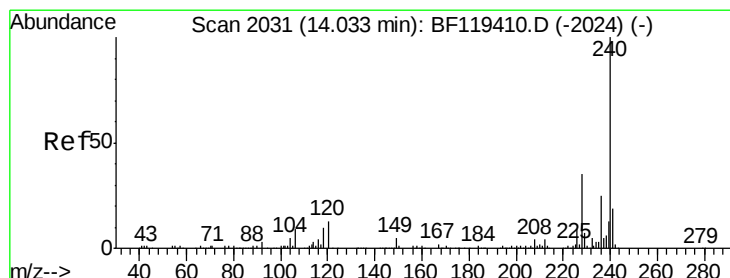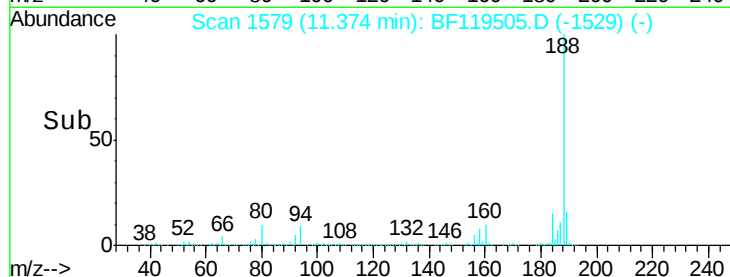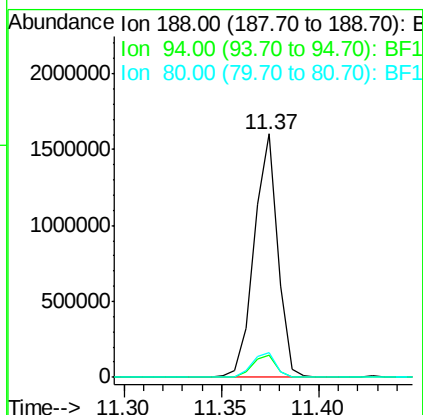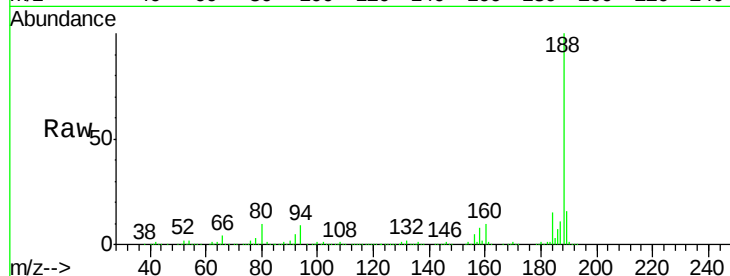

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2028
Delta R.T. -0.01 min
Lab File: BF119505.D
Acq: 25 Mar 2020 15:04

Tgt Ion:240 Resp: 1054271
Ion Ratio Lower Upper
240 100
120 11.3 10.2 15.4
236 25.9 20.4 30.6

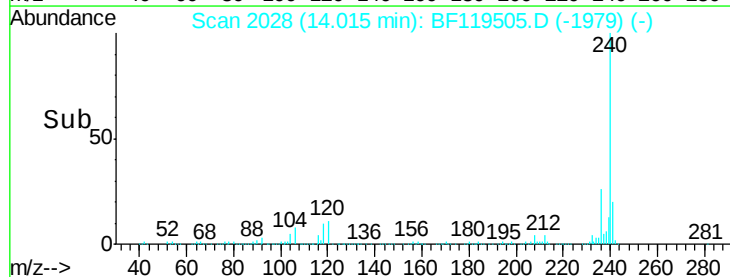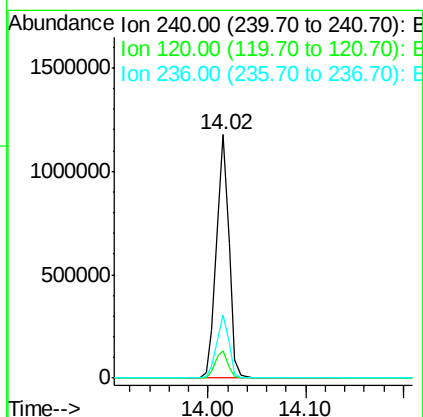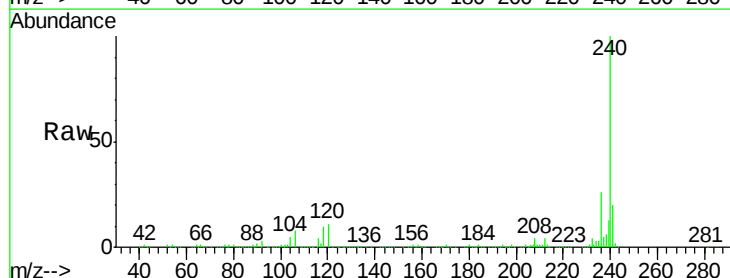

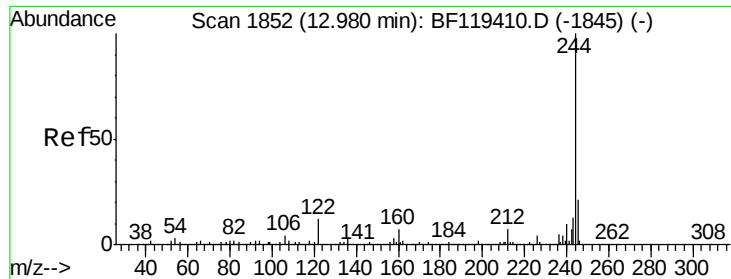

#79

Terphenyl-d14

Concen: 84.794 ng

RT: 12.97 min Scan# 1850

Delta R.T. -0.00 min

Lab File: BF119505.D

Acq: 25 Mar 2020 15:04

Instrument :

BNA_F

ClientSampleId :

PB127799BL


Tot Ion:244 Resp: 4562856

Ion Ratio Lower Upper

244 100

212 7.5 5.7 8.5




122 14.0 9.8 14.8

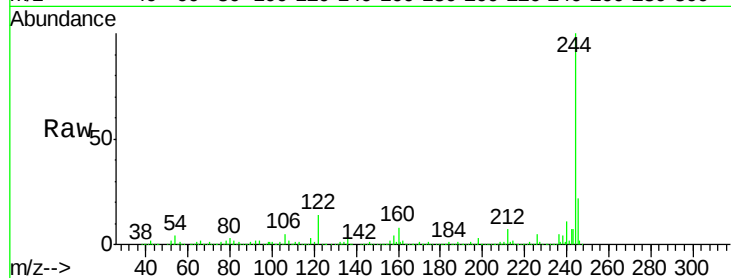

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

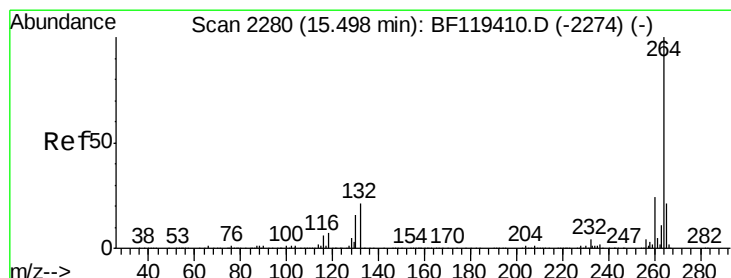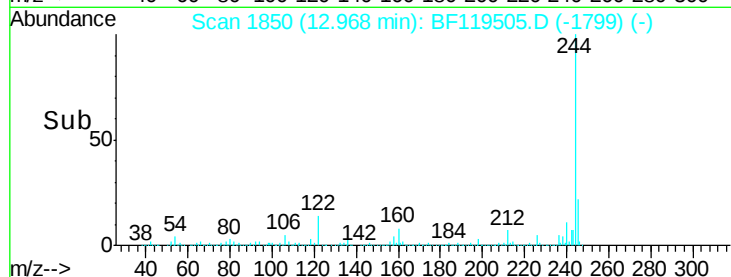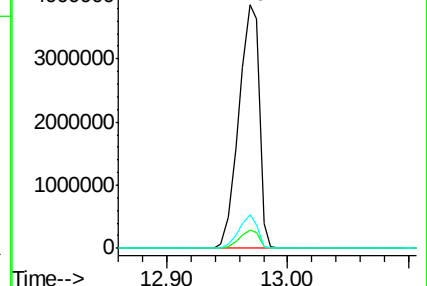

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.48 min Scan# 2277

Delta R.T. -0.01 min

Lab File: BF119505.D

Acq: 25 Mar 2020 15:04


Tgt Ion:264 Resp: 859884

Ion Ratio Lower Upper

264 100

260 23.1 19.2 28.8

265 21.7 16.9 25.3

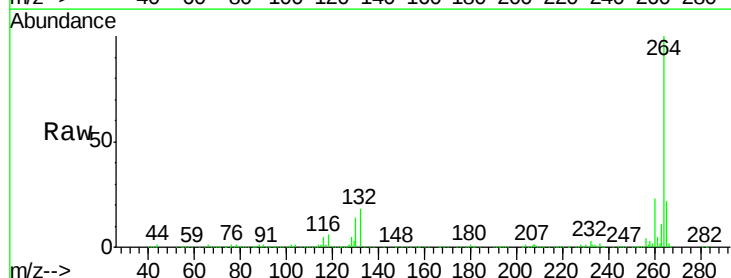

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

