


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032520\
 Data File : BF119499.D
 Acq On : 25 Mar 2020 11:16
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 18 15:11:18 2020

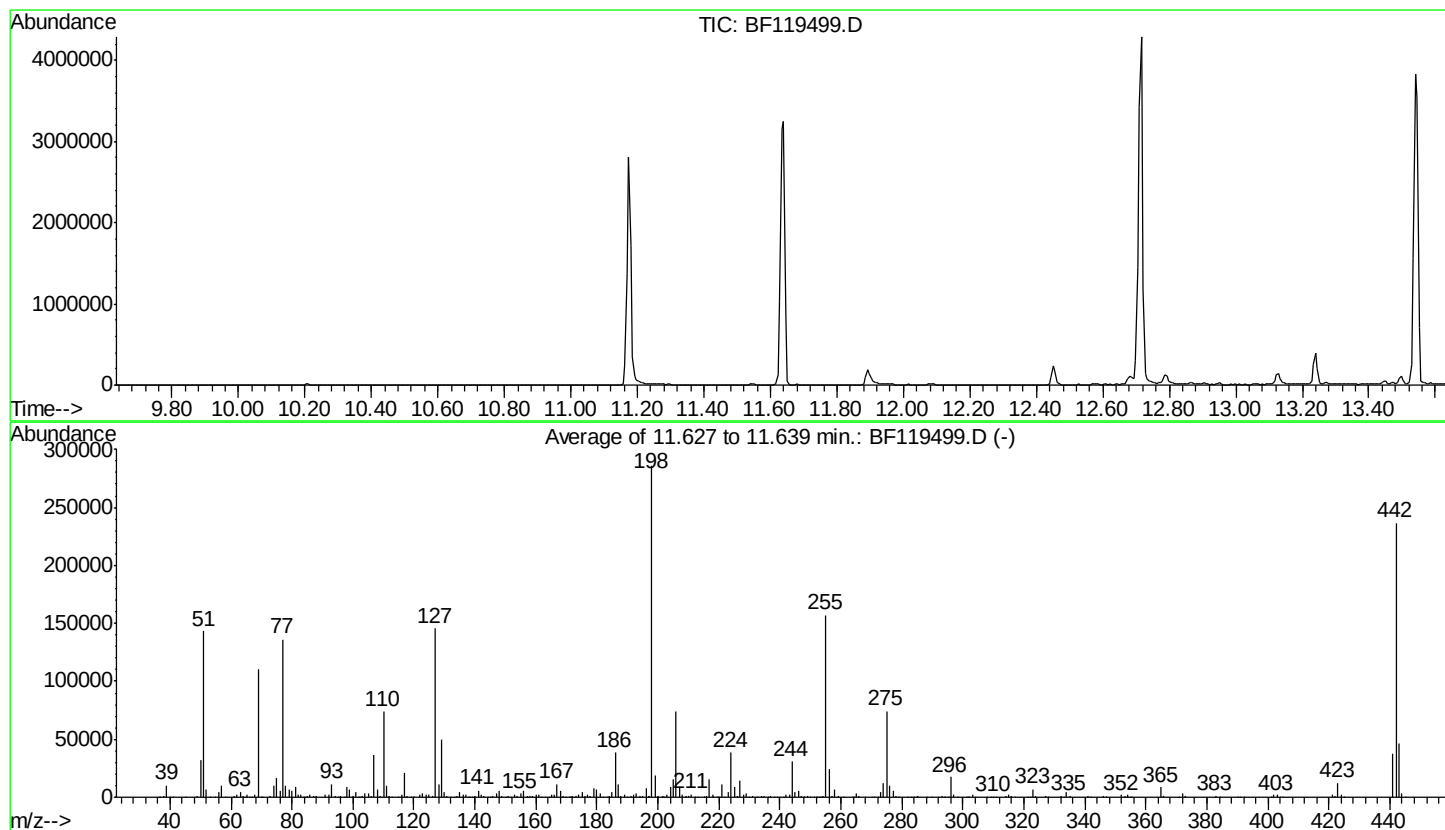

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.0	143056	PASS
68	69	0.00	2	1.6	1767	PASS
69	198	0.00	100	38.6	110505	PASS
70	69	0.00	2	0.3	292	PASS
127	198	10	80	50.8	145293	PASS
197	198	0.00	2	0.3	914	PASS
198	198	100	100	100.0	286029	PASS
199	198	5	9	6.5	18479	PASS
275	198	10	60	25.9	74026	PASS
365	198	1	100	3.0	8507	PASS
441	198	0.01	100	13.2	37860	PASS
442	198	50	100	82.7	236594	PASS
443	442	15	24	19.7	46700	PASS