


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF032520\
 Data File : BF119518.D
 Acq On : 25 Mar 2020 22:48
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 18 15:11:18 2020

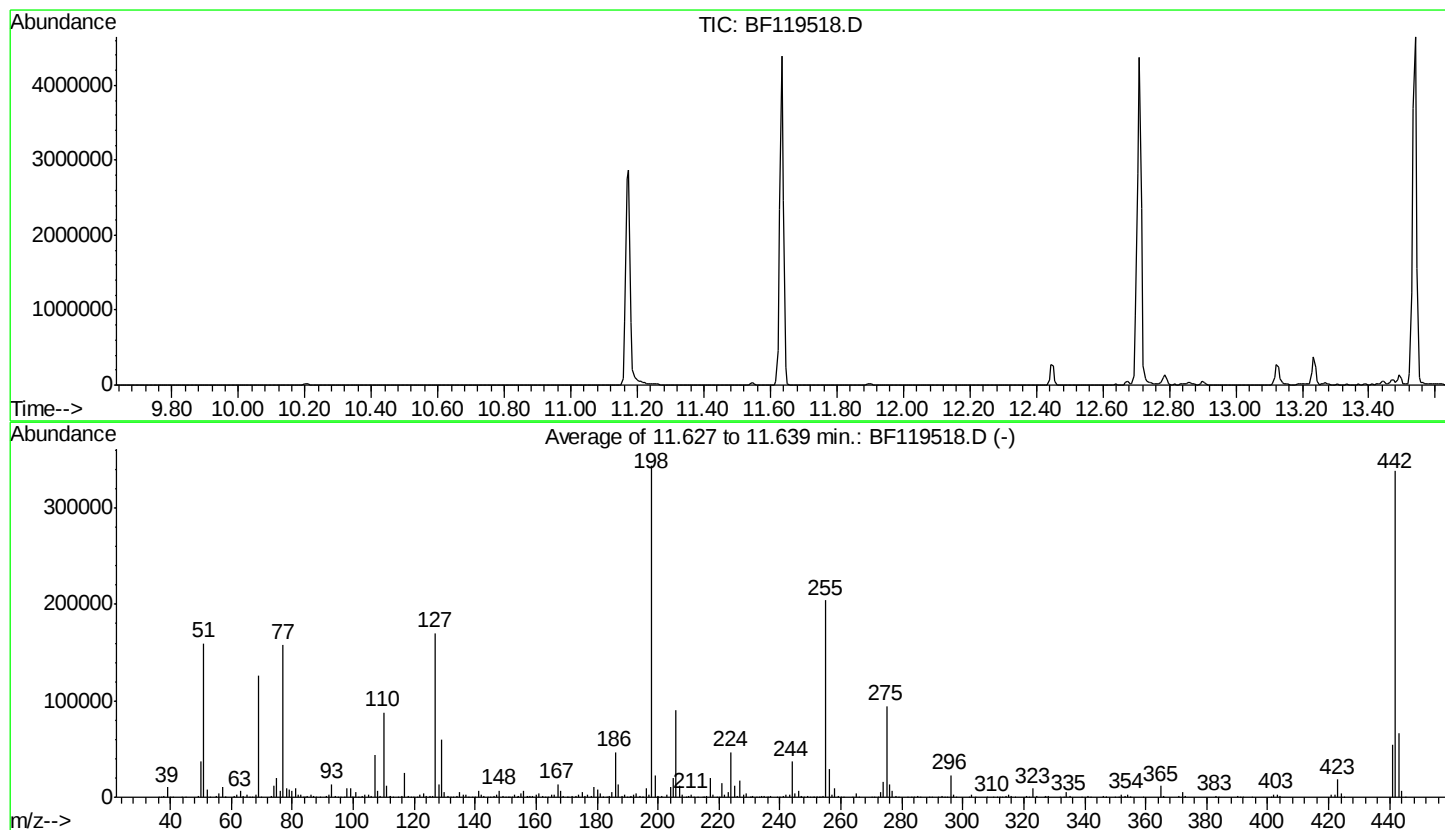

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.3	159413	PASS
68	69	0.00	2	1.7	2126	PASS
69	198	0.00	100	36.6	126000	PASS
70	69	0.00	2	0.6	702	PASS
127	198	10	80	49.6	170536	PASS
197	198	0.00	2	0.8	2682	PASS
198	198	100	100	100.0	343978	PASS
199	198	5	9	6.6	22616	PASS
275	198	10	60	27.5	94442	PASS
365	198	1	100	3.4	11628	PASS
441	198	0.01	100	15.9	54538	PASS
442	198	50	100	98.4	338474	PASS
443	442	15	24	19.7	66578	PASS