
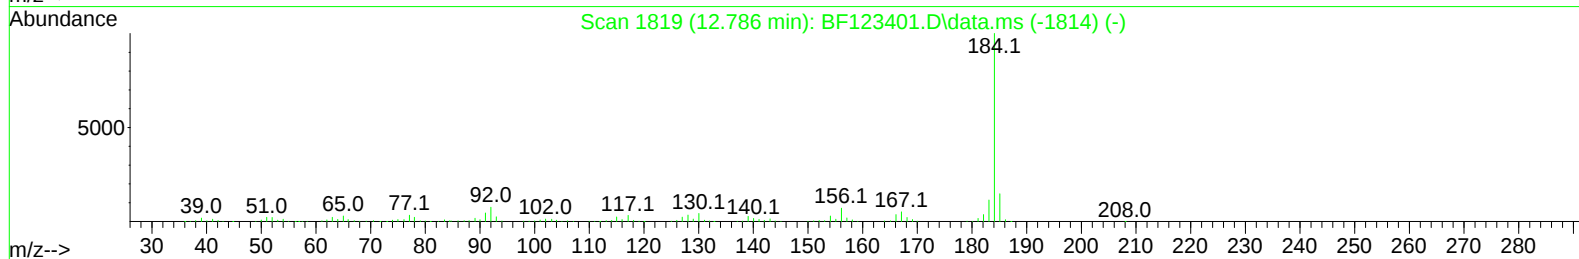
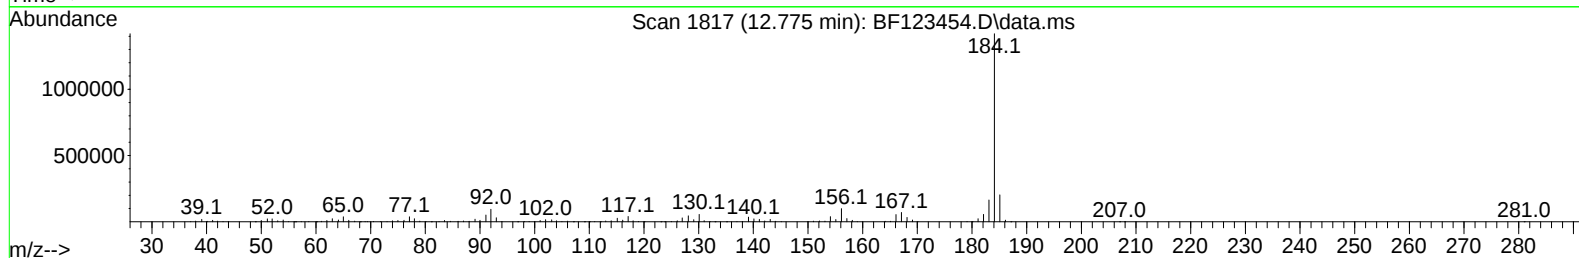


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
Data File : BF123454.D
Acq On : 25 Mar 2021 10:50
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 12:34:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:51:15 2021
Response via : Initial Calibration

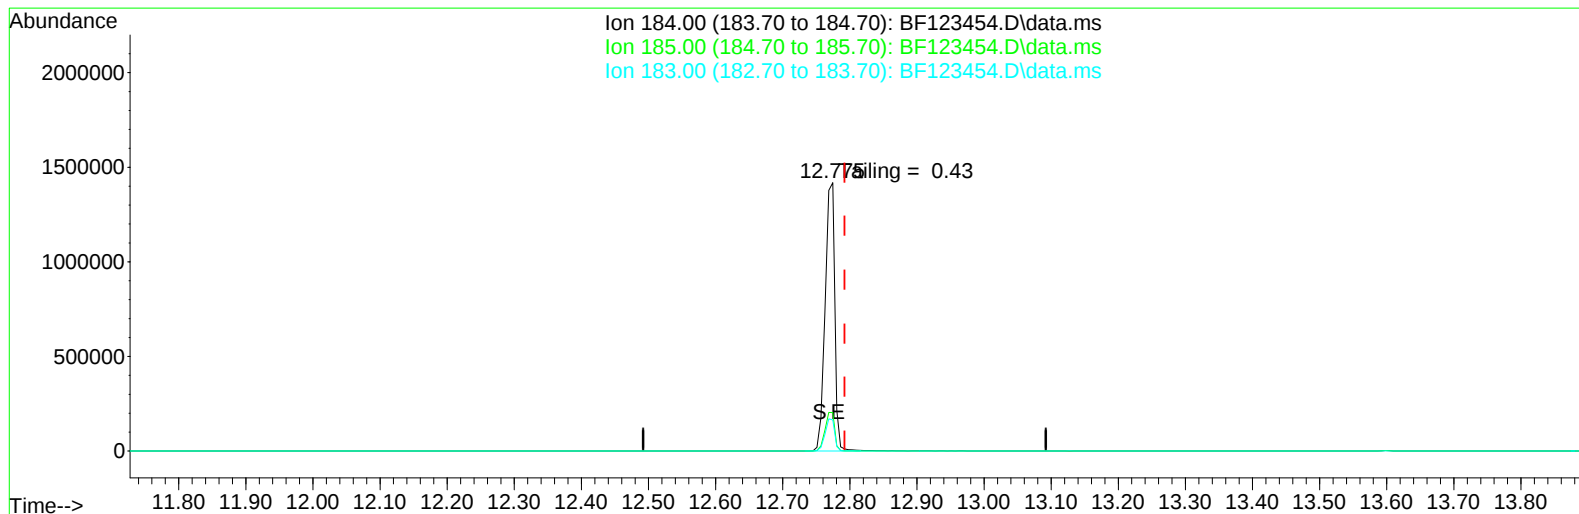

TIC: BF123454.D\data.ms

(77) Benzidine




12.775min (-0.018) 0.00 ng

response 1413711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.31
183.00	12.10	11.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
Data File : BF123454.D
Acq On : 25 Mar 2021 10:50
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 12:34:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:51:15 2021
Response via : Initial Calibration

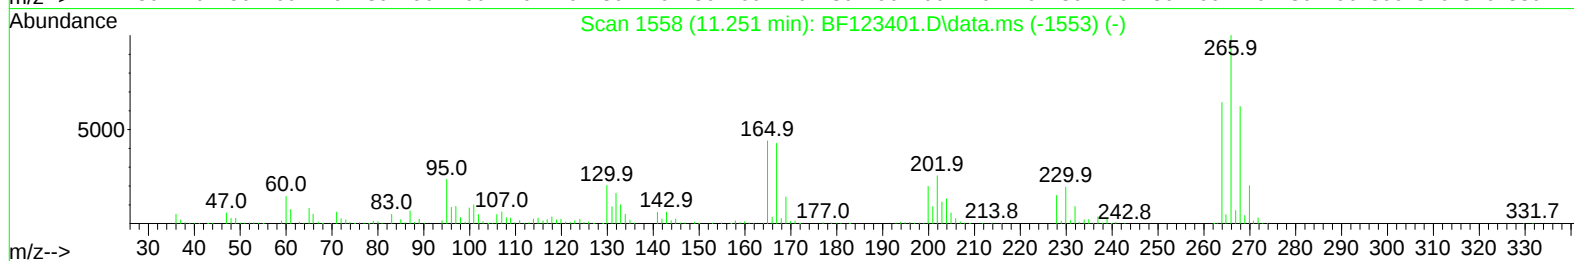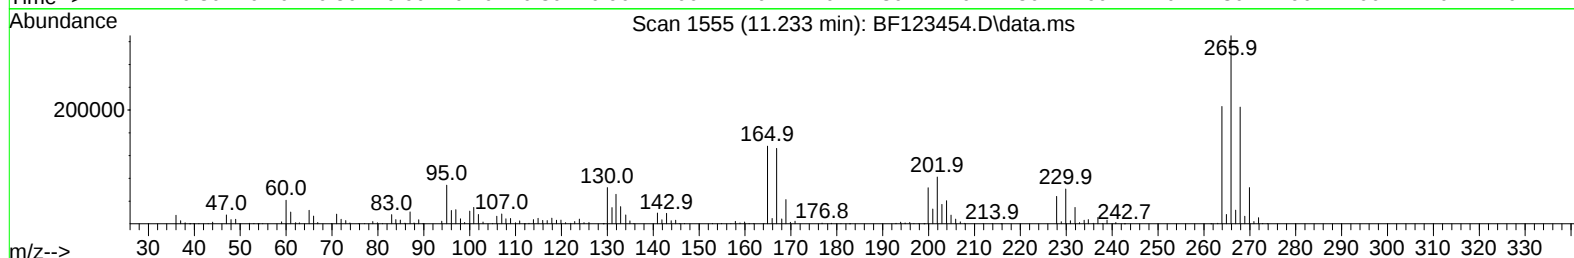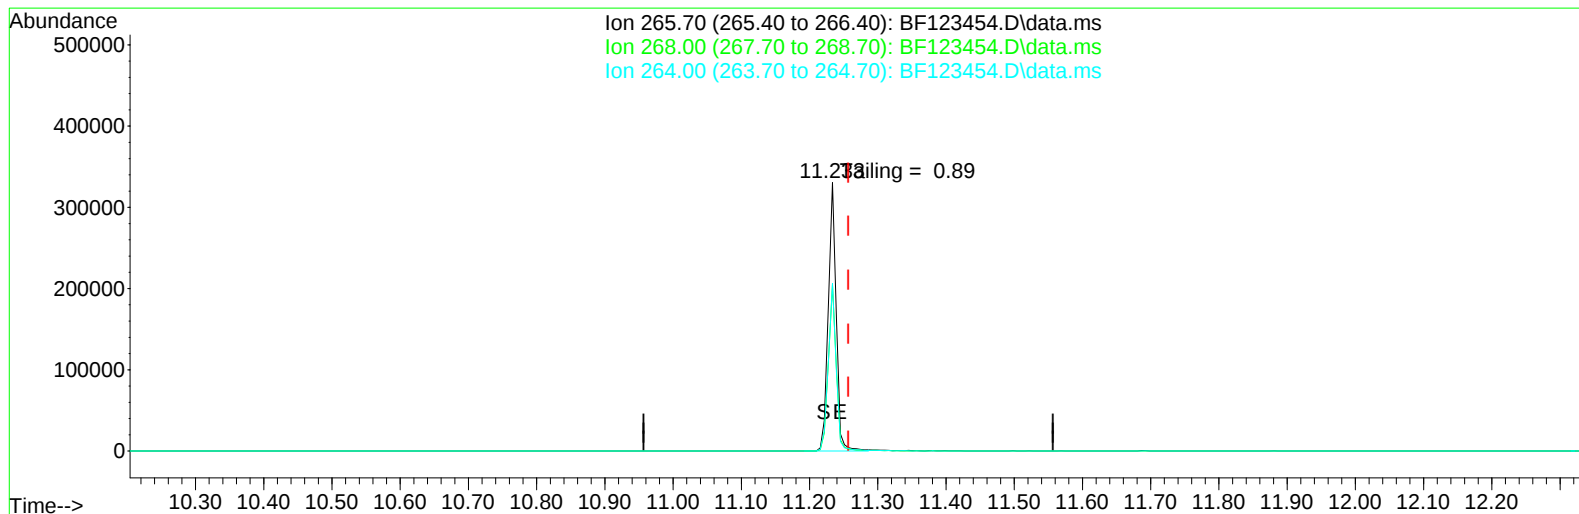

TIC: BF123454.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.023) 46822.46 ng

response 270580

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.10
264.00	62.30	62.41
0.00	0.00	0.00