

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
 Data File : BF123456.D
 Acq On : 25 Mar 2021 12:02
 Operator : JU/CG
 Sample : PB135237BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB135237BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123456.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.287	21	34	39	rVB	102285	145953	2.09%	0.325%
2	2.393	46	52	57	rVB	68736	85658	1.22%	0.191%
3	5.145	517	520	527	rVB	86859	107838	1.54%	0.240%
4	5.528	579	585	588	rBV	6054973	5976502	85.47%	13.313%
5	6.522	748	754	757	rBV	5556203	6078631	86.93%	13.540%
6	6.898	814	818	821	rBV	1706101	1328896	19.00%	2.960%
7	7.457	907	913	916	rBV	3563656	3932399	56.24%	8.759%
8	8.180	1031	1036	1040	rBV	1828941	1715648	24.54%	3.822%
9	9.263	1214	1220	1223	rBV	7392421	6613490	94.58%	14.732%
10	9.939	1330	1335	1339	rBV	2232198	1925774	27.54%	4.290%
11	10.733	1463	1470	1473	rBV	4658562	4399439	62.92%	9.800%
12	11.433	1583	1589	1592	rBV	2072482	1952528	27.92%	4.349%
13	11.951	1671	1677	1688	rBV3	71310	134531	1.92%	0.300%
14	13.027	1854	1860	1863	rBV	7377457	6992623	100.00%	15.576%
15	13.998	2019	2025	2034	rBV2	38672	136465	1.95%	0.304%
16	14.074	2034	2038	2042	rVB	1919492	1760915	25.18%	3.922%
17	15.574	2287	2293	2298	rBV2	1287999	1606222	22.97%	3.578%




Sum of corrected areas: 44893512

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
Data File : BF123456.D
Acq On : 25 Mar 2021 12:02
Operator : JU/CG
Sample : PB135237BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135237BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

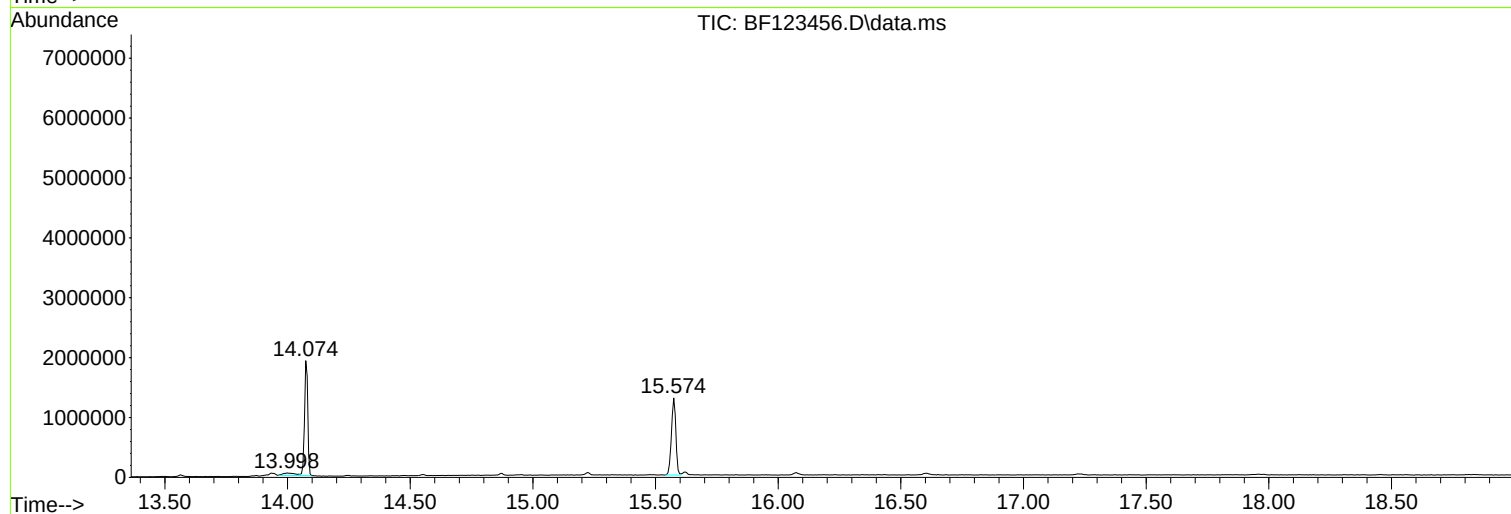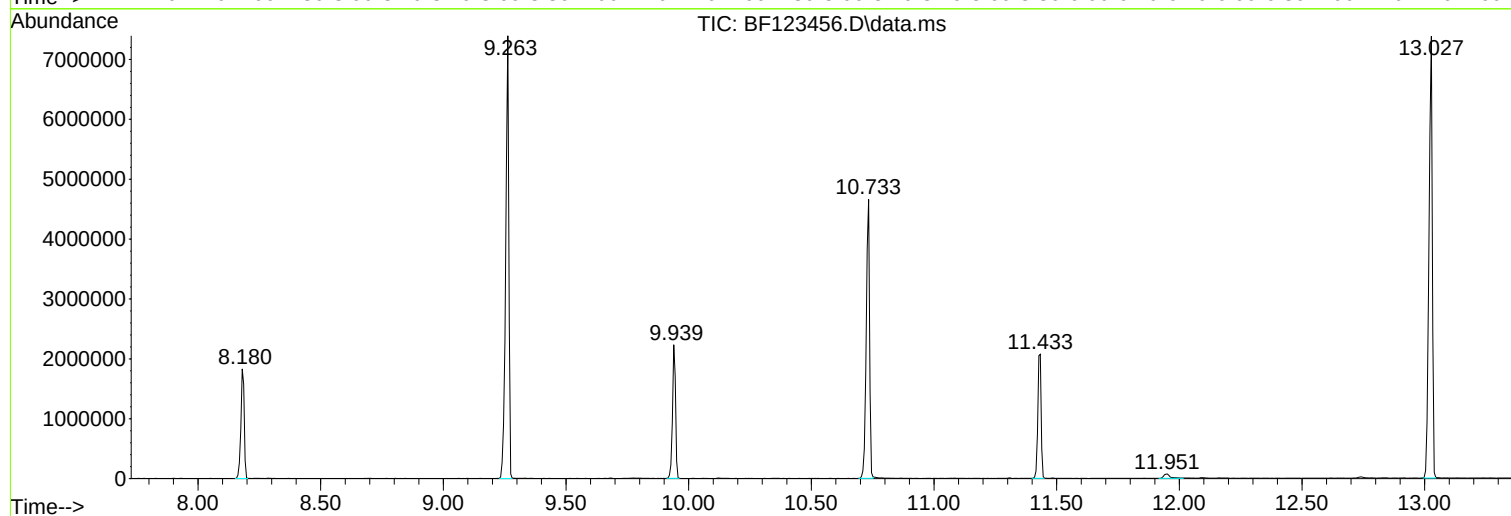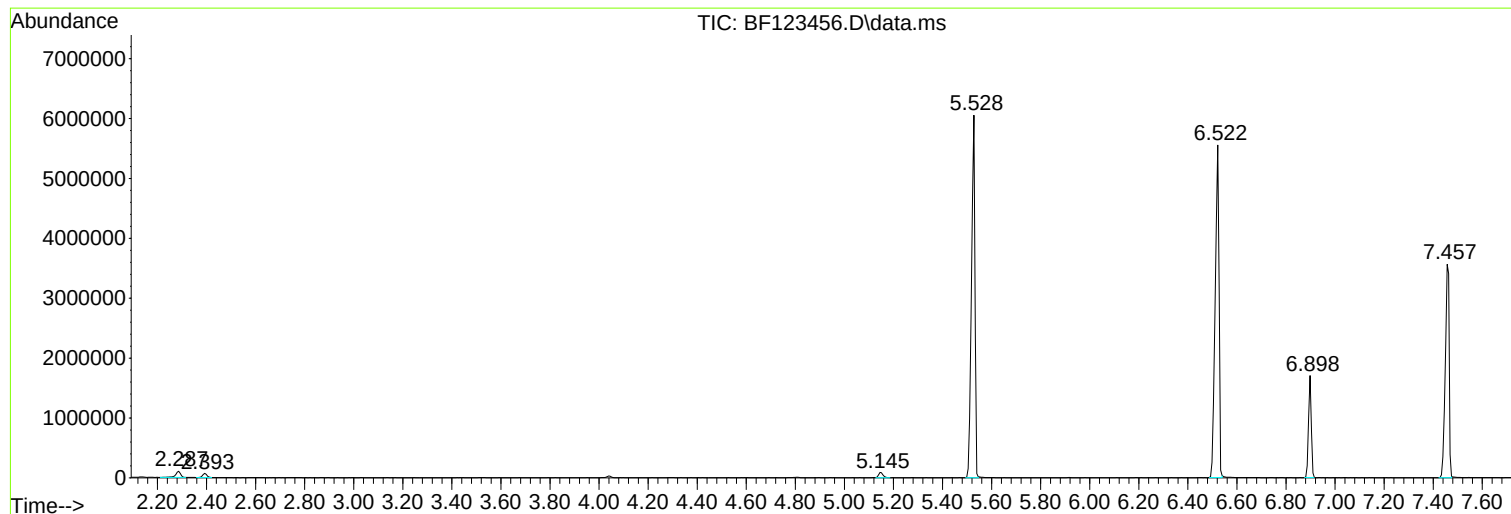

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
Data File : BF123456.D
Acq On : 25 Mar 2021 12:02
Operator : JU/CG
Sample : PB135237BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135237BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.287	2.20 ng	145953	1,4-Dichlorobenzene-d4	6.898

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2,5-Dimethyl-4-hydroxy-3-hexanone	144	C8H16O2	000815-77-0	37
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	23
4			3-Pentanol, 2,4-dimethyl-	116	C7H16O	000600-36-2	23
5			1,3-Dioxolane, 2-methyl-	88	C4H8O2	000497-26-7	23

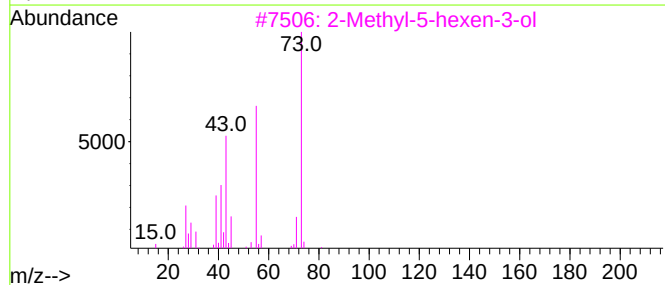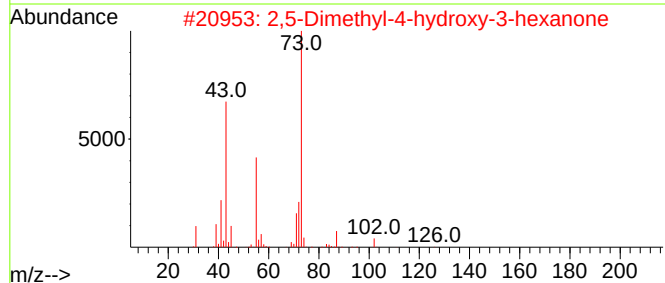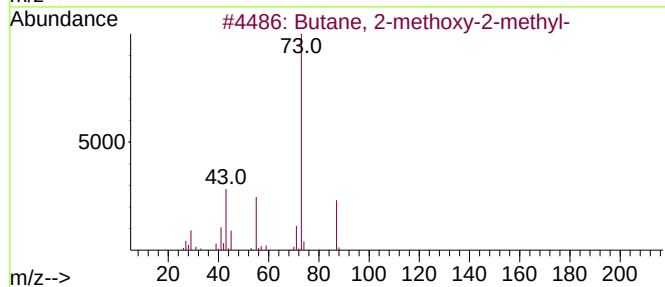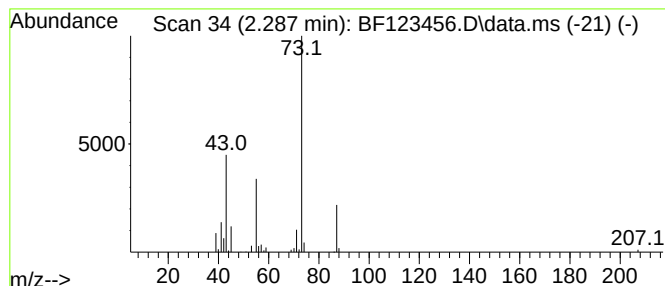

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
Data File : BF123456.D
Acq On : 25 Mar 2021 12:02
Operator : JU/CG
Sample : PB135237BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB135237BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.287	2.2	ng	145953	1	6.898	1328900	20.0