
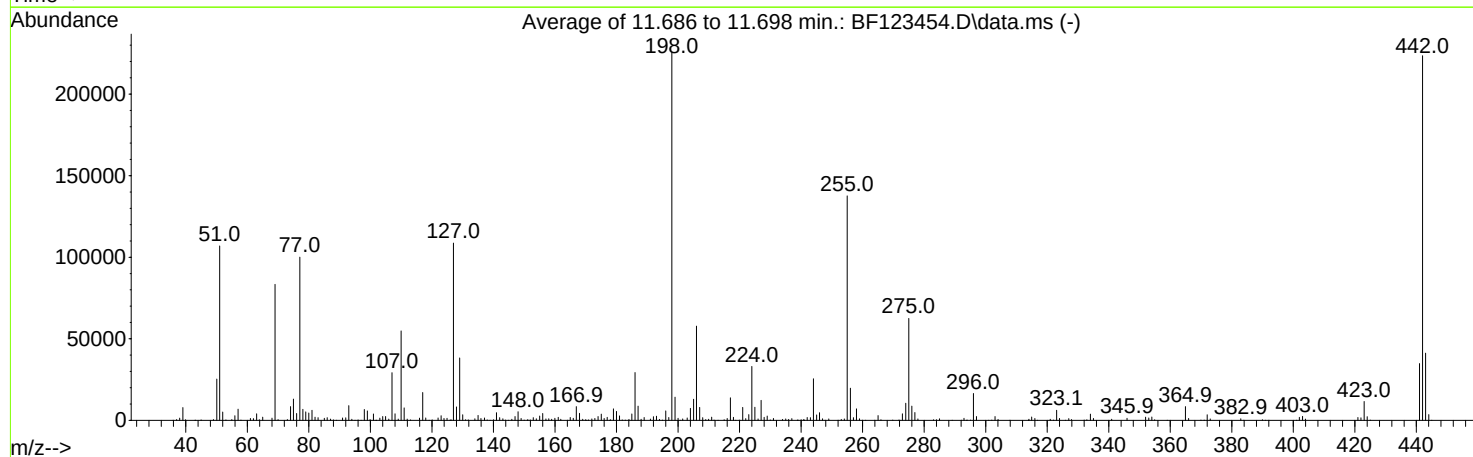


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
 Data File : BF123454.D
 Acq On : 25 Mar 2021 10:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 17:06:59 2021

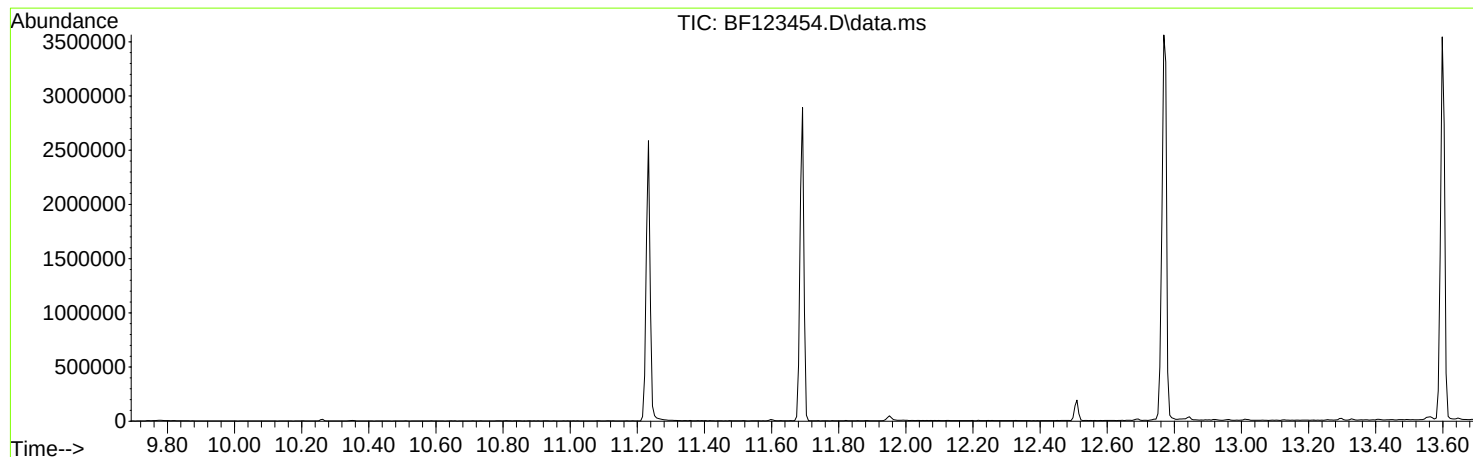

AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.4	106885	PASS
68	69	0.00	2	1.6	1373	PASS
69	198	0.00	100	37.0	83387	PASS
70	69	0.00	2	0.6	473	PASS
127	198	10	80	48.2	108736	PASS
197	198	0.00	2	0.8	1755	PASS
198	198	100	100	100.0	225523	PASS
199	198	5	9	6.3	14208	PASS
275	198	10	60	27.7	62507	PASS
365	198	1	100	3.8	8473	PASS
441	198	0.01	100	15.4	34789	PASS
442	442	50	100	100.0	223573	PASS
443	442	15	24	18.4	41160	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP




DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/25/2021	BNA_F	<u>BF123454.D</u>
Compound Name	Response	Retention Time
DDT	581352	13.59
DDD	3118	13.29
DDE	1059	12.96
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4177	585529	0.71

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
 Data File : BF123454.D
 Acq On : 25 Mar 2021 10:50
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 12:34:41 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 24 12:51:15 2021
 Response via : Initial Calibration

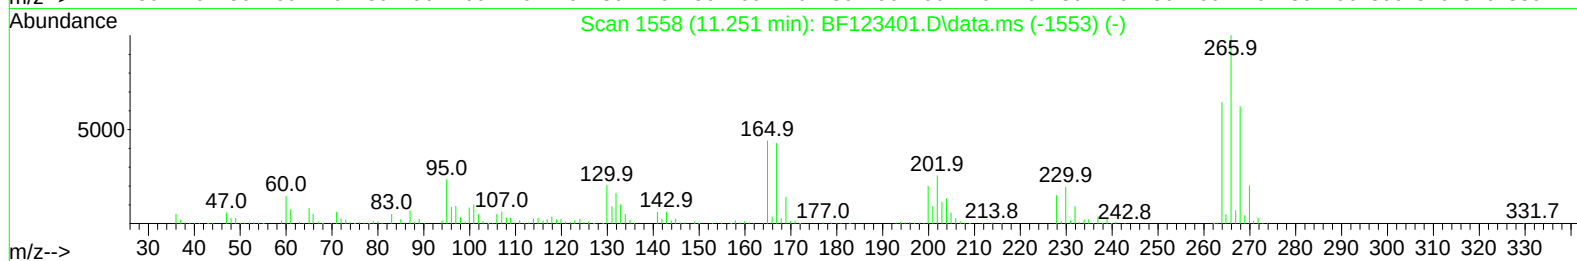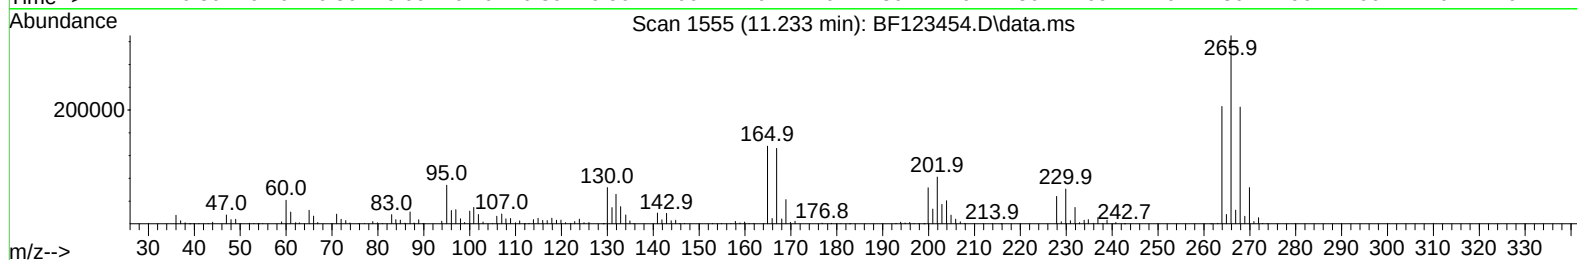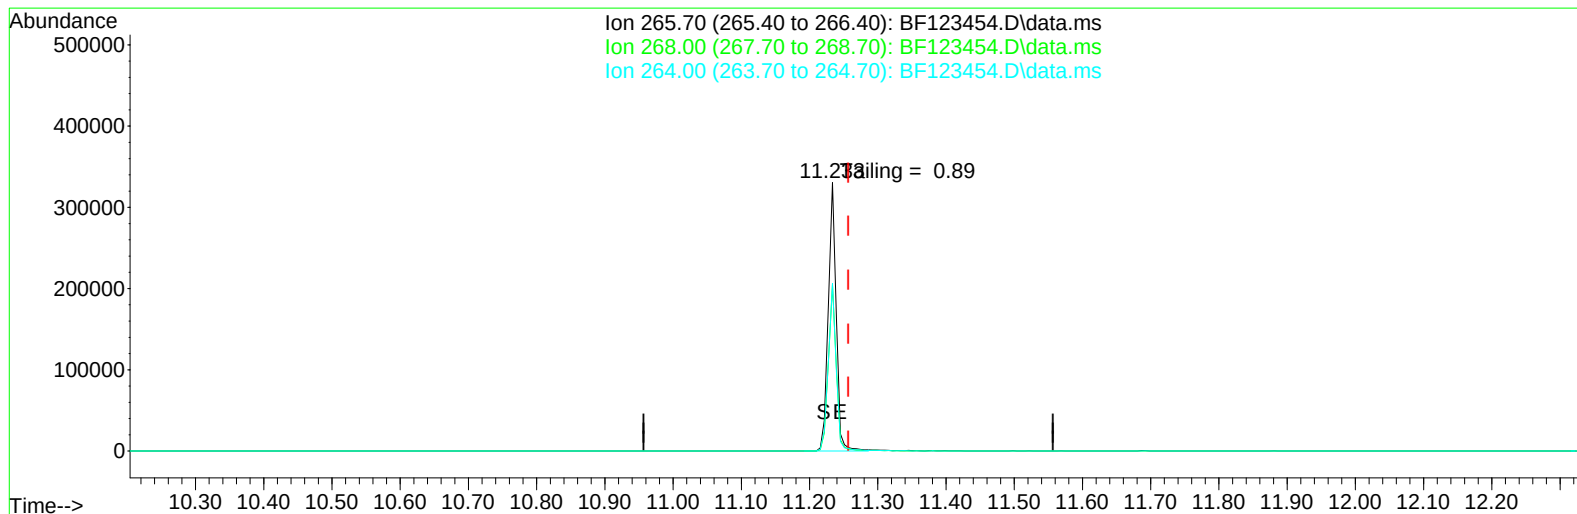

TIC: BF123454.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.023) 46822.46 ng




response 270580

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.10
264.00	62.30	62.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032521\
Data File : BF123454.D
Acq On : 25 Mar 2021 10:50
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 25 12:34:41 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 24 12:51:15 2021
Response via : Initial Calibration

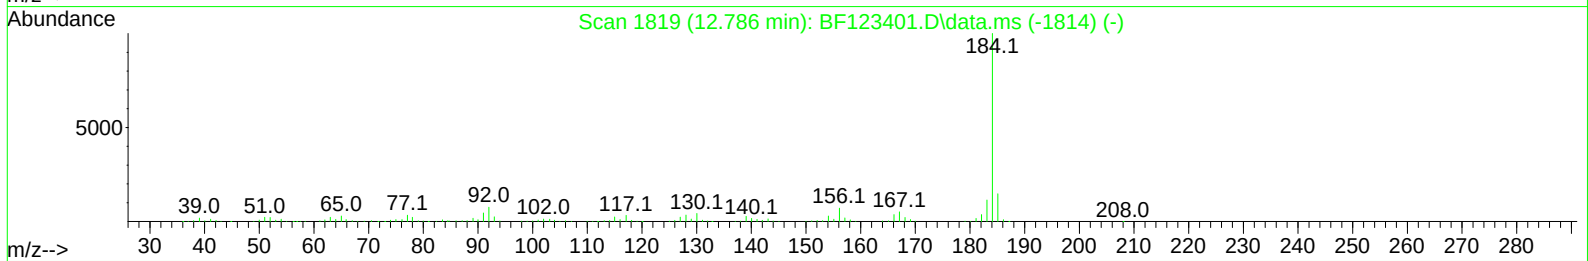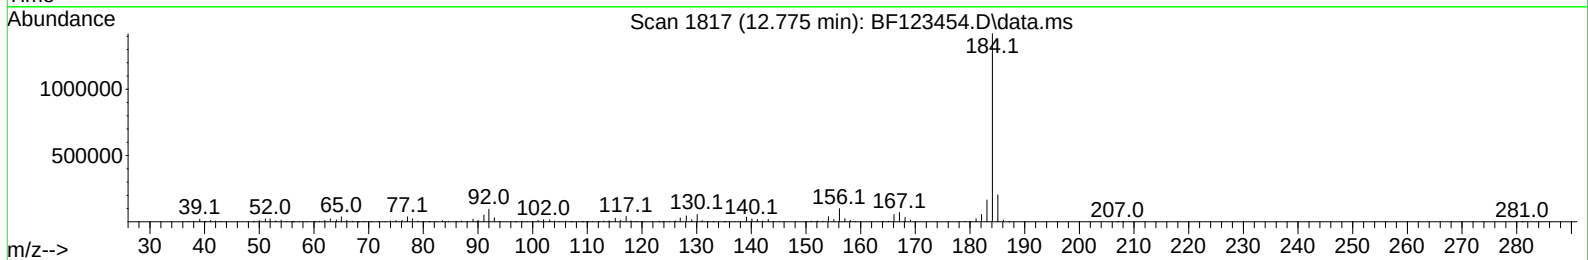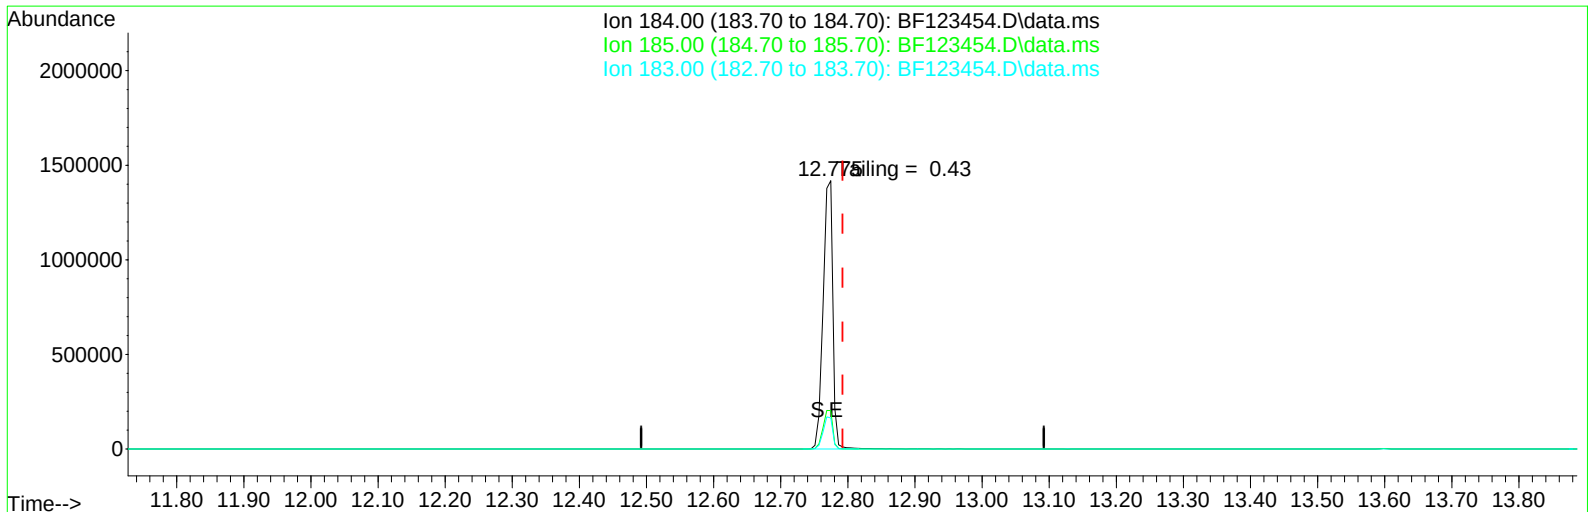

TIC: BF123454.D\data.ms

(77) Benzidine

12.775min (-0.018) 0.00 ng

response 1413711

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.31
183.00	12.10	11.58
0.00	0.00	0.00