

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
 Data File : BF142069.D
 Acq On : 25 Mar 2025 10:39
 Operator : RC/JU
 Sample : PB167274BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167274BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142069.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	12	20	30	rVB	37637	75151	1.00%	0.213%
2	5.498	573	579	585	rBV	2888869	4102818	54.71%	11.638%
3	6.498	742	749	755	rBV	2712198	4044885	53.93%	11.474%
4	6.875	807	813	824	rBV	626618	797954	10.64%	2.263%
5	7.433	901	908	913	rBV	2006096	2814616	37.53%	7.984%
6	8.151	1024	1030	1052	rBV	784617	1092212	14.56%	3.098%
7	9.227	1206	1213	1218	rBV	4480700	5970343	79.61%	16.935%
8	9.910	1323	1329	1343	rBV	995756	1337642	17.84%	3.794%
9	10.698	1457	1463	1492	rBV	3380533	4495717	59.95%	12.752%
10	11.392	1576	1581	1599	rBV	1077392	1467339	19.57%	4.162%
11	12.980	1845	1851	1857	rBV	5556848	7499638	100.00%	21.273%
12	14.033	2024	2030	2042	rBV	655873	924607	12.33%	2.623%
13	15.509	2275	2281	2294	rBV	327347	630888	8.41%	1.790%




Sum of corrected areas: 35253810

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
Data File : BF142069.D
Acq On : 25 Mar 2025 10:39
Operator : RC/JU
Sample : PB167274BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167274BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

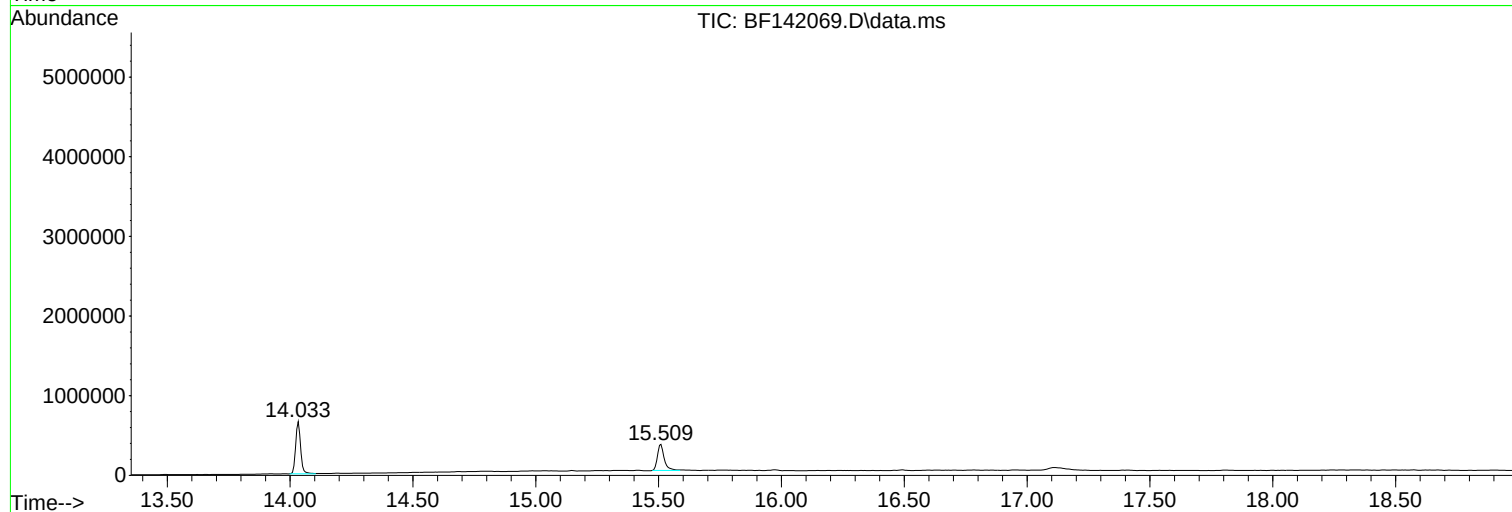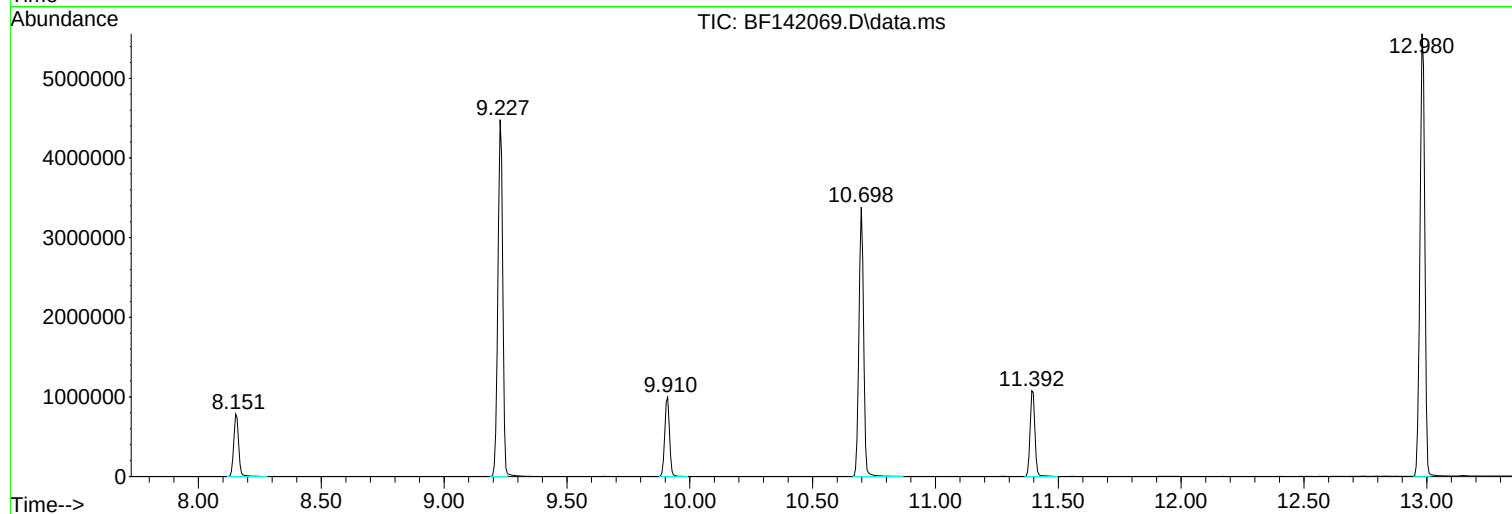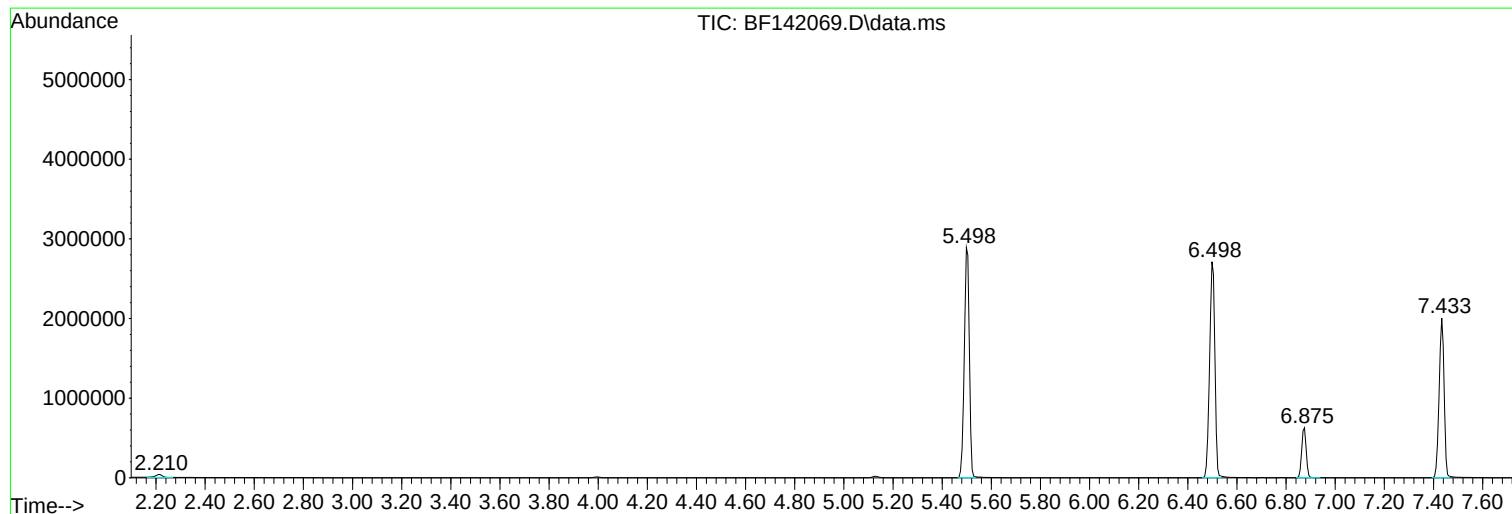

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
Data File : BF142069.D
Acq On : 25 Mar 2025 10:39
Operator : RC/JU
Sample : PB167274BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167274BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032525\
Data File : BF142069.D
Acq On : 25 Mar 2025 10:39
Operator : RC/JU
Sample : PB167274BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167274BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------