


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF032615\  
 Data File : BF078012.D  
 Acq On : 27 Mar 2015 00:14  
 Operator : TP/IZ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF031115.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 27 00:54:57 2015

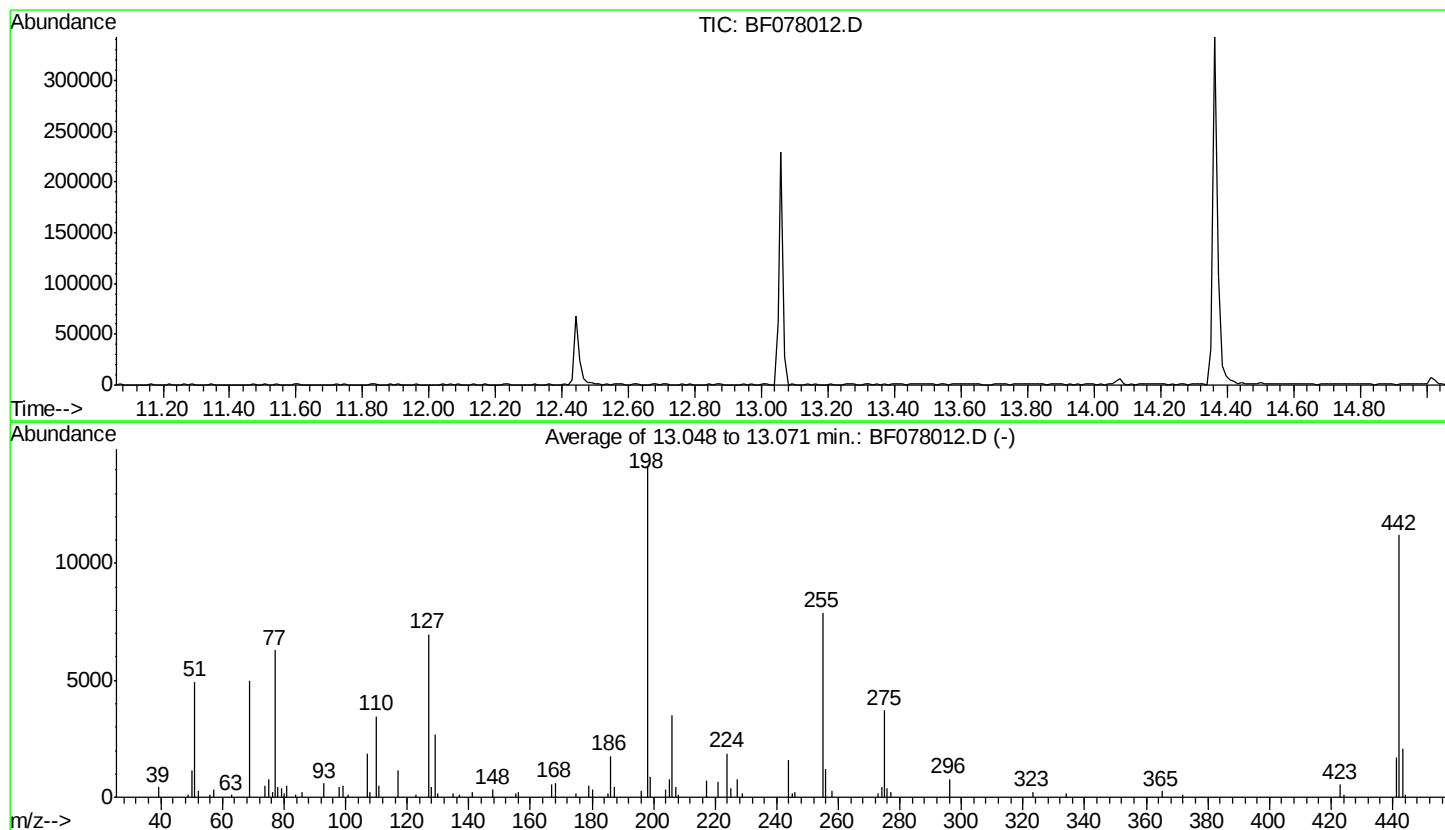

AutoFind: Scans 1064, 1065, 1066; Background Corrected with Scan 1061

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.9      | 4955    | PASS             |
| 68          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 69          | 198          | 0.00         | 100          | 35.1      | 4978    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 49.1      | 6971    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 14187   | PASS             |
| 199         | 198          | 5            | 9            | 6.3       | 893     | PASS             |
| 275         | 198          | 10           | 60           | 26.1      | 3703    | PASS             |
| 365         | 198          | 1            | 100          | 1.8       | 252     | PASS             |
| 441         | 442          | 0.01         | 24           | 15.1      | 1690    | PASS             |
| 442         | 198          | 50           | 100          | 79.0      | 11209   | PASS             |
| 443         | 442          | 15           | 24           | 18.5      | 2077    | PASS             |