

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032615\
 Data File : BF078033.D
 Acq On : 27 Mar 2015 10:46
 Operator : TP/IZ
 Sample : G1642-10
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-15

Quant Time: Mar 27 15:20:50 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 19 02:09:19 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.09	152	39069	20.00	ng	-0.07
21) Naphthalene-d8	8.67	136	159369	20.00	ng	-0.07
38) Acenaphthene-d10	10.84	164	78176	20.00	ng	-0.07
63) Phenanthrene-d10	12.67	188	149700	20.00	ng	-0.08
75) Chrysene-d12	15.95	240	158504	20.00	ng	-0.18
86) Perylene-d12	17.67	264	149304	20.00	ng	-0.43
System Monitoring Compounds						
5) 2-Fluorophenol	5.39	112	150553	67.26	ng	-0.05
7) Phenol-d6	6.69	99	119729	43.30	ng	-0.03
23) Nitrobenzene-d5	7.79	82	245637	101.03	ng	-0.07
41) 2,4,6-Tribromophenol	11.82	330	103721	138.67	ng	-0.07
44) 2-Fluorobiphenyl	10.02	172	526535	98.98	ng	-0.07
78) Terphenyl-d14	14.67	244	564907	87.06	ng	-0.09


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032615\
Data File : BF078033.D
Acq On : 27 Mar 2015 10:46
Operator : TP/IZ
Sample : G1642-10
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-15

Quant Time: Mar 27 15:20:50 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 19 02:09:19 2015
Response via : Initial Calibration

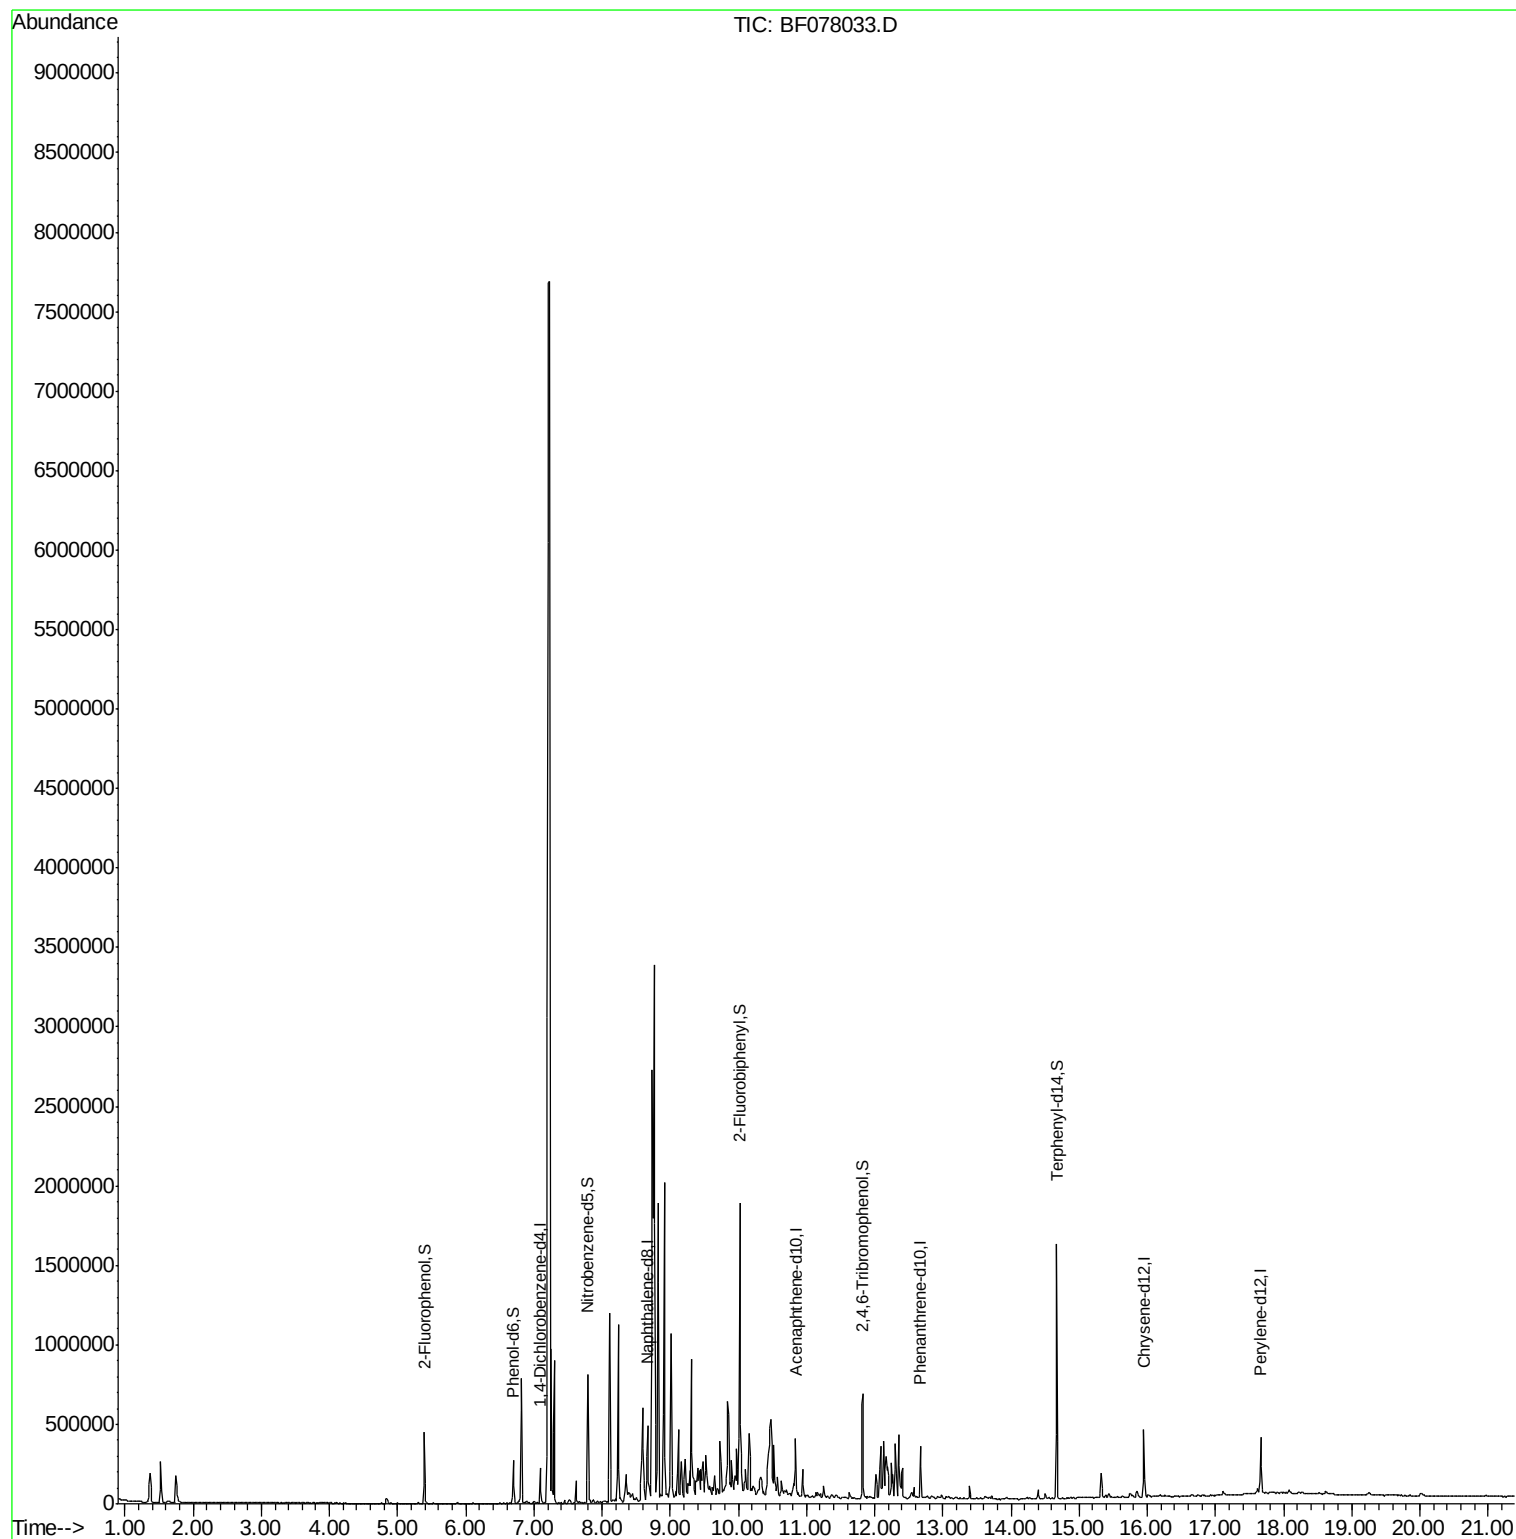

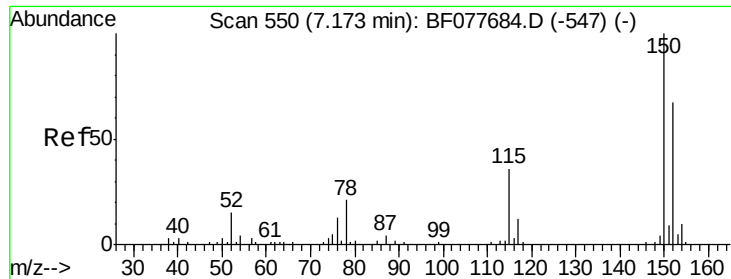


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.09 min Scan# 543
Delta R.T. -0.07 min
Lab File: BF078033.D
Acq: 27 Mar 2015 10:46

Instrument :
BNA_F
ClientSampleId :
MW-15

Tgt Ion:152 Resp: 39069
Ion Ratio Lower Upper
152 100
150 157.9 119.5 179.3
115 60.7 43.0 64.4

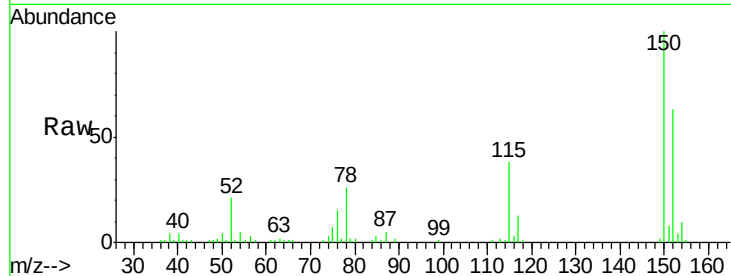


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

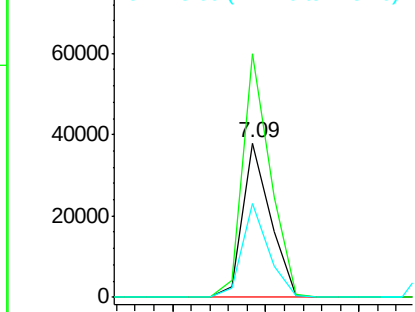



#5


2-Fluorophenol
Concen: 67.26 ng
RT: 5.39 min Scan# 394
Delta R.T. -0.05 min
Lab File: BF078033.D
Acq: 27 Mar 2015 10:46

Tgt Ion:112 Resp: 150553
Ion Ratio Lower Upper
112 100
64 54.5 38.6 57.8
63 27.9 19.3 28.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

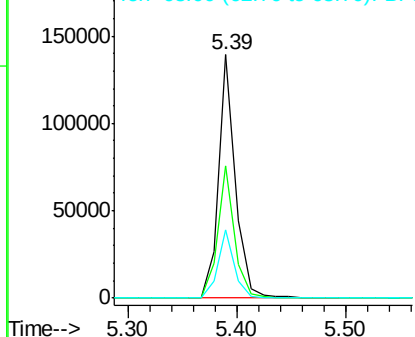

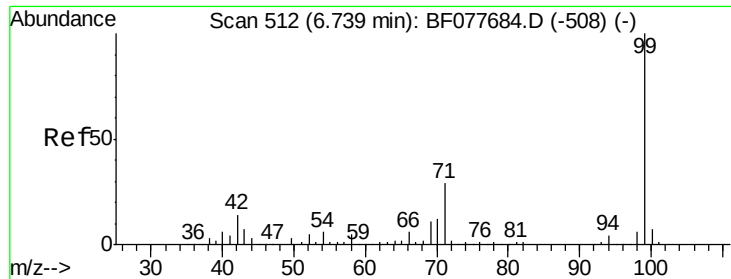

#7

Phenol-d6

Concen: 43.30 ng

RT: 6.69 min Scan# 508

Delta R.T. -0.03 min

Lab File: BF078033.D

Acq: 27 Mar 2015 10:46

Instrument :

BNA_F

ClientSampled :

MW-15


Tgt Ion: 99 Resp: 119729

Ion Ratio Lower Upper

99 100

42 17.6 11.0 16.4#




71 30.7 23.4 35.2



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

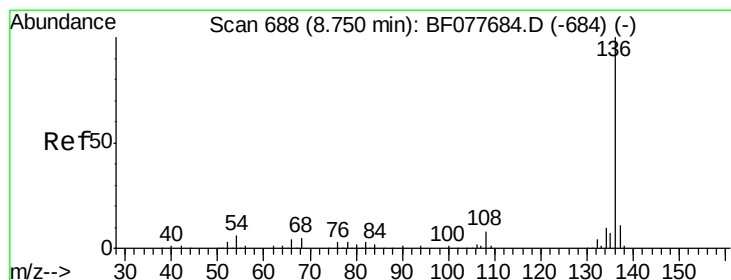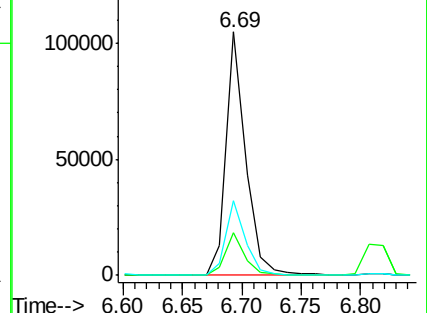

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.67 min Scan# 681

Delta R.T. -0.07 min

Lab File: BF078033.D

Acq: 27 Mar 2015 10:46

Tgt Ion: 136 Resp: 159369


Ion Ratio Lower Upper

136 100

137 11.8 8.7 13.1

54 7.9 4.6 6.8#

68 6.3 3.7 5.5#


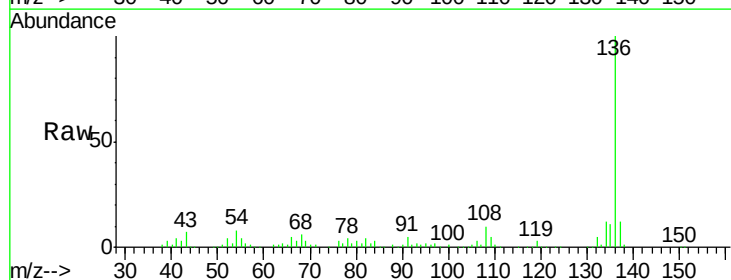



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

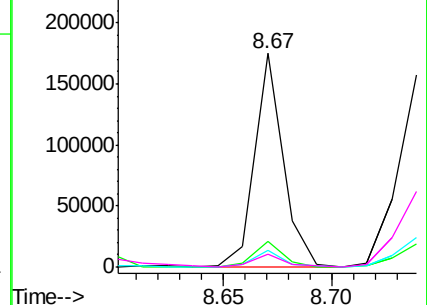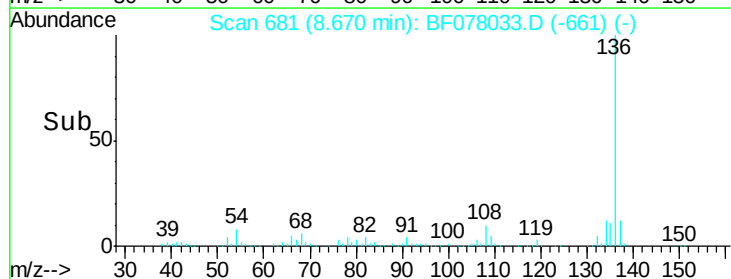


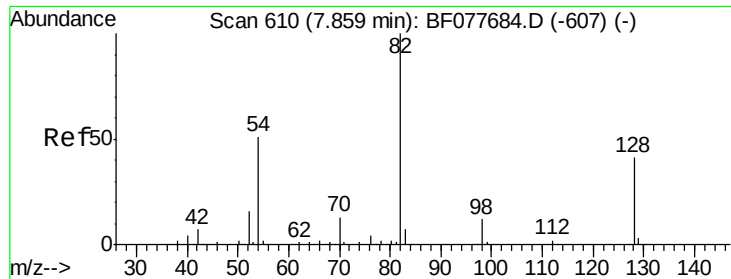




#23
 Nitrobenzene-d5
 Concen: 101.03 ng
 RT: 7.79 min Scan# 604
 Delta R.T. -0.07 min
 Lab File: BF078033.D
 Acq: 27 Mar 2015 10:46

Instrument :
 BNA_F
 ClientSampleId :
 MW-15

Tgt Ion: 82 Resp: 245637
 Ion Ratio Lower Upper
 82 100
 128 42.9 32.8 49.2
 54 50.5 40.6 60.8

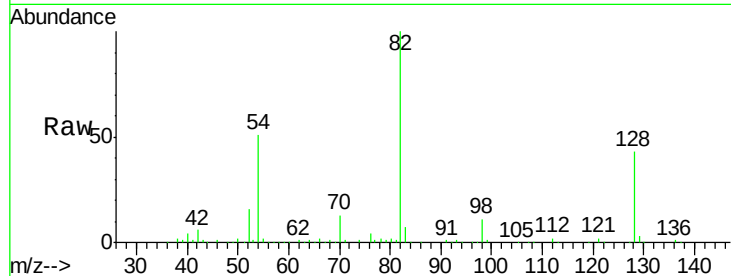


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0


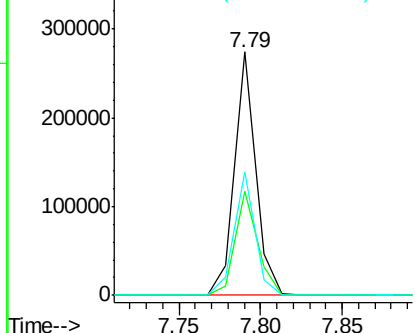



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.84 min Scan# 871
 Delta R.T. -0.07 min
 Lab File: BF078033.D
 Acq: 27 Mar 2015 10:46

Tgt Ion: 164 Resp: 78176
 Ion Ratio Lower Upper
 164 100
 162 103.6 82.4 123.6
 160 44.9 35.8 53.6



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

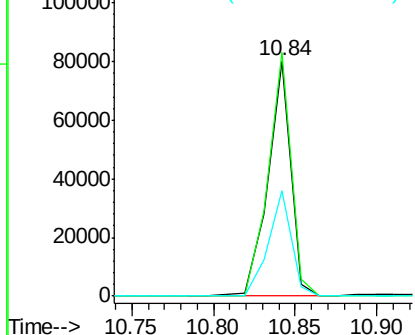


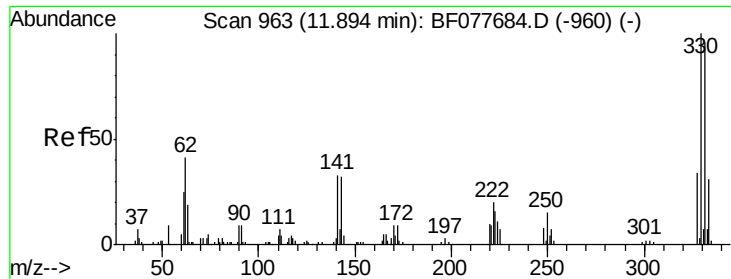




#41
 2,4,6-Tribromophenol
 Concen: 138.67 ng
 RT: 11.82 min Scan# 957
 Delta R.T. -0.07 min
 Lab File: BF078033.D
 Acq: 27 Mar 2015 10:46

Instrument :
 BNA_F
 ClientSampleId :
 MW-15

Tgt Ion	Ratio	Lower	Upper
330	100		
332	97.0	0.0	0.0#
141	36.7	0.0	0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


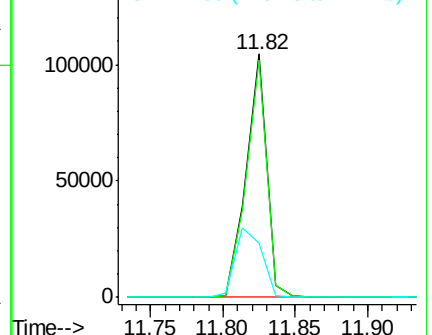



#44
 2-Fluorobiphenyl
 Concen: 98.98 ng
 RT: 10.02 min Scan# 799
 Delta R.T. -0.07 min
 Lab File: BF078033.D
 Acq: 27 Mar 2015 10:46

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.0	28.5	42.7
170	23.7	18.8	28.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



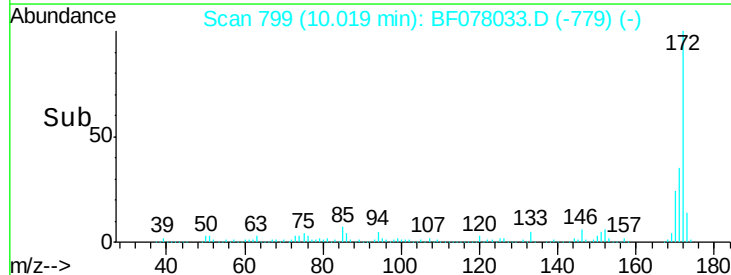
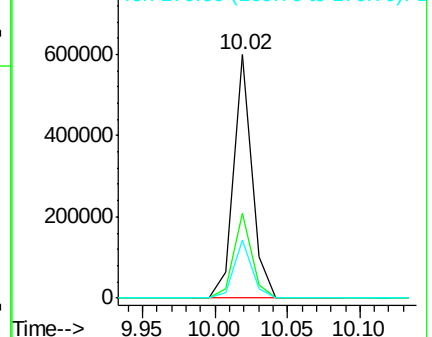


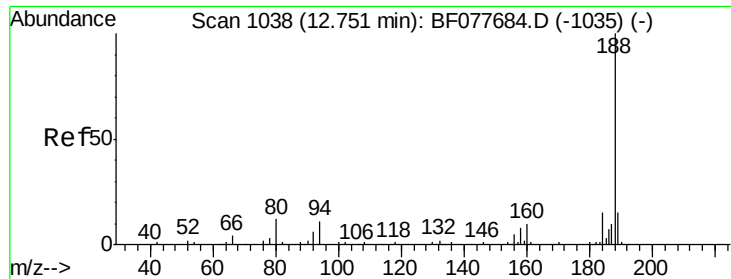

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.67 min Scan# 1031
Delta R.T. -0.08 min
Lab File: BF078033.D
Acq: 27 Mar 2015 10:46




Instrument :
BNA_F
ClientSampleId :
MW-15


Tgt Ion:188 Resp: 149700
Ion Ratio Lower Upper
188 100
94 12.2 8.7 13.1
80 12.8 9.3 13.9

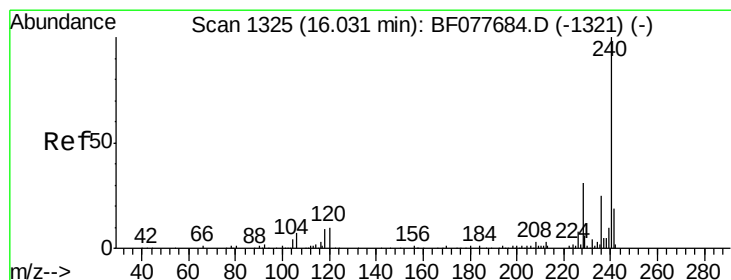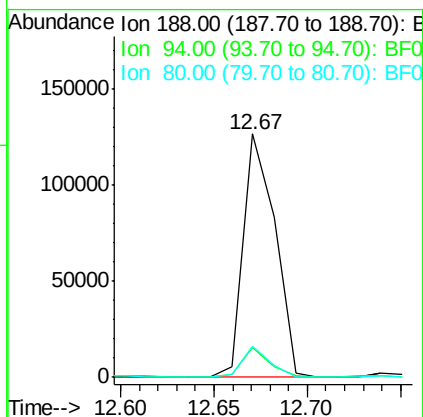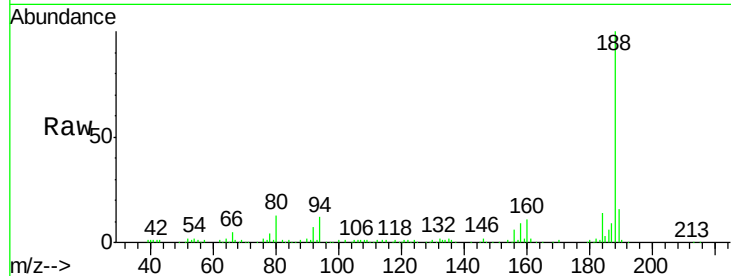

#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.95 min Scan# 1318
Delta R.T. -0.18 min
Lab File: BF078033.D
Acq: 27 Mar 2015 10:46

Tgt Ion:240 Resp: 158504
Ion Ratio Lower Upper
240 100
120 12.0 8.2 12.2
236 25.7 20.0 30.0



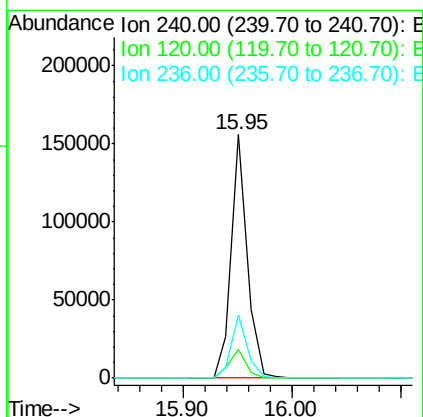





#78
 Terphenyl-d14
 Concen: 87.06 ng
 RT: 14.67 min Scan# 1206
 Delta R.T. -0.09 min
 Lab File: BF078033.D
 Acq: 27 Mar 2015 10:46

Instrument :
 BNA_F
 ClientSampleId :
 MW-15

Tgt Ion:244 Resp: 564907
 Ion Ratio Lower Upper
 244 100
 212 6.8 4.9 7.3
 122 13.0 6.2 9.4#

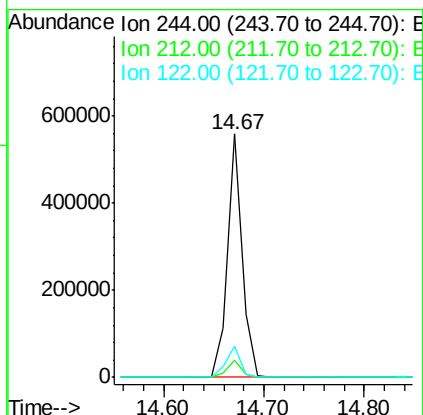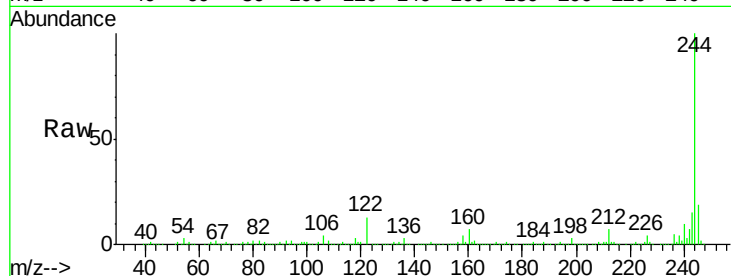

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.67 min Scan# 1468
 Delta R.T. -0.43 min
 Lab File: BF078033.D
 Acq: 27 Mar 2015 10:46

Tgt Ion:264 Resp: 149304
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.6 27.8
 265 22.7 17.3 25.9

