


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032615\
 Data File : BF077991.D
 Acq On : 26 Mar 2015 12:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 02:09:19 2015

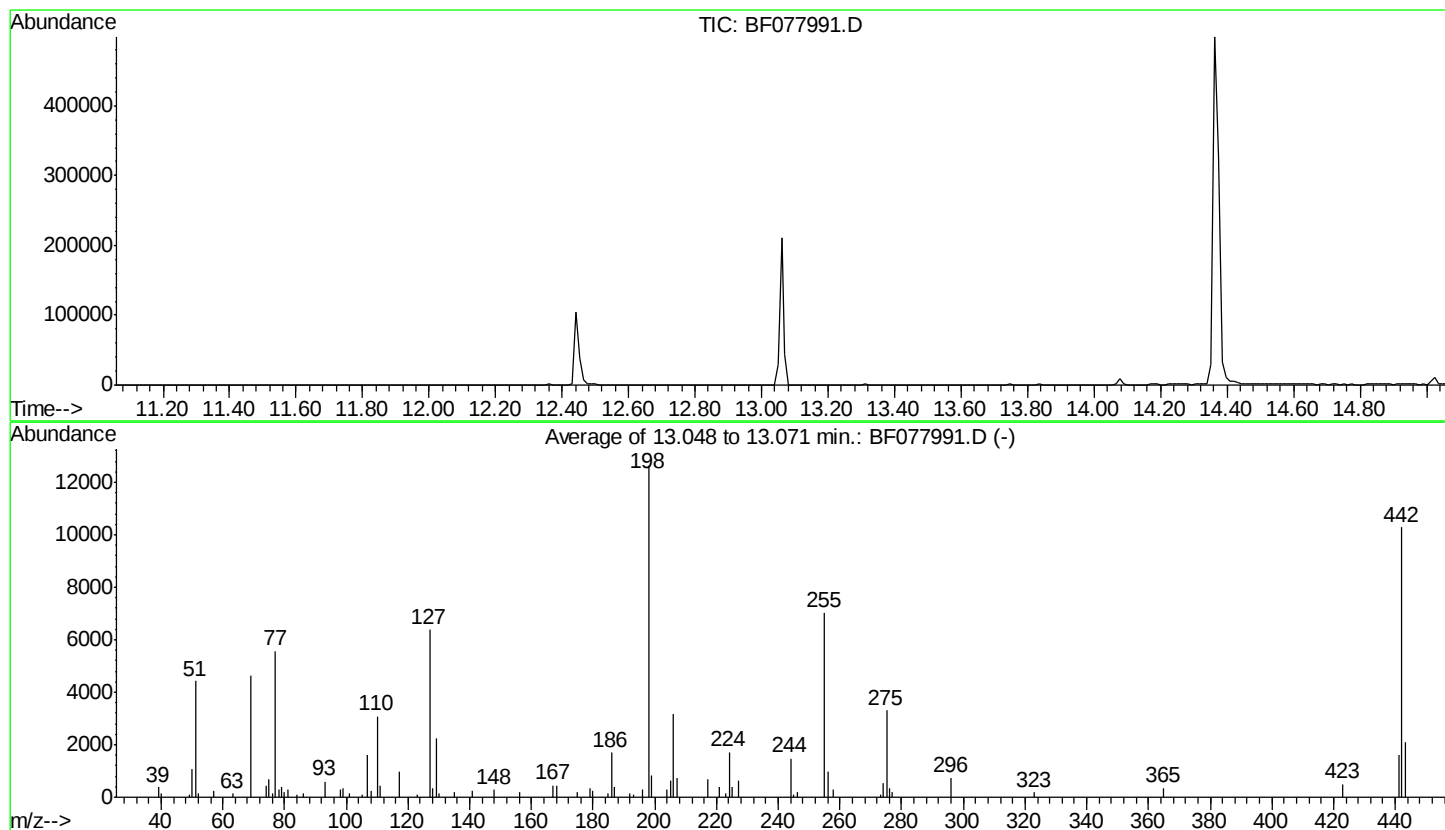

AutoFind: Scans 1064, 1065, 1066; Background Corrected with Scan 1061

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	4425	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.8	4645	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.4	6372	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12639	PASS
199	198	5	9	6.6	831	PASS
275	198	10	60	26.1	3304	PASS
365	198	1	100	2.8	348	PASS
441	442	0.01	24	15.9	1635	PASS
442	198	50	100	81.3	10274	PASS
443	442	15	24	20.3	2087	PASS