


Data Path : Z:\HPCHEM1\BNA F\Data\BF032618\
Data File : BF103912.D
Acq On : 26 Mar 2018 8:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Mar 23 13:26:17 2018

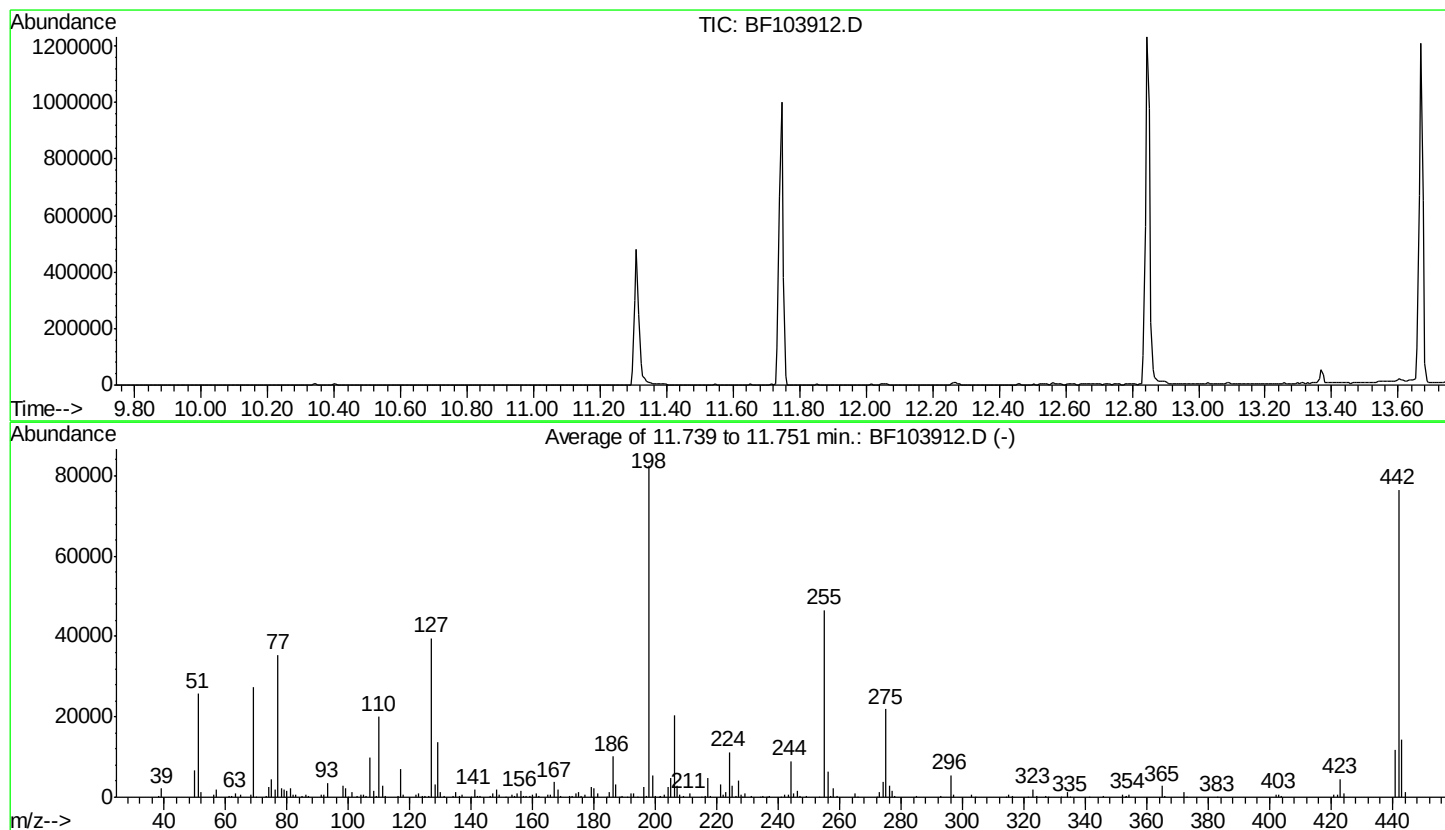

AutoFind: Scans 1641, 1642, 1643; Background Corrected with Scan 1636

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.1	25678	PASS
68	69	0.00	2	2.0	552	PASS
69	198	0.00	100	33.4	27532	PASS
70	69	0.00	2	0.4	111	PASS
127	198	10	80	48.0	39644	PASS
197	198	0.00	2	0.4	355	PASS
198	198	100	100	100.0	82512	PASS
199	198	5	9	6.7	5502	PASS
275	198	10	60	26.5	21838	PASS
365	198	1	100	3.4	2809	PASS
441	443	0.01	100	83.0	11884	PASS
442	198	50	100	92.7	76509	PASS
443	442	15	24	18.7	14312	PASS