
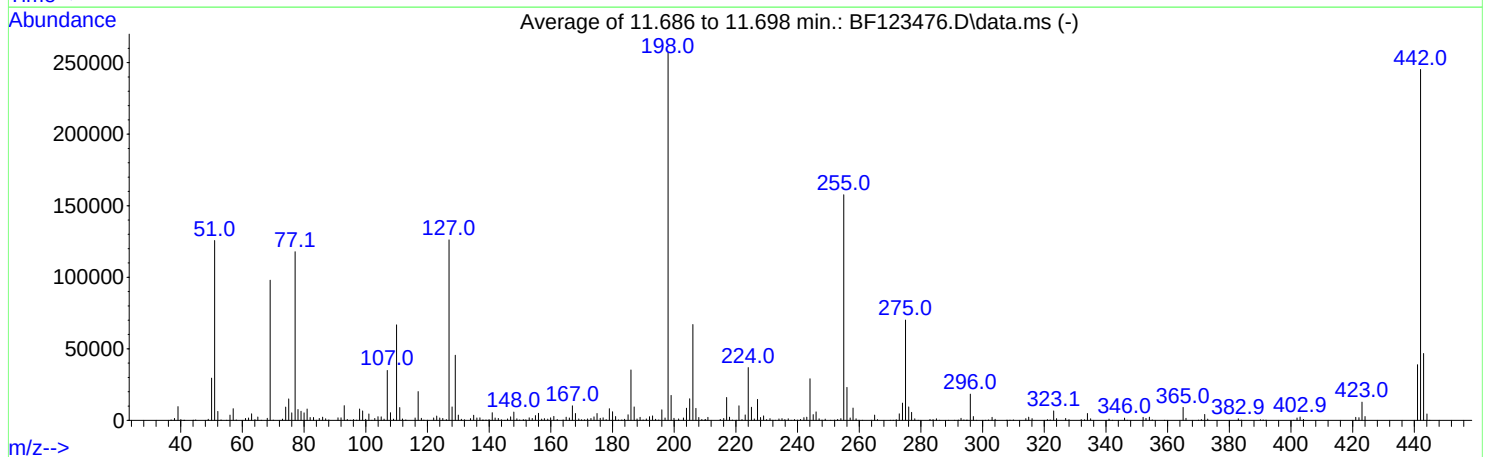


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032621\
 Data File : BF123476.D
 Acq On : 26 Mar 2021 9:16
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 26 12:51:59 2021

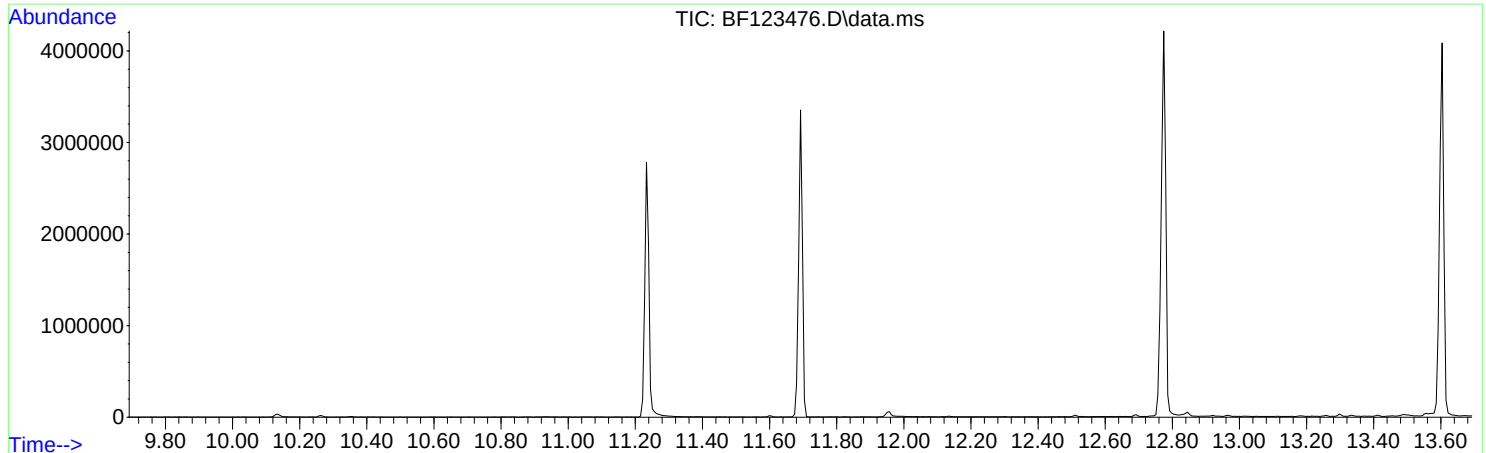




AutoFind: Scans 1632, 1633, 1634; Background Corrected with Scan 1627

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	125693	PASS
68	69	0.00	2	1.5	1492	PASS
69	198	0.00	100	38.1	97933	PASS
70	69	0.00	2	0.3	283	PASS
127	198	10	80	49.1	126157	PASS
197	198	0.00	2	0.7	1679	PASS
198	198	100	100	100.0	257088	PASS
199	198	5	9	6.8	17414	PASS
275	198	10	60	27.3	70147	PASS
365	198	1	100	3.5	9046	PASS
441	198	0.01	100	15.1	38923	PASS
442	442	50	100	100.0	245245	PASS
443	442	15	24	19.1	46723	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032621\
Data File : BF123476.D
Acq On : 26 Mar 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 26 12:47:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 17:06:59 2021
Response via : Initial Calibration

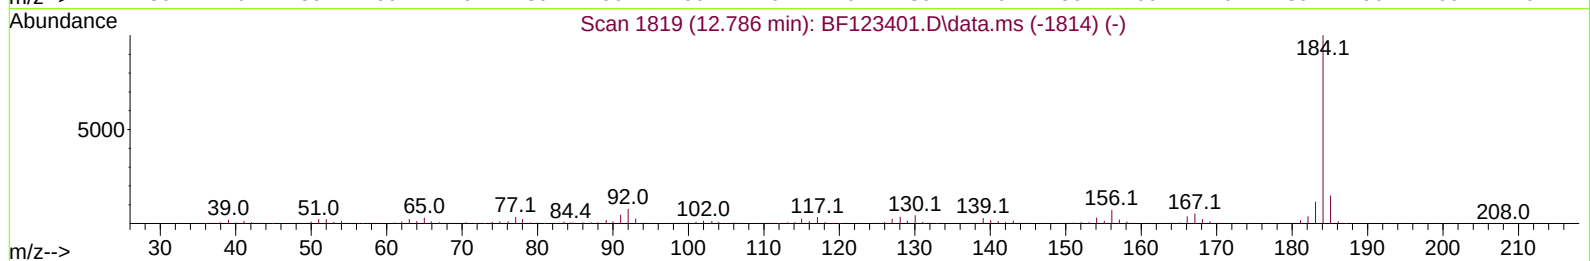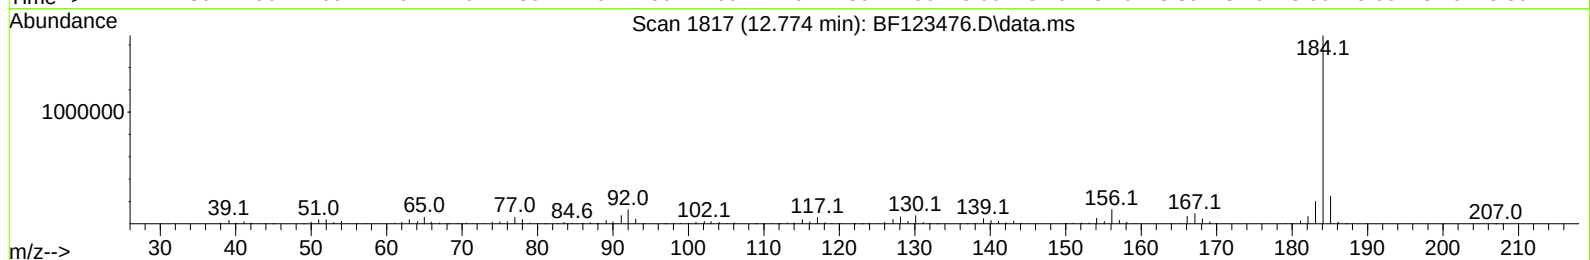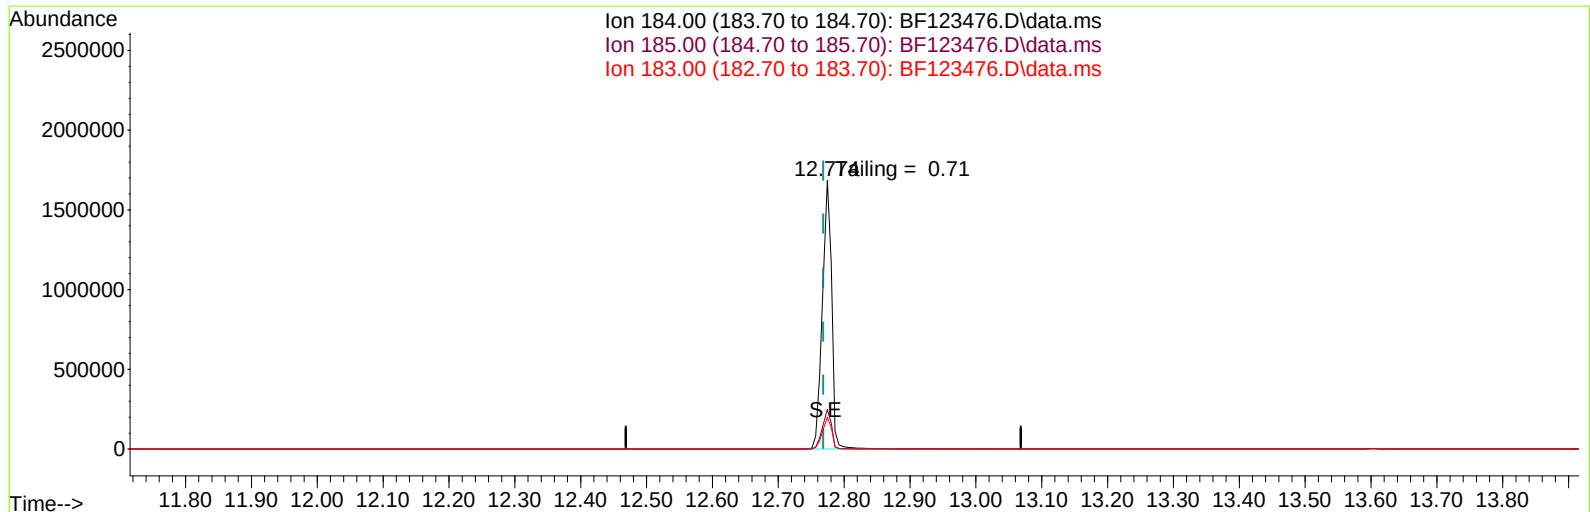

TIC: BF123476.D\data.ms

(77) Benzidine

12.774min (+ 0.006) 0.00 ng




response 1664557

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.72
183.00	12.10	11.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032621\
Data File : BF123476.D
Acq On : 26 Mar 2021 9:16
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 26 12:47:45 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 17:06:59 2021
Response via : Initial Calibration

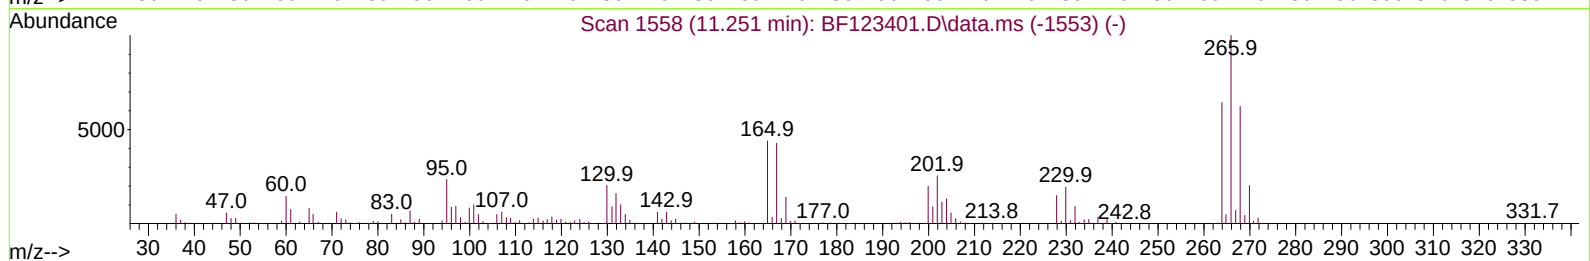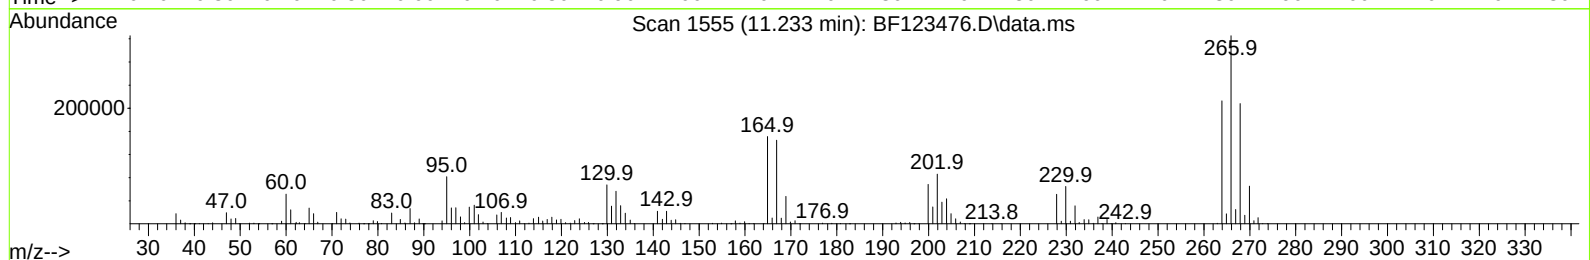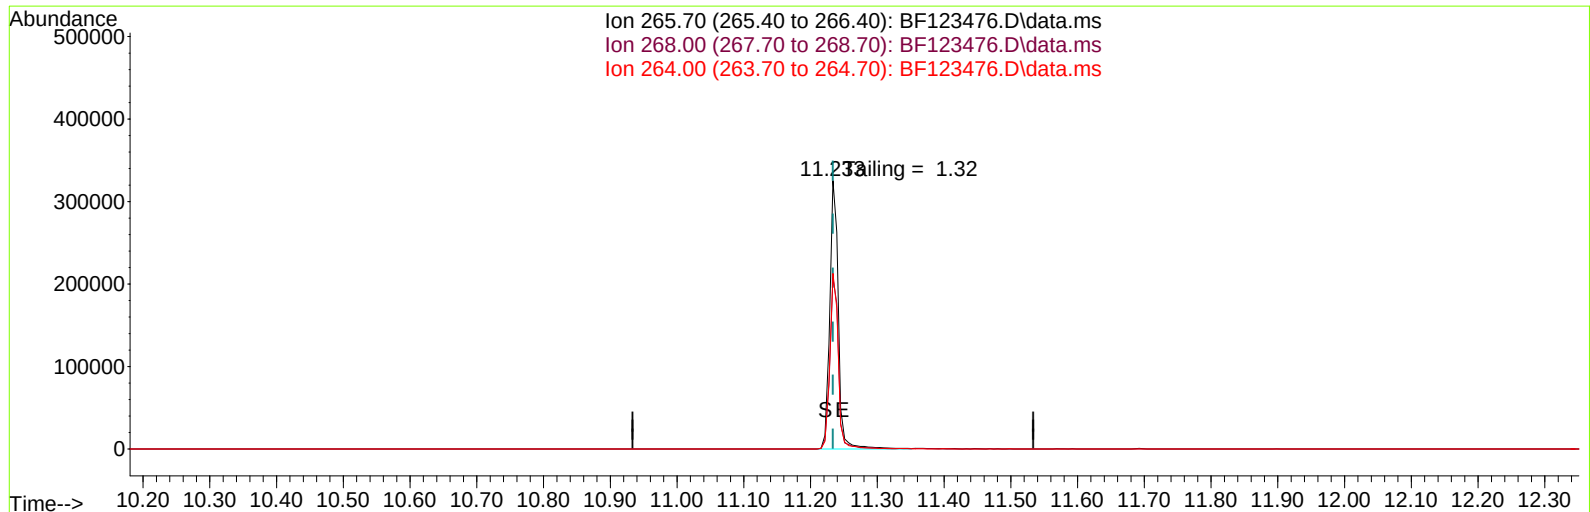

TIC: BF123476.D\data.ms

(70) Pentachlorophenol (C)

11.233min (-0.000) 36040.21 ng

response 293881

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.93
264.00	62.30	65.40
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/26/2021	BNA_F	<u>BF123476.D</u>
Compound Name	Response	Retention Time
DDT	699675	13.604
DDD	6892	13.298
DDE	2197	12.963
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9089	708764	1.28