

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032625\
 Data File : BF142105.D
 Acq On : 26 Mar 2025 19:09
 Operator : RC/JU
 Sample : Q1636-05
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-2

Quant Time: Mar 27 01:04:20 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 10 15:46:22 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.869	152	124569	20.000	ng	-0.01
21) Naphthalene-d8	8.151	136	488974	20.000	ng	-0.01
39) Acenaphthene-d10	9.904	164	278444	20.000	ng	-0.01
64) Phenanthrene-d10	11.392	188	523529	20.000	ng	-0.01
76) Chrysene-d12	14.033	240	405207	20.000	ng	0.00
86) Perylene-d12	15.504	264	343378	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.487	112	634471	85.006	ng	0.00
7) Phenol-d6	6.493	99	786157	82.726	ng	-0.01
23) Nitrobenzene-d5	7.428	82	515931	59.378	ng	-0.02
42) 2,4,6-Tribromophenol	10.692	330	313255	88.680	ng	-0.01
45) 2-Fluorobiphenyl	9.228	172	1027209	56.104	ng	-0.01
79) Terphenyl-d14	12.980	244	1319200	48.133	ng	0.00
Target Compounds						Qvalue
19) n-Nitroso-di-n-propyla...	7.428	70	68408	11.203	ng	# 77
25) Isophorone	7.428	82	507830	33.064	ng	# 64
51) 2,6-Dinitrotoluene	9.904	165	35184	8.666	ng	# 23
57) 2,4-Dinitrotoluene	9.904	165	35184	6.635	ng	# 24
63) Azobenzene	10.616	77	49448	2.736	ng	# 1
67) 4-Bromophenyl-phenylether	10.692	248	19990	3.040	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032625\
Data File : BF142105.D
Acq On : 26 Mar 2025 19:09
Operator : RC/JU
Sample : Q1636-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-2


Quant Time: Mar 27 01:04:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

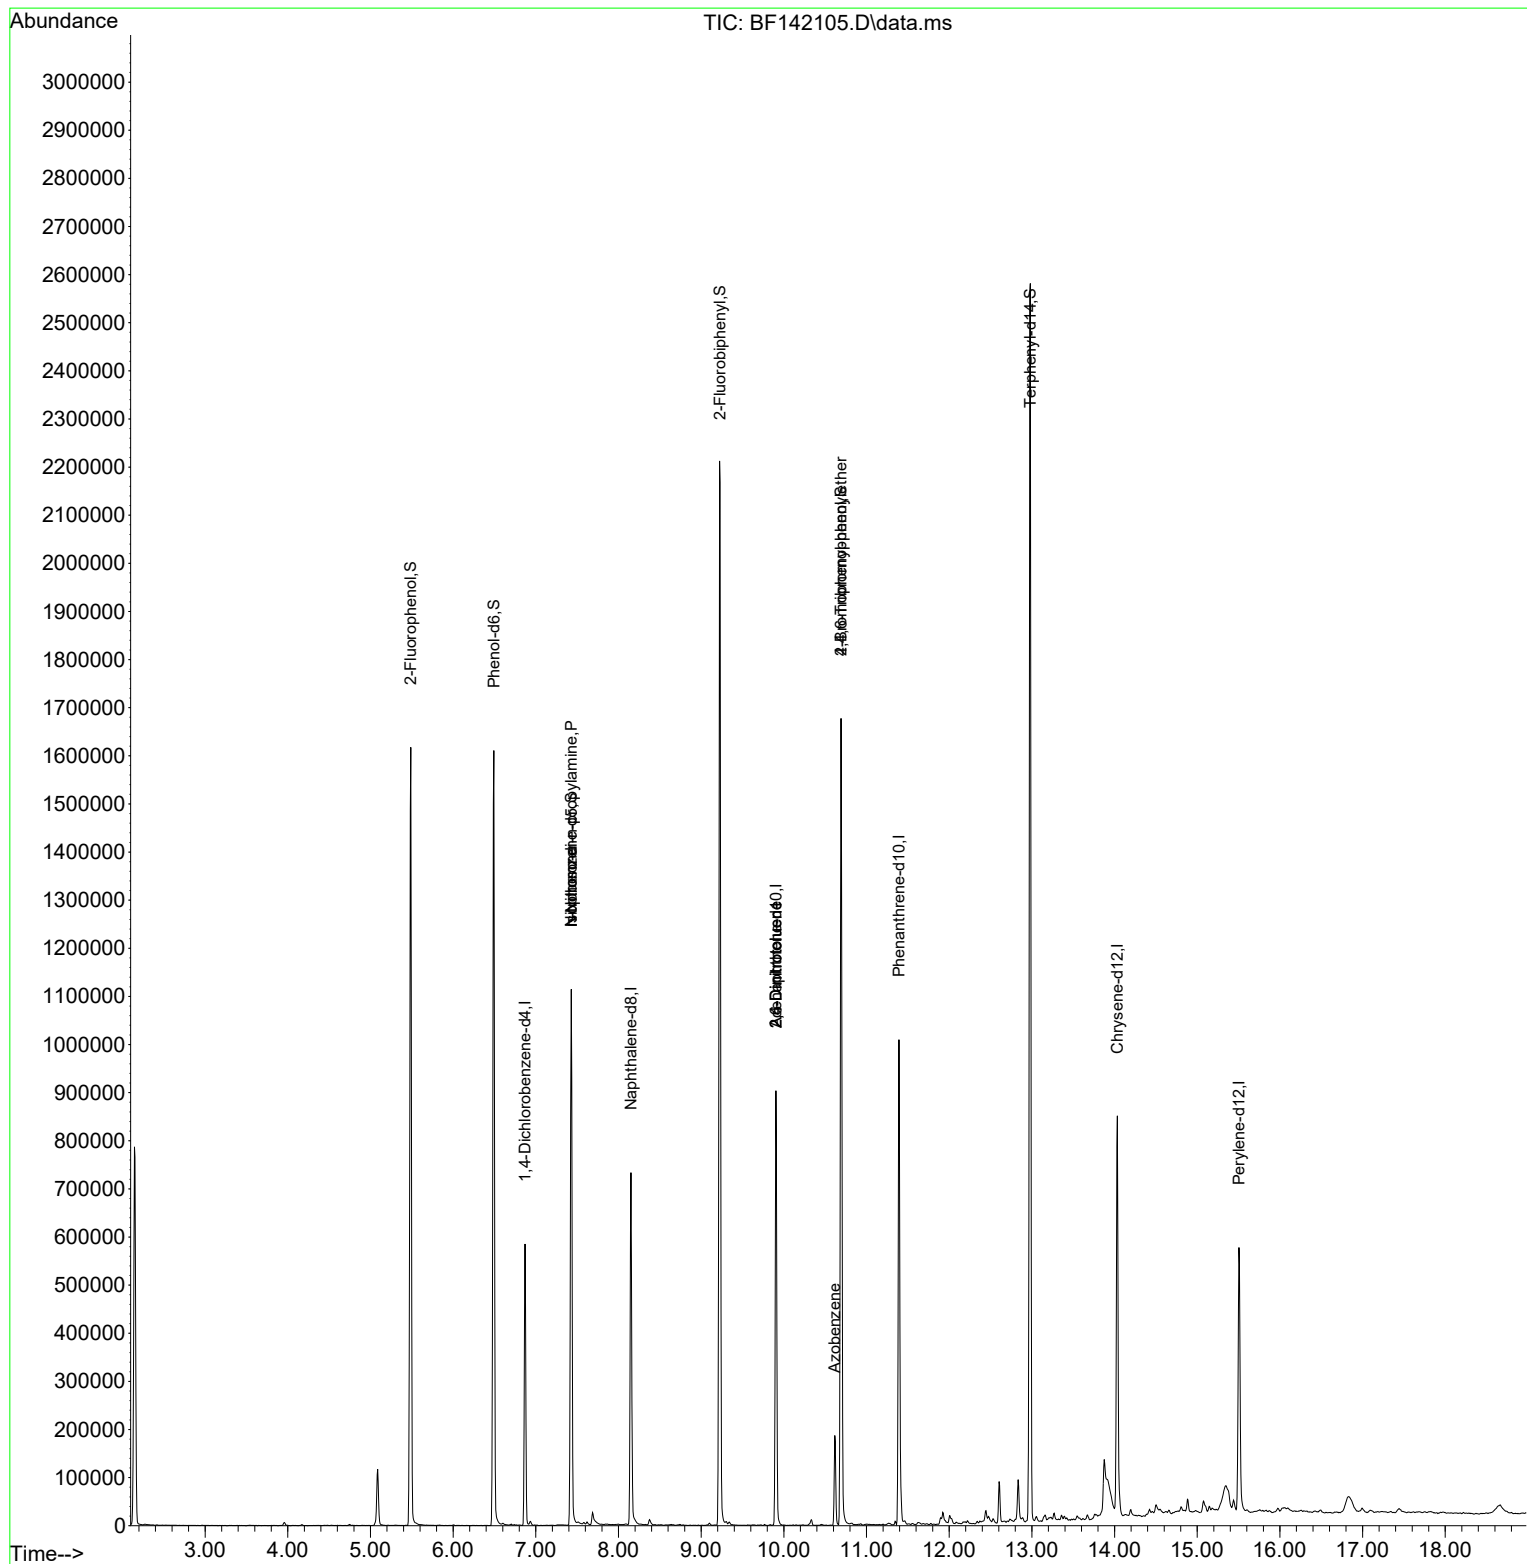






#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.869 min Scan# 814
Delta R.T. -0.012 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Instrument :
BNA_F
ClientSampleId :
WC-2



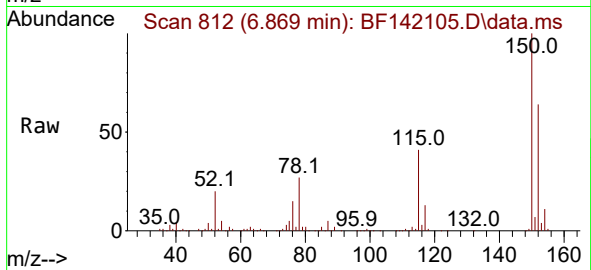



Tgt Ion:152 Resp: 124569
Ion Ratio Lower Upper
152 100
150 155.3 127.4 191.2
115 64.4 51.9 77.9

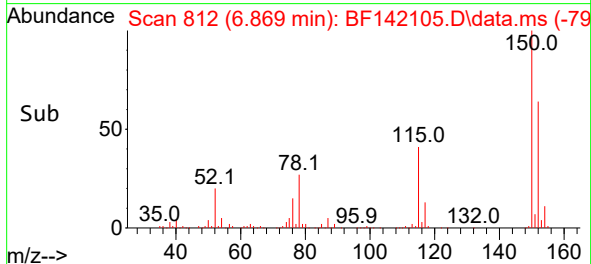

#5
2-Fluorophenol
Concen: 85.006 ng
RT: 5.487 min Scan# 577
Delta R.T. -0.006 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion:112 Resp: 634471
Ion Ratio Lower Upper
112 100
64 55.1 46.5 69.7
63 30.2 25.4 38.2


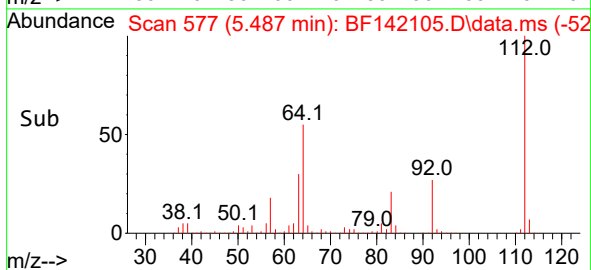

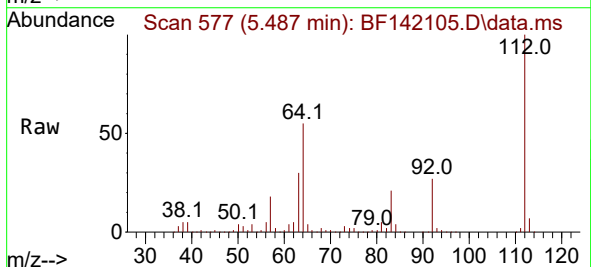


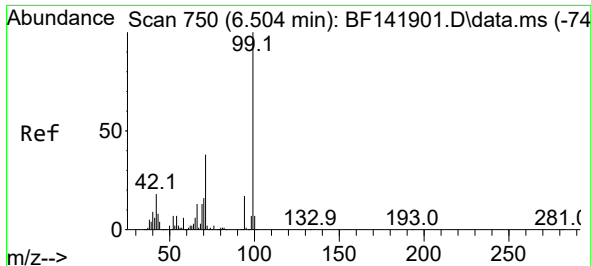

#7
Phenol-d6
Concen: 82.726 ng
RT: 6.493 min Scan# 74
Delta R.T. -0.012 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09




Instrument :
BNA_F
ClientSampleId :
WC-2


Tgt Ion: 99 Resp: 786157
Ion Ratio Lower Upper
99 100
42 16.8 14.6 21.8
71 38.0 30.8 46.2

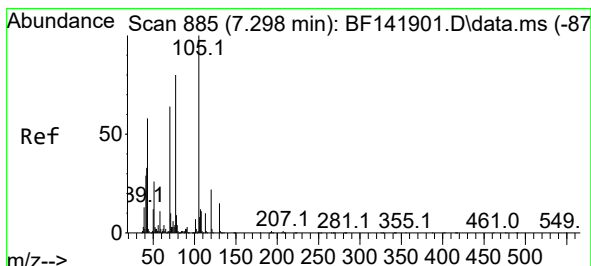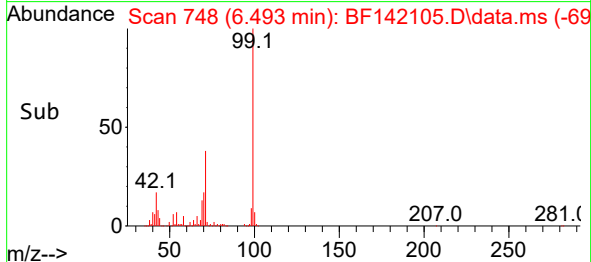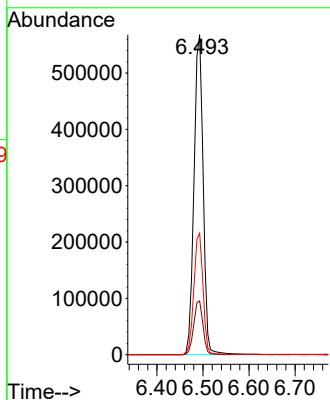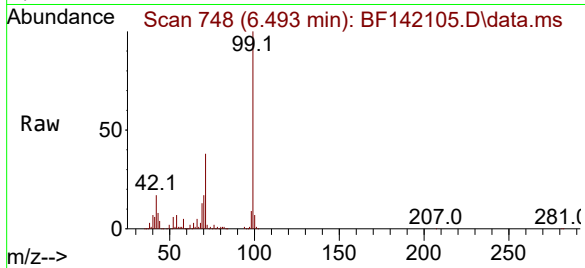

#19
n-Nitroso-di-n-propylamine
Concen: 11.203 ng
RT: 7.428 min Scan# 907
Delta R.T. 0.130 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion: 70 Resp: 68408
Ion Ratio Lower Upper
70 100
42 42.3 41.4 62.0
101 0.0 8.2 12.2#
130 2.3 18.2 27.4#


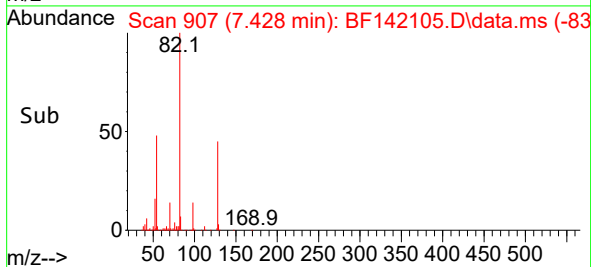
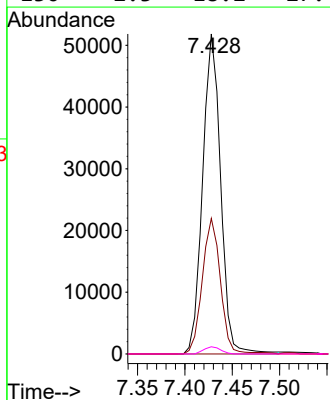
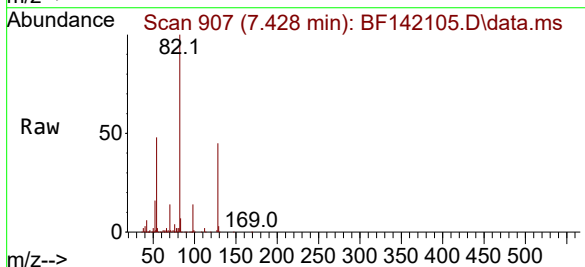


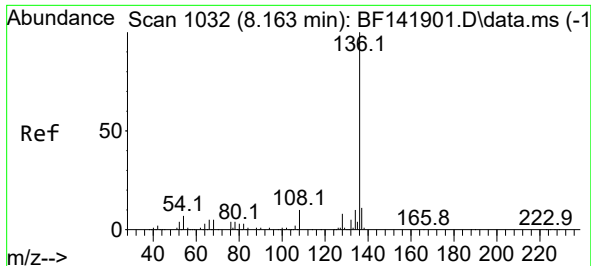

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.151 min Scan# 1030
Delta R.T. -0.012 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09




Instrument :
BNA_F
ClientSampleId :
WC-2


Tgt Ion:136 Resp: 488974
Ion Ratio Lower Upper
136 100
137 10.9 8.8 13.2
54 6.4 5.8 8.8
68 4.7 4.1 6.1

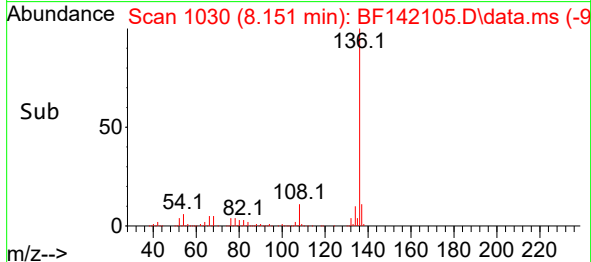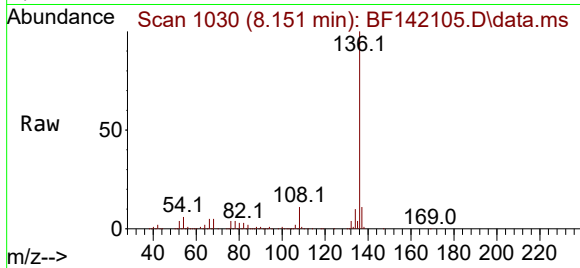

#23
Nitrobenzene-d5
Concen: 59.378 ng
RT: 7.428 min Scan# 907
Delta R.T. -0.017 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion: 82 Resp: 515931
Ion Ratio Lower Upper
82 100
128 45.2 36.0 54.0
54 47.9 39.6 59.4


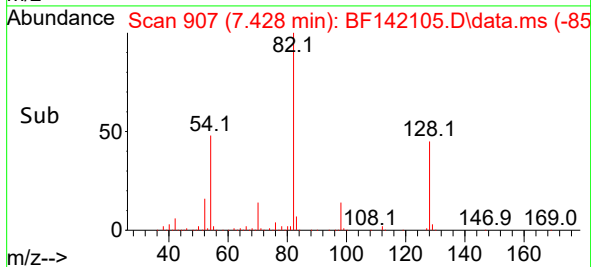

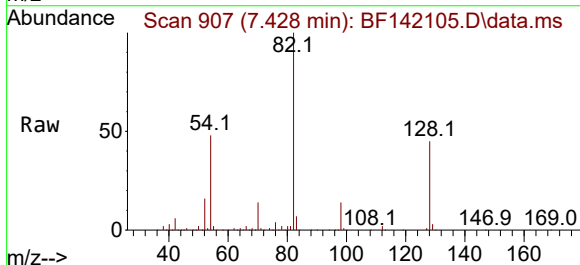


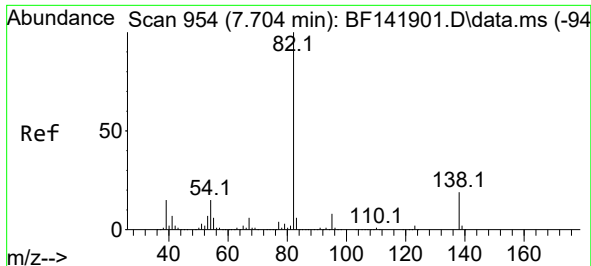

#25
Isophorone
Concen: 33.064 ng
RT: 7.428 min Scan# 90
Delta R.T. -0.276 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09




Instrument :
BNA_F
ClientSampleId :
WC-2


Tgt Ion: 82 Resp: 507830
Ion Ratio Lower Upper
82 100
95 0.0 6.4 9.6#
138 0.0 14.9 22.3#

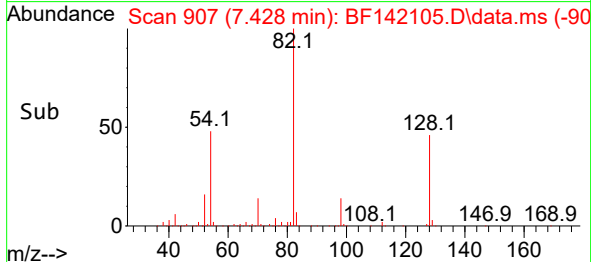

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.904 min Scan# 1328
Delta R.T. -0.012 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion:164 Resp: 278444
Ion Ratio Lower Upper
164 100
162 103.2 81.8 122.6
160 45.0 36.7 55.1


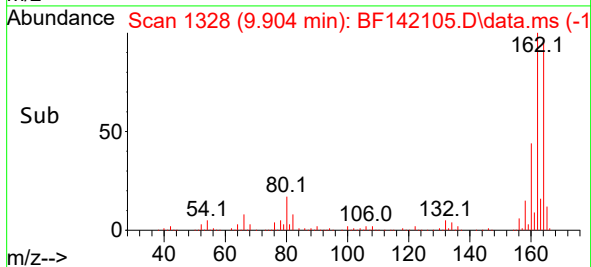

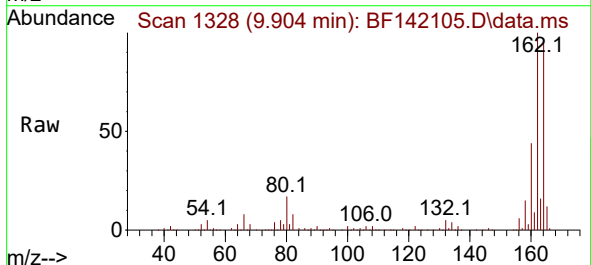




#42
 2,4,6-Tribromophenol
 Concen: 88.680 ng
 RT: 10.692 min Scan# 1462
 Delta R.T. -0.012 min
 Lab File: BF142105.D
 Acq: 26 Mar 2025 19:09




Instrument :
 BNA_F
 ClientSampleId :
 WC-2


Tgt Ion:330 Resp: 313255
 Ion Ratio Lower Upper
 330 100
 332 98.1 77.6 116.4
 141 29.8 24.7 37.1

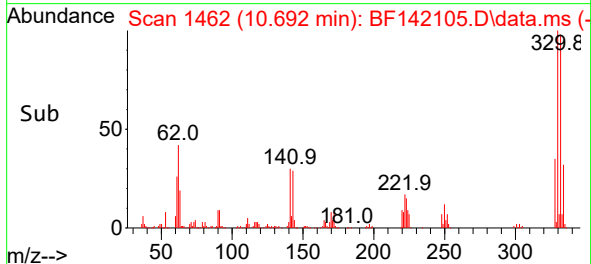

#45
 2-Fluorobiphenyl
 Concen: 56.104 ng
 RT: 9.228 min Scan# 1213
 Delta R.T. -0.012 min
 Lab File: BF142105.D
 Acq: 26 Mar 2025 19:09

Tgt Ion:172 Resp: 1027209
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.3 43.9
 170 23.4 19.4 29.0


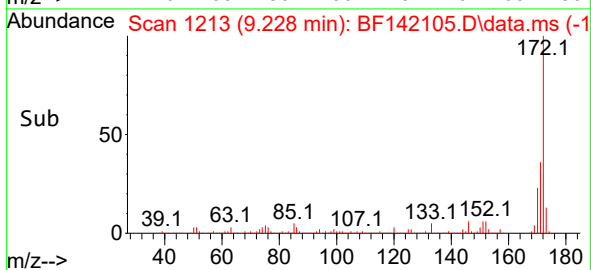

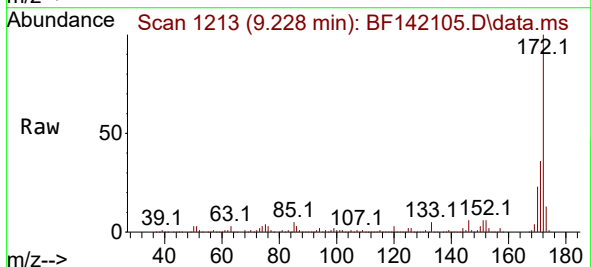


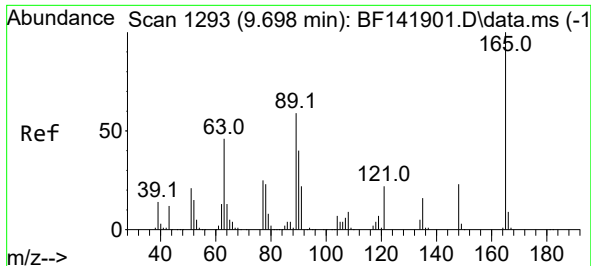

#51
2,6-Dinitrotoluene
Concen: 8.666 ng
RT: 9.904 min Scan# 11
Delta R.T. 0.206 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09




Instrument :
BNA_F
ClientSampleId :
WC-2


Tgt Ion:165 Resp: 35184
Ion Ratio Lower Upper
165 100
63 1.3 47.0 70.4#
89 1.3 47.4 71.2#

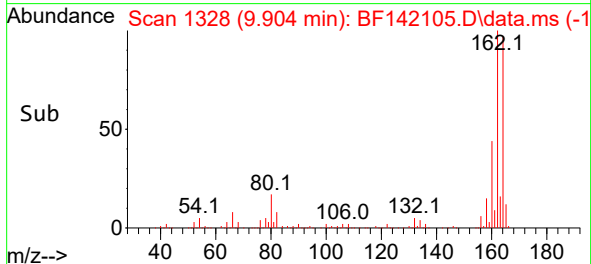

#57
2,4-Dinitrotoluene
Concen: 6.635 ng
RT: 9.904 min Scan# 1328
Delta R.T. -0.200 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion:165 Resp: 35184
Ion Ratio Lower Upper
165 100
63 1.3 35.4 53.2#
89 1.3 56.6 84.8#
182 0.0 2.2 3.4#



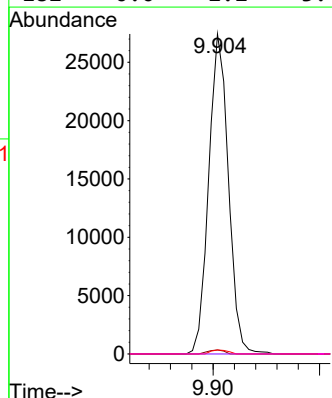
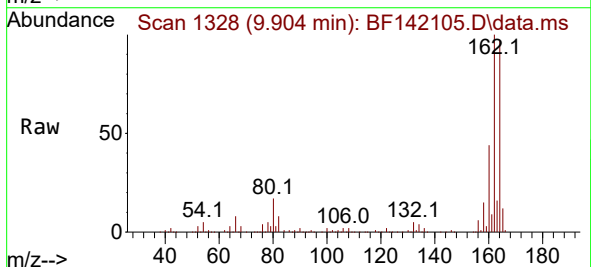


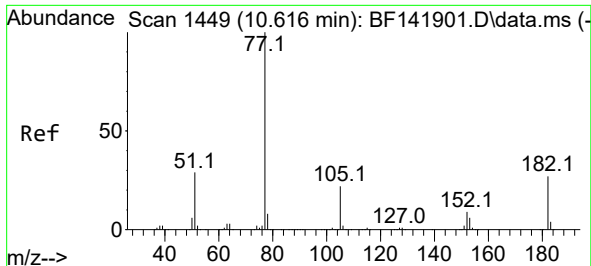

#63
Azobenzene
Concen: 2.736 ng
RT: 10.616 min Scan# 1449
Delta R.T. 0.000 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09




Instrument :
BNA_F
ClientSampleId :
WC-2


Tgt Ion: 77 Resp: 49448
Ion Ratio Lower Upper
77 100
182 80.8 6.6 46.6#
105 149.5 1.3 41.3#
51 36.7 10.4 50.4

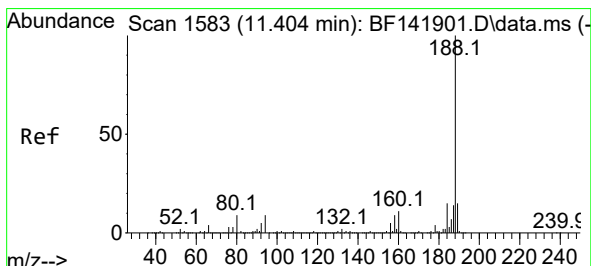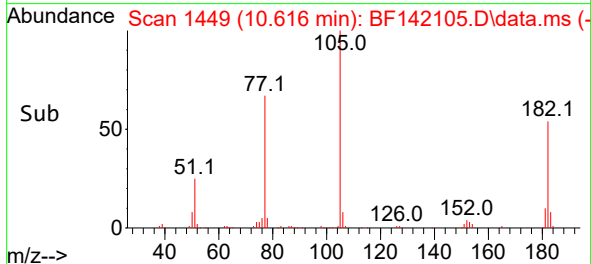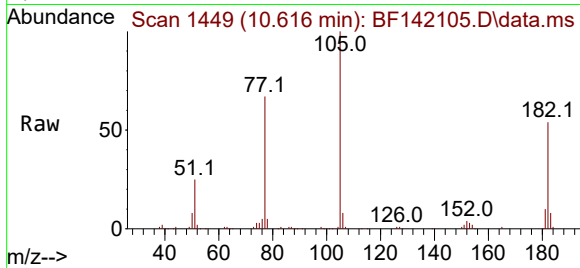

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.392 min Scan# 1581
Delta R.T. -0.012 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion: 188 Resp: 523529
Ion Ratio Lower Upper
188 100
94 8.0 6.8 10.2
80 9.0 7.6 11.4


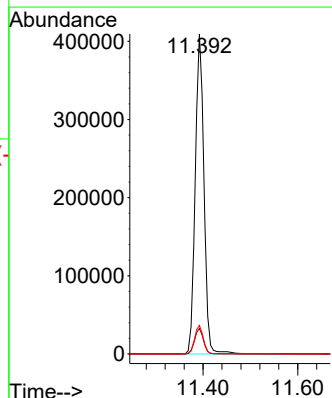

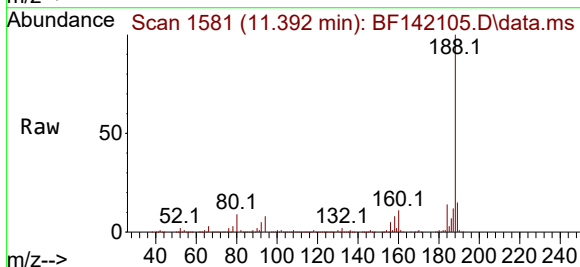




#67
4-Bromophenyl-phenylether
Concen: 3.040 ng
RT: 10.692 min Scan# 14
Delta R.T. -0.253 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09




Instrument :
BNA_F
ClientSampleId :
WC-2


Tgt Ion:248 Resp: 19990
Ion Ratio Lower Upper
248 100
250 186.8 77.8 116.8#
141 459.4 62.6 93.8#

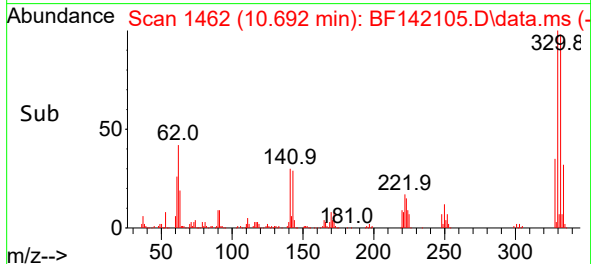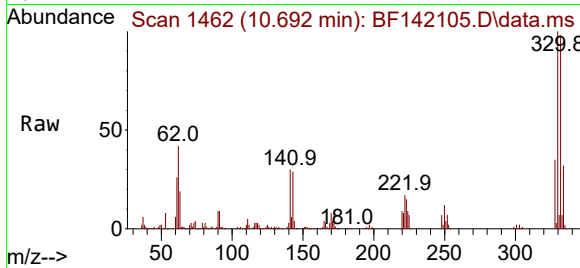

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.033 min Scan# 2030
Delta R.T. -0.006 min
Lab File: BF142105.D
Acq: 26 Mar 2025 19:09

Tgt Ion:240 Resp: 405207
Ion Ratio Lower Upper
240 100
120 8.8 8.4 12.6
236 25.1 20.5 30.7


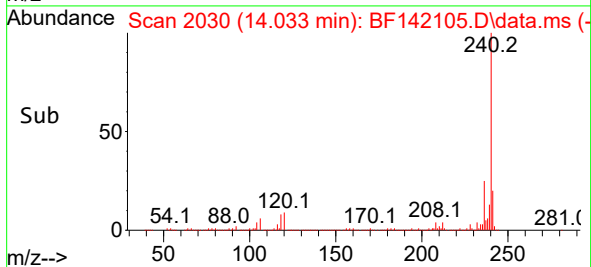

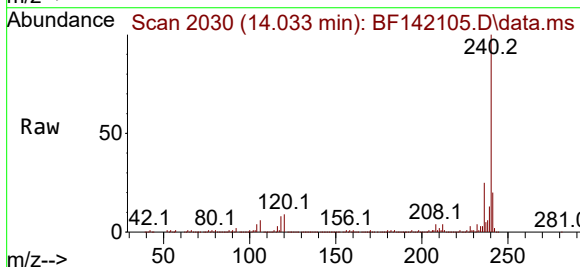


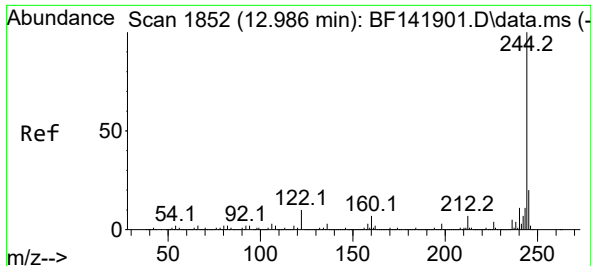

#79
 Terphenyl-d14
 Concen: 48.133 ng
 RT: 12.980 min Scan# 1851
 Delta R.T. -0.006 min
 Lab File: BF142105.D
 Acq: 26 Mar 2025 19:09

Instrument :
 BNA_F
 ClientSampleId :
 WC-2

Tgt Ion:244 Resp: 1319200
 Ion Ratio Lower Upper
 244 100
 212 6.8 6.0 9.0
 122 8.3 7.7 11.5

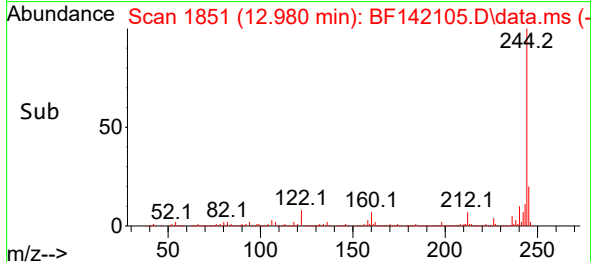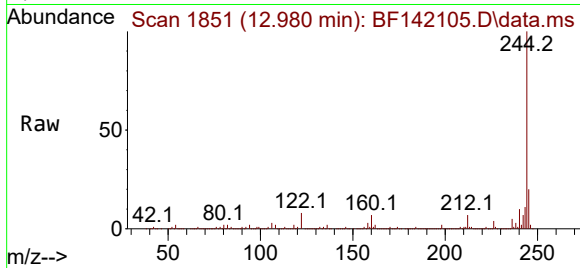

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.504 min Scan# 2280
 Delta R.T. -0.006 min
 Lab File: BF142105.D
 Acq: 26 Mar 2025 19:09

Tgt Ion:264 Resp: 343378
 Ion Ratio Lower Upper
 264 100
 260 23.0 19.1 28.7
 265 21.4 17.5 26.3

