
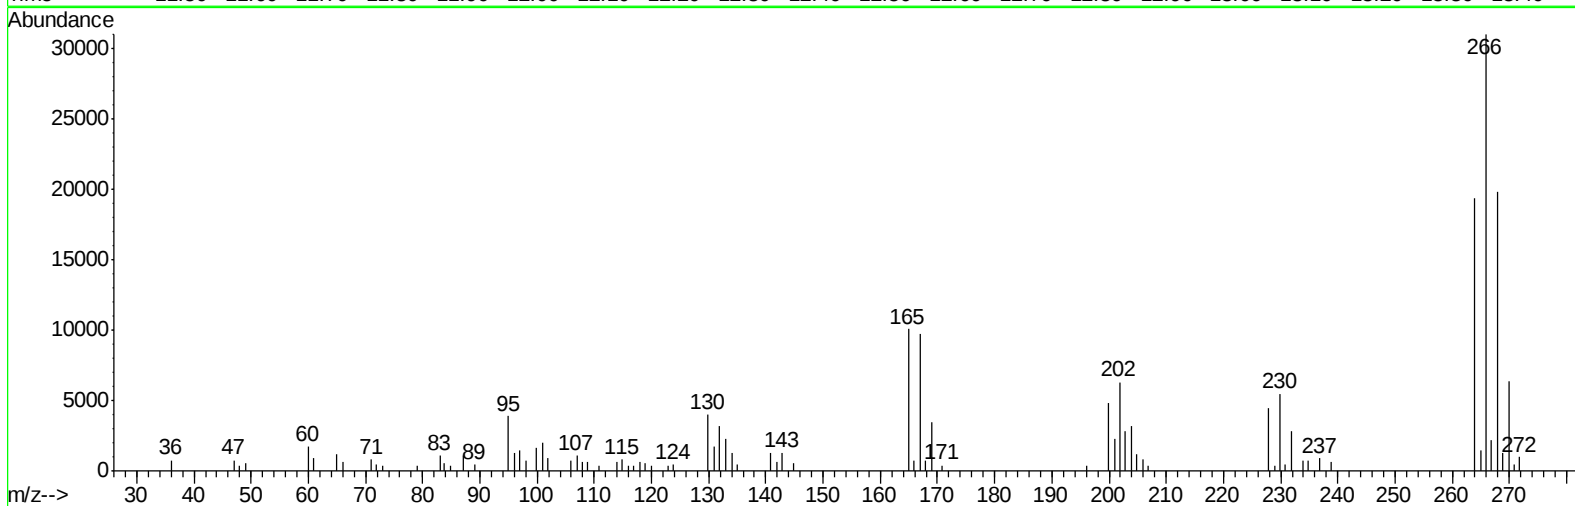


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032715\
Data File : BF078056.D
Acq On : 28 Mar 2015 00:33
Operator : TP/IZ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 30 03:45:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 30 00:50:20 2015
Response via : Initial Calibration

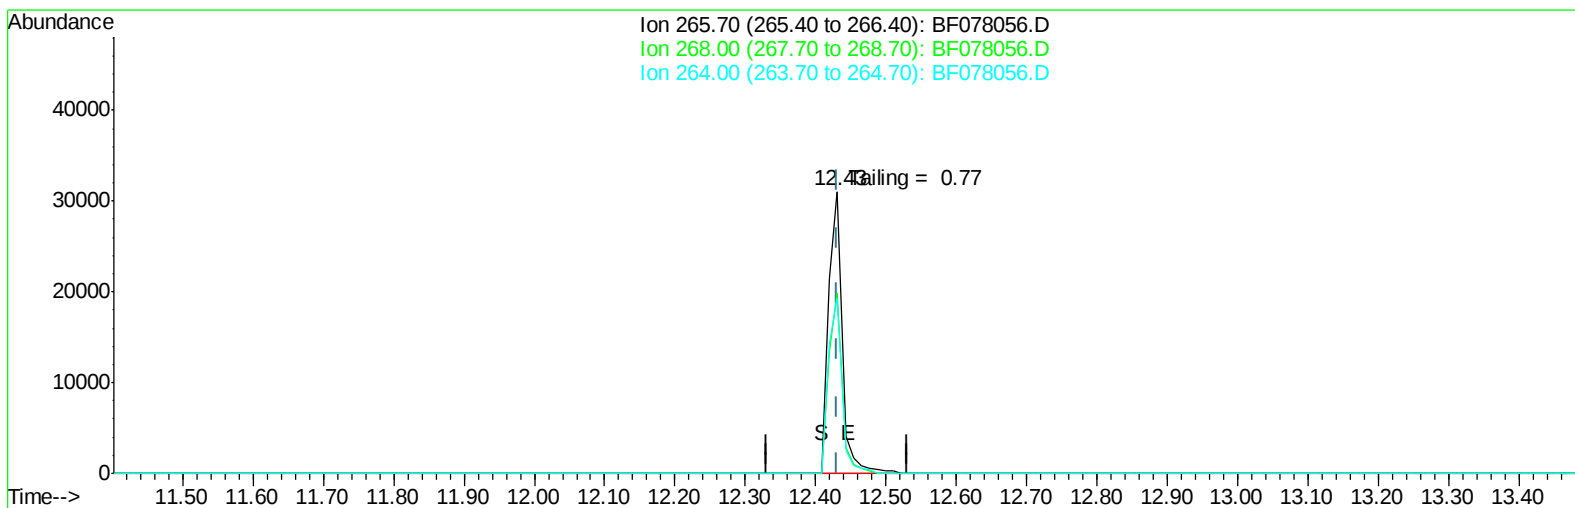

TIC: BF078056.D

(69) Pentachlorophenol (C)



12.431min (-0.000) 29.53ng

response 41234

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	63.92
264.00	61.20	62.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032715\
Data File : BF078056.D
Acq On : 28 Mar 2015 00:33
Operator : TP/IZ
Sample : SSTDCCC040
Misc :
ALS Vial : 2 Sample Multiplier: 1

Quant Time: Mar 30 03:45:35 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 30 00:50:20 2015
Response via : Initial Calibration

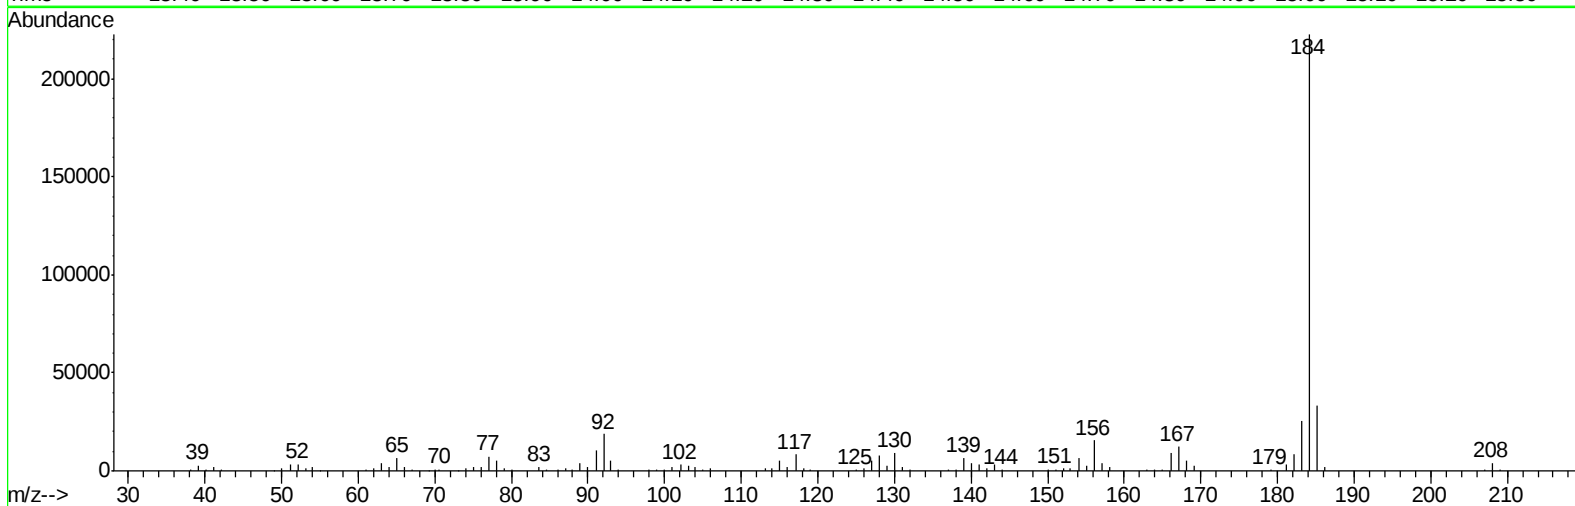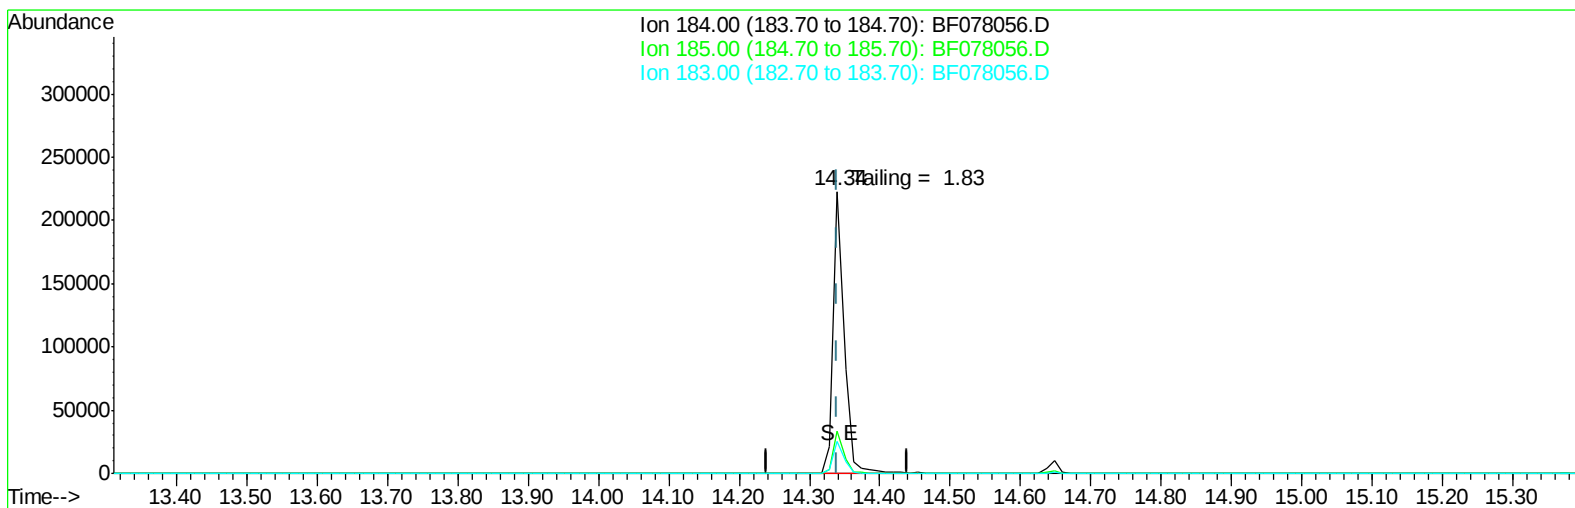

TIC: BF078056.D

(76) Benzidine

14.340min (-0.000) 35.98ng

response 235622

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	15.05
183.00	11.10	11.37
0.00	0.00	0.00