

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032715\
 Data File : BF078060.D
 Acq On : 28 Mar 2015 4:33
 Operator : TP/IZ
 Sample : G1672-02
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-100-32615

Quant Time: Mar 28 06:42:24 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 28 05:39:24 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.07	152	39975	20.00	ng	0.00
21) Naphthalene-d8	8.65	136	165902	20.00	ng	0.00
38) Acenaphthene-d10	10.82	164	80836	20.00	ng	0.00
63) Phenanthrene-d10	12.65	188	164965	20.00	ng	-0.01
75) Chrysene-d12	15.93	240	172424	20.00	ng	0.00
86) Perylene-d12	17.68	264	170435	20.00	ng	0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	120786	52.74	ng	0.00
7) Phenol-d6	6.67	99	88769	31.37	ng	0.00
23) Nitrobenzene-d5	7.77	82	219910	86.89	ng	-0.01
41) 2,4,6-Tribromophenol	11.80	330	98824	127.77	ng	0.00
44) 2-Fluorobiphenyl	10.00	172	488911	88.88	ng	0.00
78) Terphenyl-d14	14.65	244	577835	81.86	ng	0.00


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032715\
Data File : BF078060.D
Acq On : 28 Mar 2015 4:33
Operator : TP/IZ
Sample : G1672-02
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DCW-WW-100-32615

Quant Time: Mar 28 06:42:24 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 28 05:39:24 2015
Response via : Initial Calibration

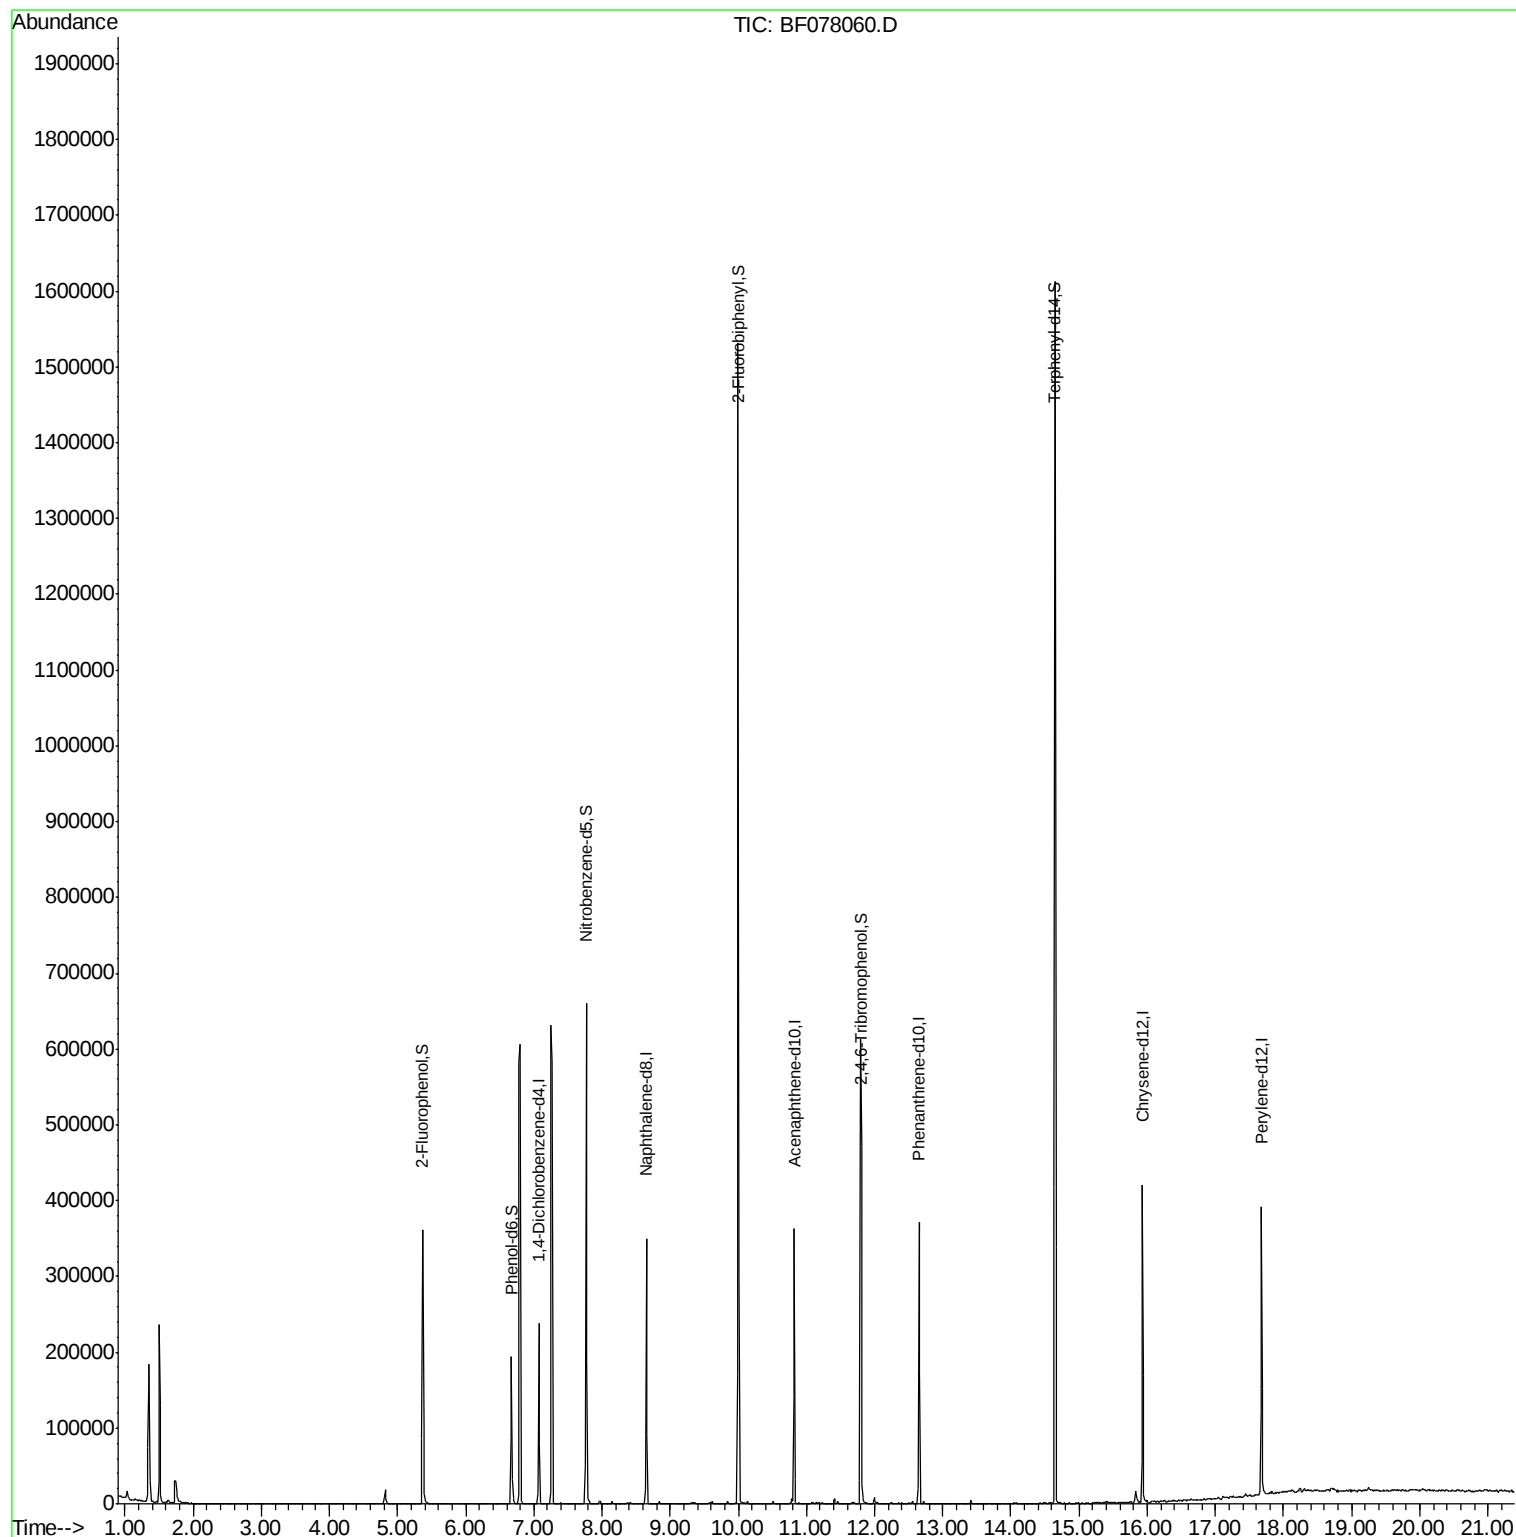




#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.07 min Scan# 541
Delta R.T. -0.00 min
Lab File: BF078060.D
Acq: 28 Mar 2015 4:33

Instrument :
BNA_F
ClientSampleId :
DCW-WW-100-32615

Tot Ion:152 Resp: 39975
Ion Ratio Lower Upper
152 100
150 162.8 119.5 179.3
115 63.5 43.0 64.4

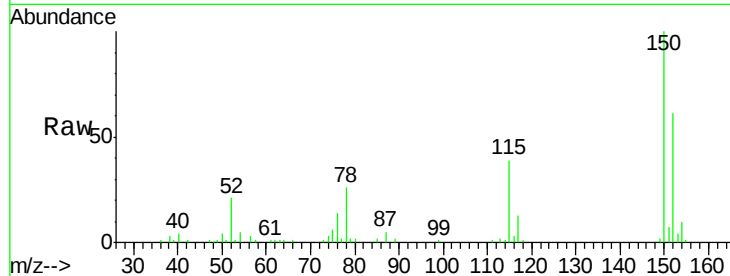


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

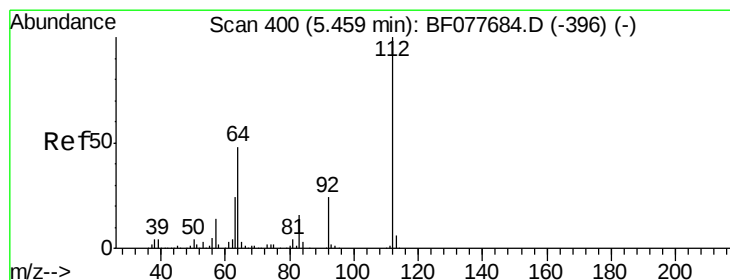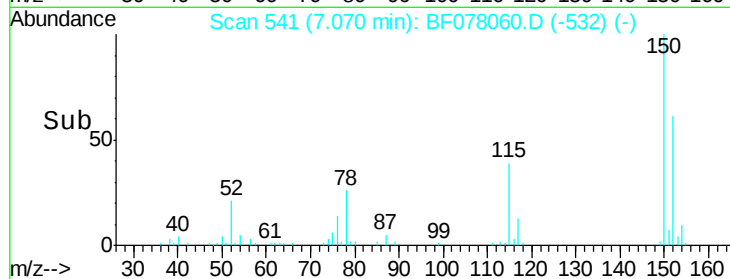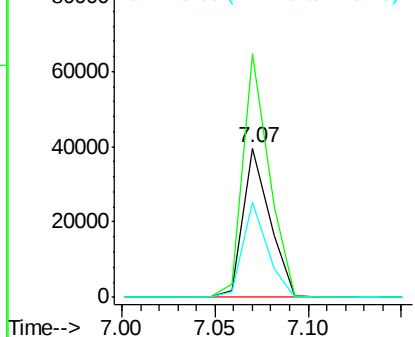



#5

2-Fluorophenol
Concen: 52.74 ng
RT: 5.37 min Scan# 392
Delta R.T. -0.00 min
Lab File: BF078060.D
Acq: 28 Mar 2015 4:33

Tgt Ion:112 Resp: 120786
Ion Ratio Lower Upper
112 100
64 54.8 38.6 57.8
63 28.1 19.3 28.9

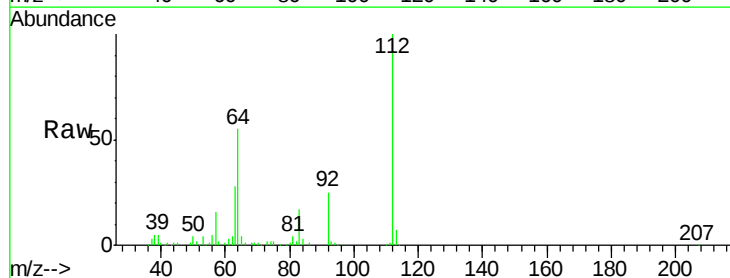

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

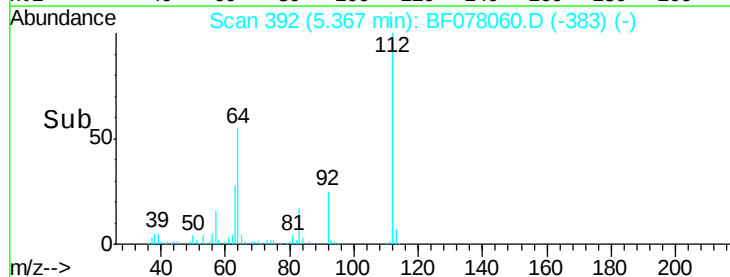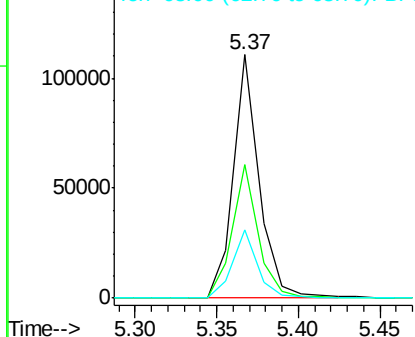



#7

Phenol-d6

Concen: 31.37 ng

RT: 6.67 min Scan# 506

Delta R.T. -0.00 min

Lab File: BF078060.D

Acq: 28 Mar 2015 4:33

Instrument :

BNA_F

ClientSampleId :

DCW-WW-100-32615


Tot Ion: 99 Resp: 88769

Ion Ratio Lower Upper

99 100

42 14.1 11.0 16.4



71 28.6 23.4 35.2

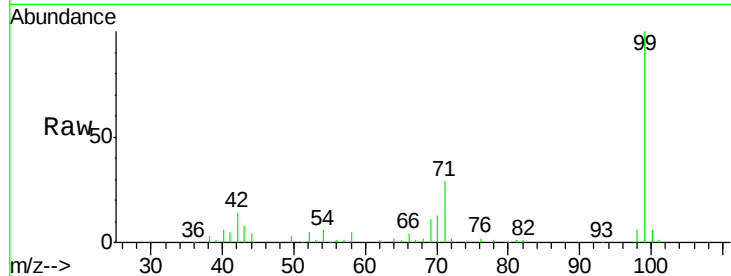

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

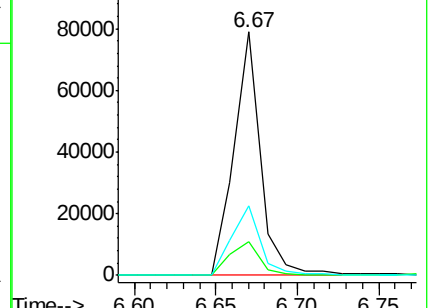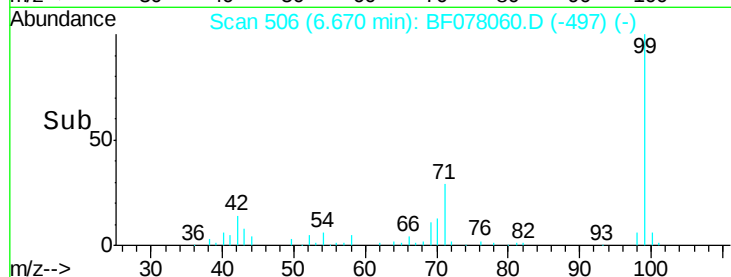

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.65 min Scan# 679

Delta R.T. -0.00 min

Lab File: BF078060.D

Acq: 28 Mar 2015 4:33

Tgt Ion: 136 Resp: 165902


Ion Ratio Lower Upper

136 100

137 10.9 8.7 13.1

54 7.6 4.6 6.8#

68 6.2 3.7 5.5#


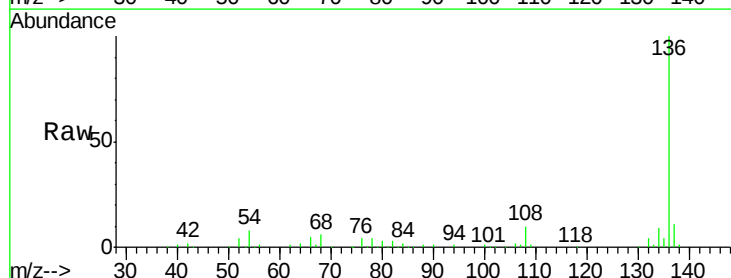



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

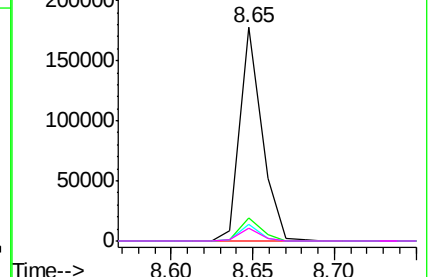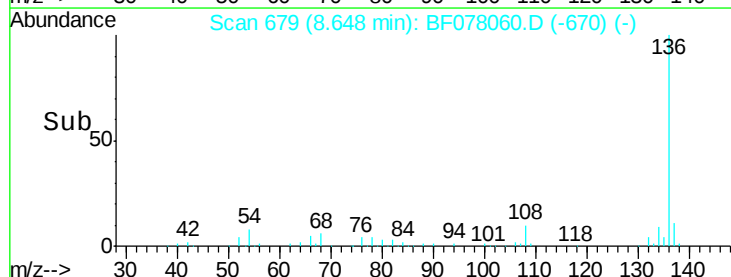


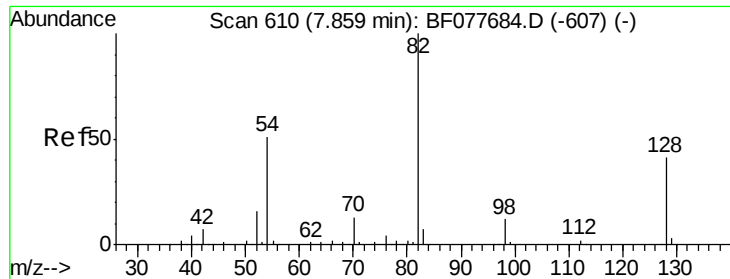




#23
 Nitrobenzene-d5
 Concen: 86.89 ng
 RT: 7.77 min Scan# 602
 Delta R.T. -0.01 min
 Lab File: BF078060.D
 Acq: 28 Mar 2015 4:33

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-100-32615

Tot Ion	82	Resp	219910
Ion Ratio	100	Lower	Upper
128	42.6	32.8	49.2
54	49.7	40.6	60.8

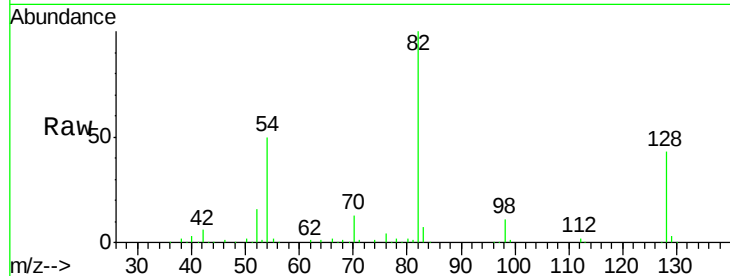


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

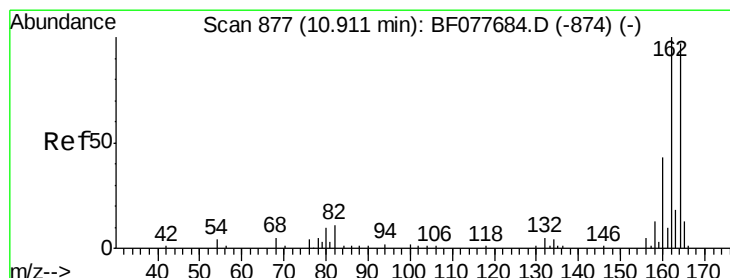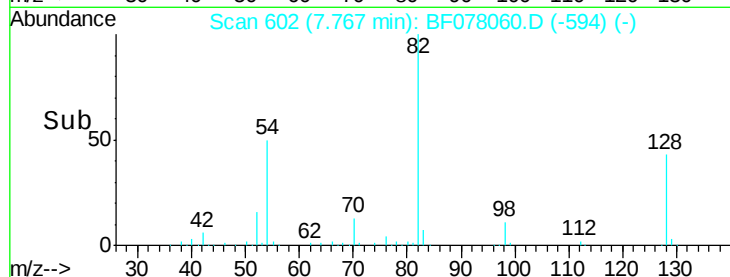
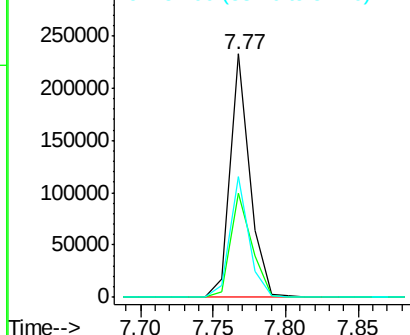


#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.82 min Scan# 869
 Delta R.T. -0.00 min
 Lab File: BF078060.D
 Acq: 28 Mar 2015 4:33

Tgt Ion	164	Resp	80836
Ion Ratio	100	Lower	Upper
162	105.4	82.4	123.6
160	45.3	35.8	53.6

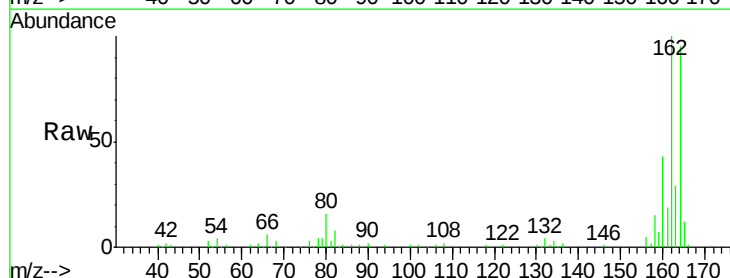

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

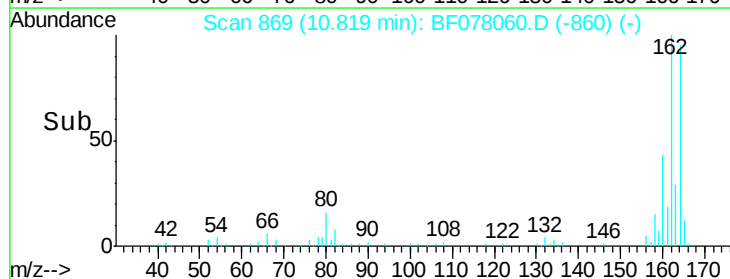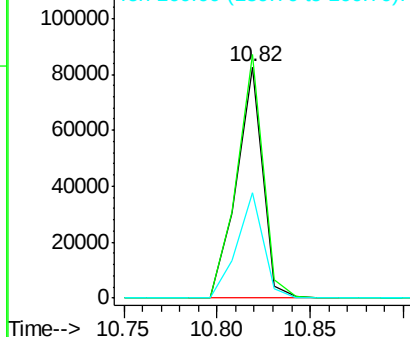






#41
 2,4,6-Tribromophenol
 Concen: 127.77 ng
 RT: 11.80 min Scan# 955
 Delta R.T. -0.00 min
 Lab File: BF078060.D
 Acq: 28 Mar 2015 4:33

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-100-32615

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.5	0.0	0.0#
141	36.4	0.0	0.0#

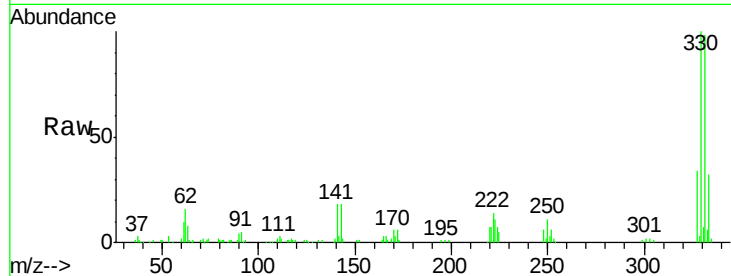


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

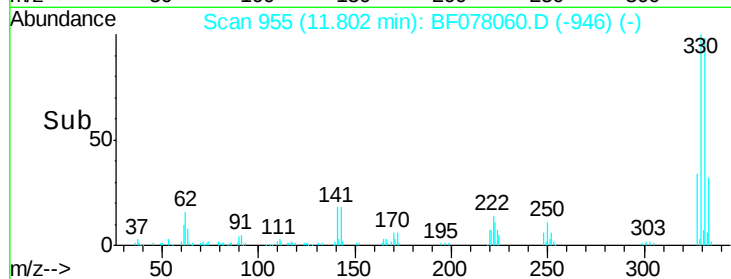
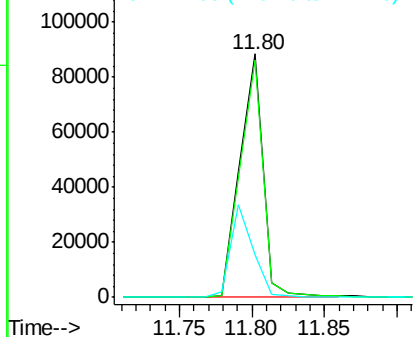



#44
 2-Fluorobiphenyl
 Concen: 88.88 ng
 RT: 10.00 min Scan# 797
 Delta R.T. -0.00 min
 Lab File: BF078060.D
 Acq: 28 Mar 2015 4:33

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	28.5	42.7
170	23.5	18.8	28.2

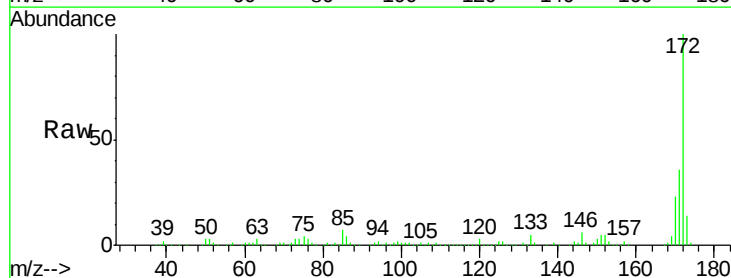

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

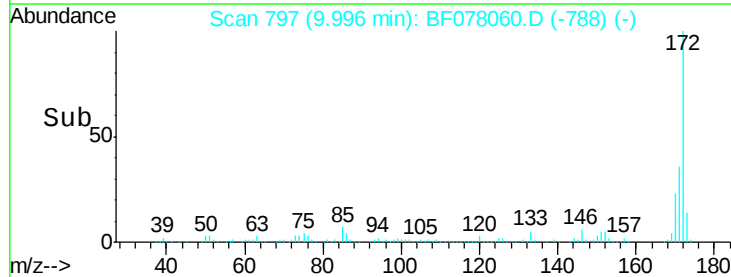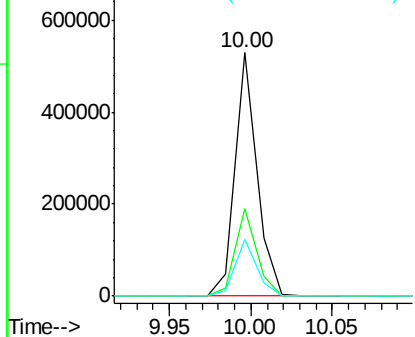


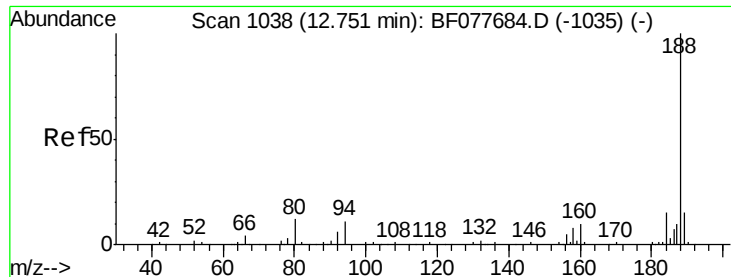



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.65 min Scan# 1029
Delta R.T. -0.01 min
Lab File: BF078060.D
Acq: 28 Mar 2015 4:33

Instrument :
BNA_F
ClientSampleId :
DCW-WW-100-32615

Tot Ion:188 Resp: 164965
Ion Ratio Lower Upper
188 100
94 11.5 8.7 13.1
80 12.1 9.3 13.9

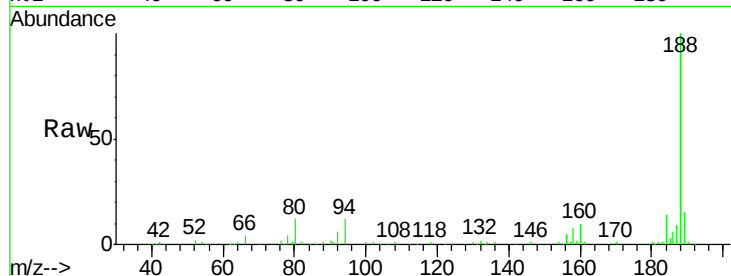


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

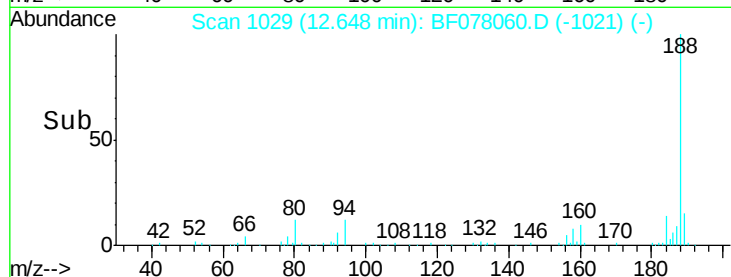
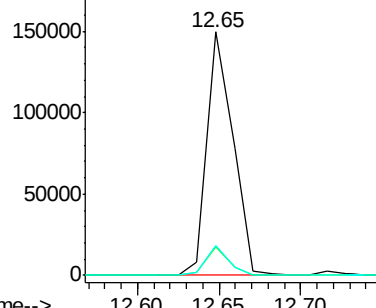


#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.93 min Scan# 1316
Delta R.T. -0.00 min
Lab File: BF078060.D
Acq: 28 Mar 2015 4:33

Tgt Ion:240 Resp: 172424
Ion Ratio Lower Upper
240 100
120 13.6 8.2 12.2#
236 25.0 20.0 30.0

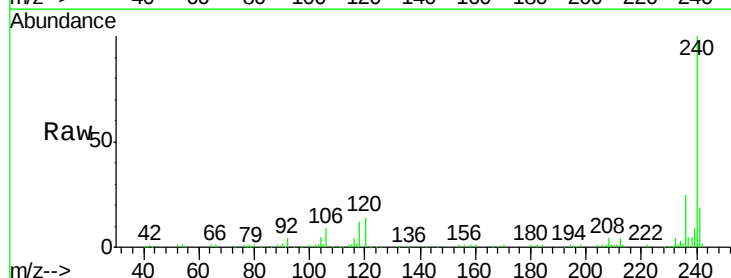

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



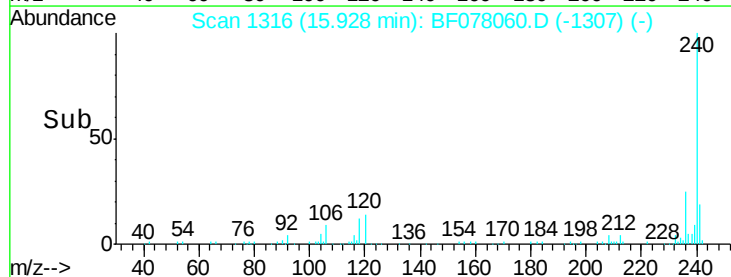
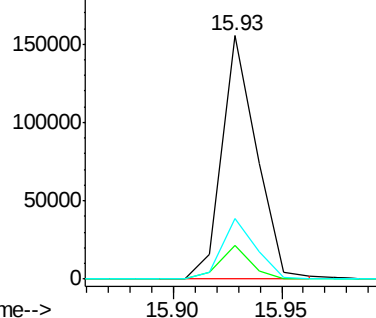




#78
 Terphenyl-d14
 Concen: 81.86 ng
 RT: 14.65 min Scan# 1204
 Delta R.T. -0.00 min
 Lab File: BF078060.D
 Acq: 28 Mar 2015 4:33

Instrument :
 BNA_F
 ClientSampleId :
 DCW-WW-100-32615

Tot Ion:244 Resp: 577835
 Ion Ratio Lower Upper
 244 100
 212 6.8 4.9 7.3
 122 12.7 6.2 9.4#

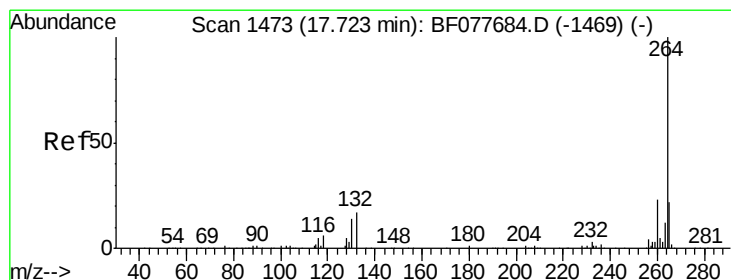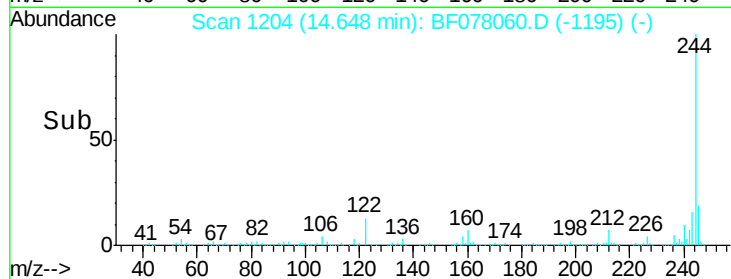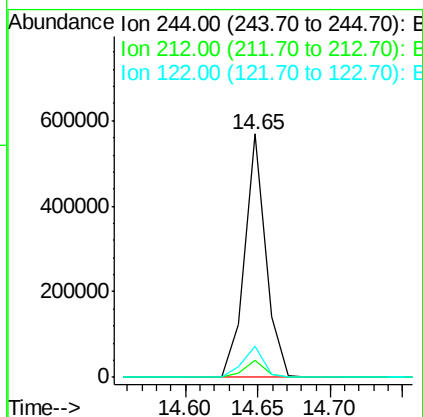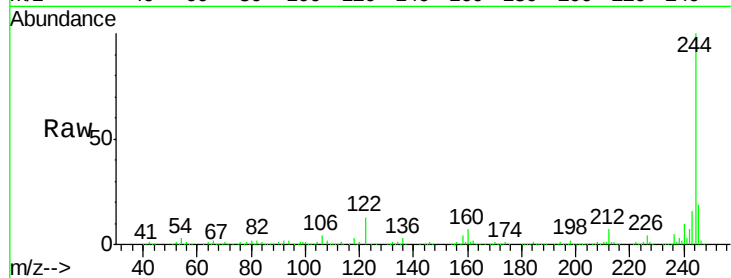

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.68 min Scan# 1469
 Delta R.T. 0.06 min
 Lab File: BF078060.D
 Acq: 28 Mar 2015 4:33

Tgt Ion:264 Resp: 170435
 Ion Ratio Lower Upper
 264 100
 260 23.9 18.6 27.8
 265 21.3 17.3 25.9

