

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032715\
 Data File : BF078074.D
 Acq On : 28 Mar 2015 11:14
 Operator : TP/IZ
 Sample : G1677-10
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PE-4(7.5-8)

Quant Time: Mar 30 02:13:01 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 30 00:50:20 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.07	152	37426	20.00	ng	0.00
21) Naphthalene-d8	8.65	136	150509	20.00	ng	0.00
38) Acenaphthene-d10	10.82	164	74116	20.00	ng	0.00
63) Phenanthrene-d10	12.65	188	146420	20.00	ng	0.00
75) Chrysene-d12	15.93	240	166153	20.00	ng	0.00
86) Perylene-d12	17.64	264	158860	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.37	112	276545	128.98	ng	0.00
7) Phenol-d6	6.66	99	344206	129.93	ng	-0.01
23) Nitrobenzene-d5	7.77	82	203417	88.59	ng	-0.01
41) 2,4,6-Tribromophenol	11.80	330	81843	115.41	ng	0.00
44) 2-Fluorobiphenyl	10.00	172	438489	86.95	ng	0.00
78) Terphenyl-d14	14.65	244	526671	77.43	ng	0.00
Target Compounds						
31) Naphthalene	8.67	128	17304	2.24	ng	# 82
37) 2-Methylnaphthalene	9.54	142	34922	6.72	ng	98
49) Dimethylphthalate	10.51	163	12167	2.21	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032715\
Data File : BF078074.D
Acq On : 28 Mar 2015 11:14
Operator : TP/IZ
Sample : G1677-10
Misc :
ALS Vial : 37 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PE-4(7.5-8)

Quant Time: Mar 30 02:13:01 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF031115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 30 00:50:20 2015
Response via : Initial Calibration

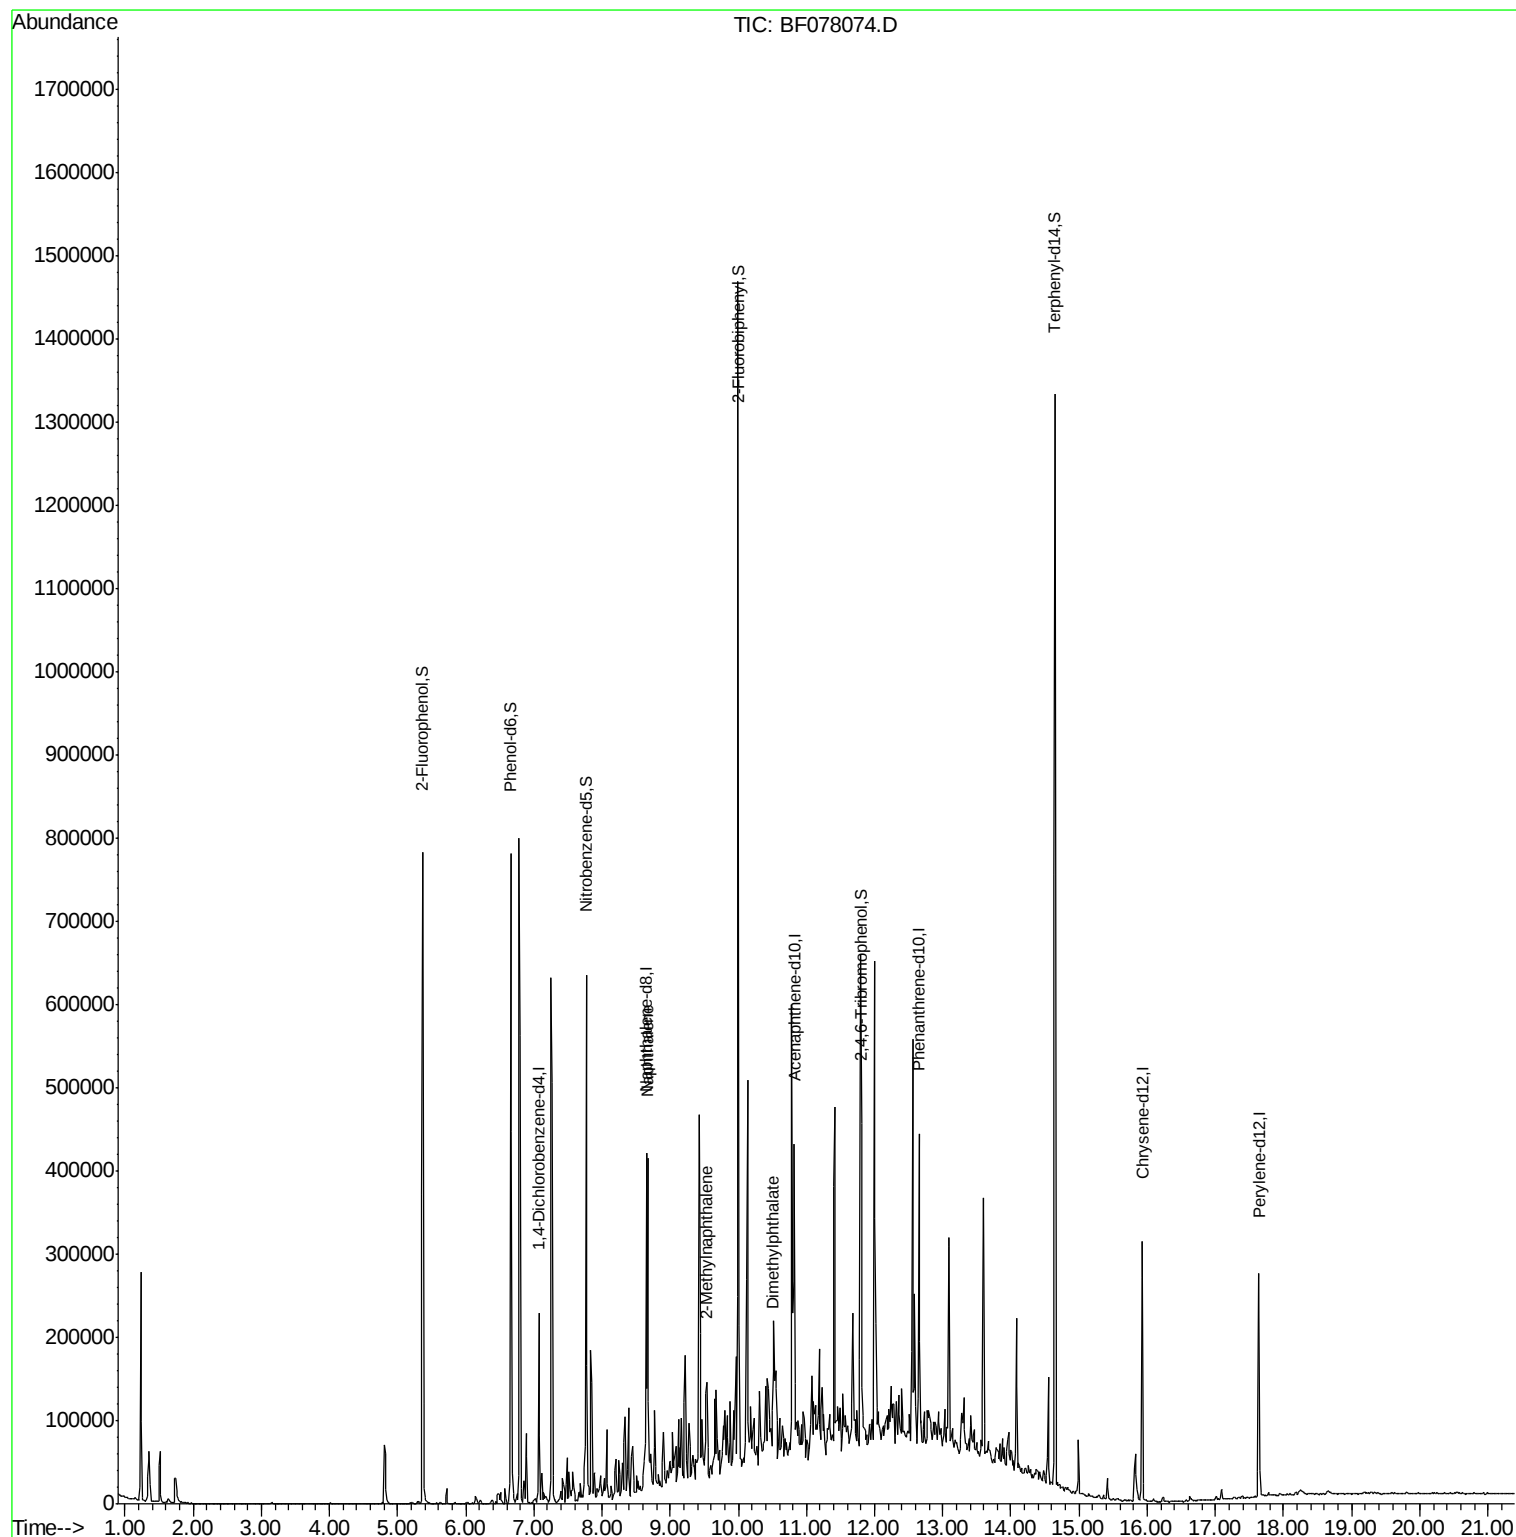

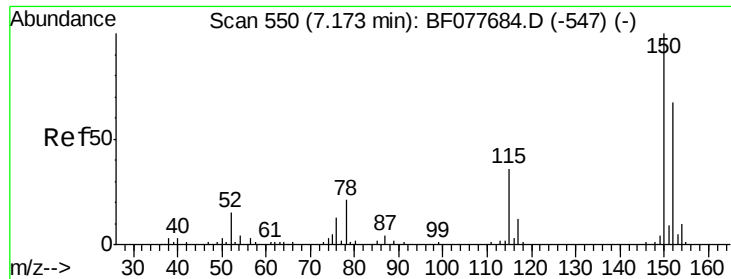


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 7.07 min Scan# 541
Delta R.T. -0.00 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14

Instrument :
BNA_F
ClientSampleId :
PE-4(7.5-8)

Tot Ion:152 Resp: 37426
Ion Ratio Lower Upper
152 100
150 156.6 119.5 179.3
115 62.5 43.0 64.4

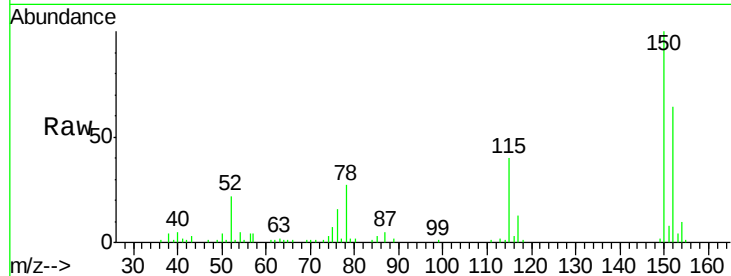


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

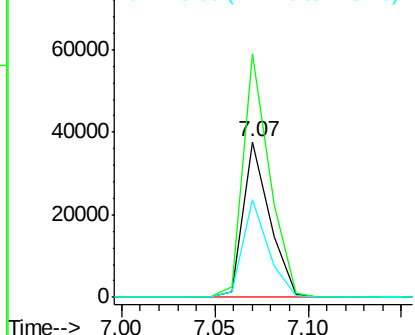



#5


2-Fluorophenol
Concen: 128.98 ng
RT: 5.37 min Scan# 392
Delta R.T. -0.00 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14

Tgt Ion:112 Resp: 276545
Ion Ratio Lower Upper
112 100
64 52.5 38.6 57.8
63 26.2 19.3 28.9



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

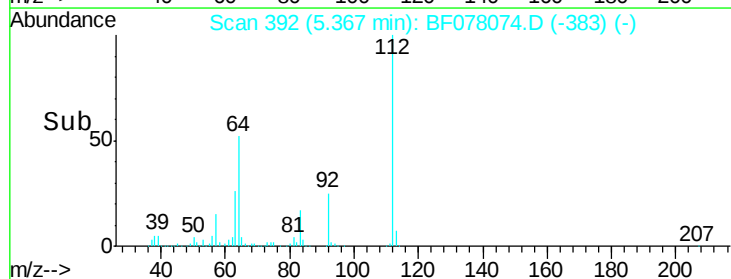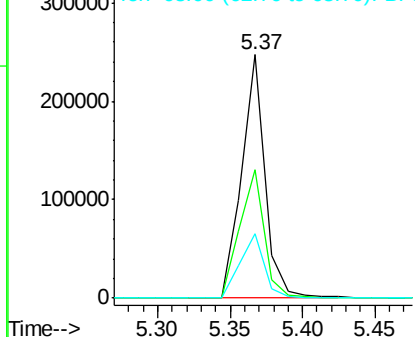

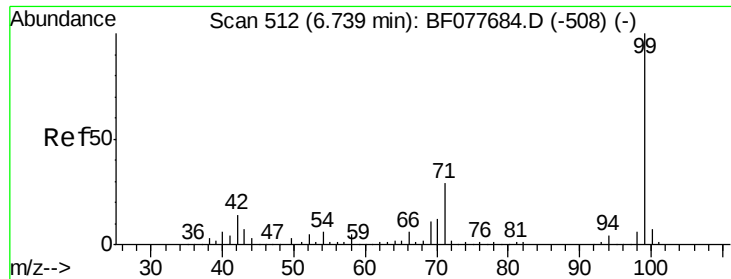

#7

Phenol-d6

Concen: 129.93 ng

RT: 6.66 min Scan# 505

Delta R.T. -0.01 min

Lab File: BF078074.D

Acq: 28 Mar 2015 11:14

Instrument :


BNA_F

ClientSampleId :

PE-4(7.5-8)

Tot Ion: 99 Resp: 344206




Ion	Ratio	Lower	Upper
99	100		
42	18.8	11.0	16.4#
71	34.0	23.4	35.2

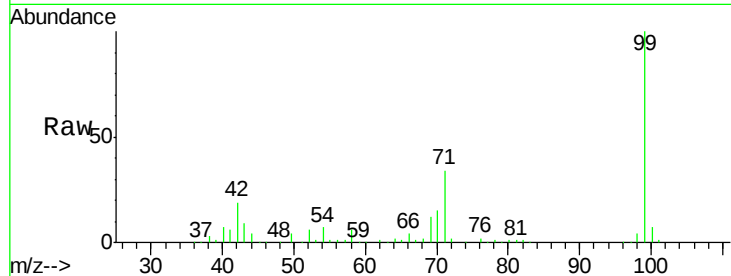

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

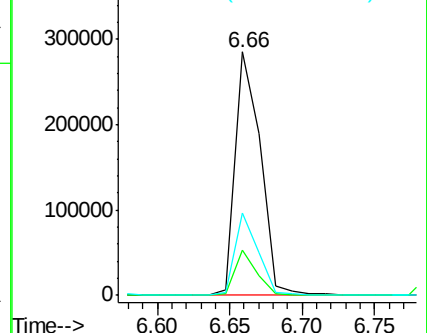

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.65 min Scan# 679


Delta R.T. -0.00 min

Lab File: BF078074.D

Acq: 28 Mar 2015 11:14

Tgt Ion: 136 Resp: 150509

Ion	Ratio	Lower	Upper
136	100		
137	11.1	8.7	13.1
54	7.6	4.6	6.8#
68	6.3	3.7	5.5#






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

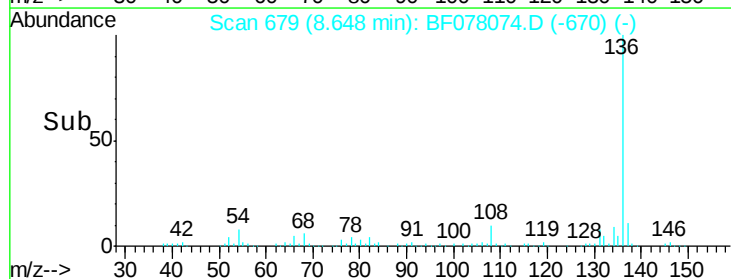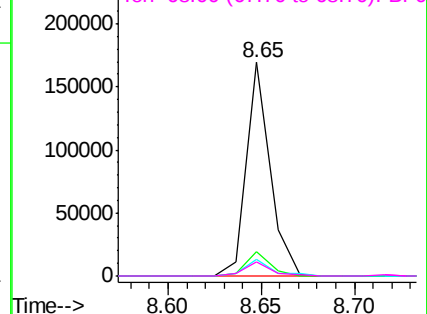


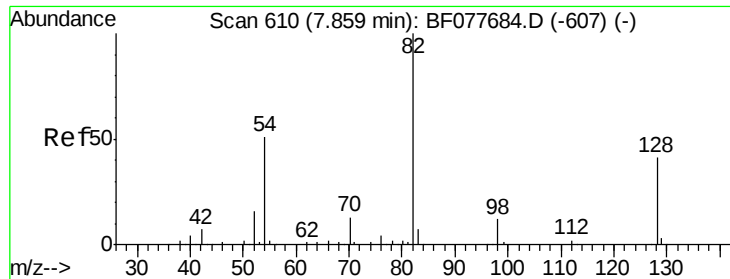




#23
 Nitrobenzene-d5
 Concen: 88.59 ng
 RT: 7.77 min Scan# 602
 Delta R.T. -0.01 min
 Lab File: BF078074.D
 Acq: 28 Mar 2015 11:14

Instrument :
 BNA_F
 ClientSampleId :
 PE-4(7.5-8)

Tot Ion	82	Resp	203417
Ion Ratio	Lower	Upper	
82	100		
128	42.3	32.8	49.2
54	48.8	40.6	60.8

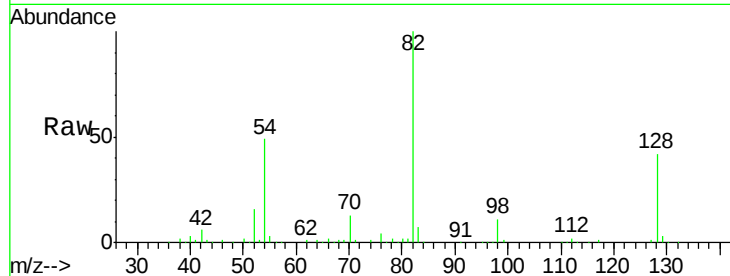


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

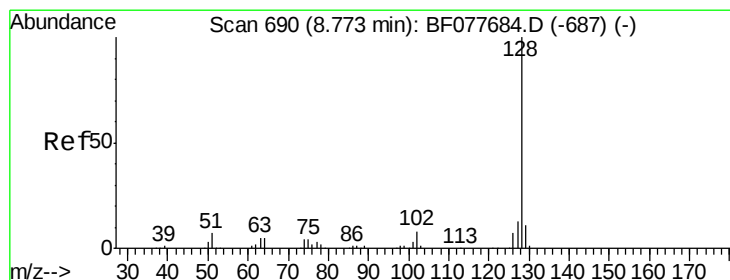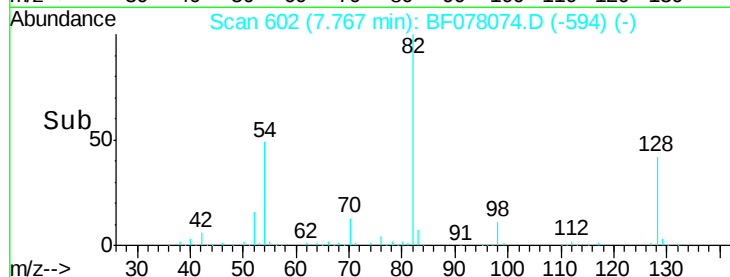
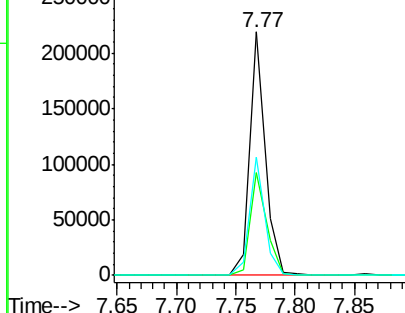



#31
 Naphthalene
 Concen: 2.24 ng
 RT: 8.67 min Scan# 681
 Delta R.T. -0.01 min
 Lab File: BF078074.D
 Acq: 28 Mar 2015 11:14

Tgt Ion	128	Resp	17304
Ion Ratio	Lower	Upper	
128	100		
129	9.5	8.9	13.3
127	24.6	10.4	15.6#

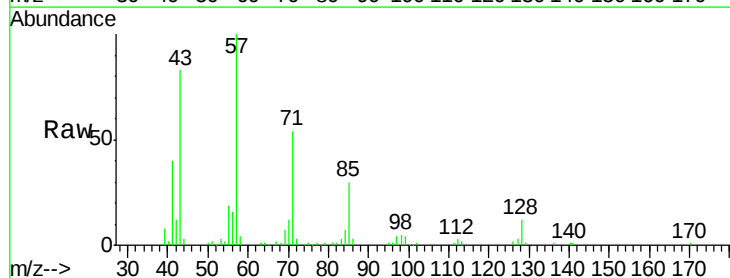

Abundance Ion 128.00 (127.70 to 128.70): E
 Ion 129.00 (128.70 to 129.70): E
 Ion 127.00 (126.70 to 127.70): E



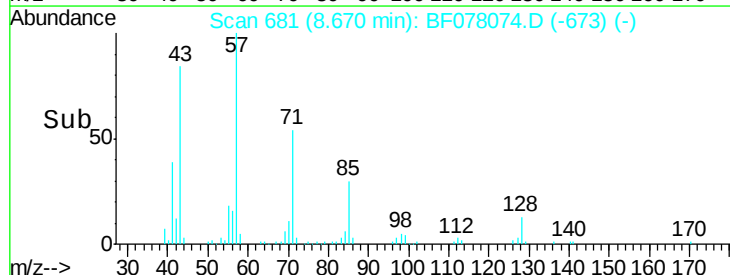
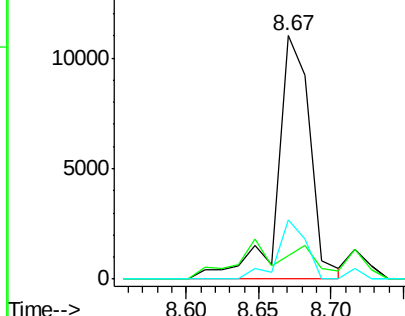


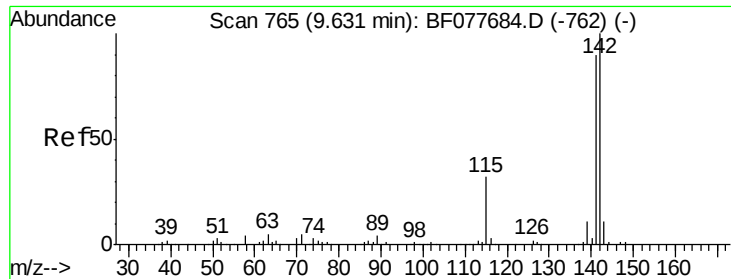

#37
2-Methylnaphthalene
Concen: 6.72 ng
RT: 9.54 min Scan# 757
Delta R.T. -0.00 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14




Instrument :
BNA_F
ClientSampleId :
PE-4(7.5-8)


Tot Ion:142 Resp: 34922
Ion Ratio Lower Upper
142 100
141 92.3 71.9 107.9
115 31.5 25.4 38.0

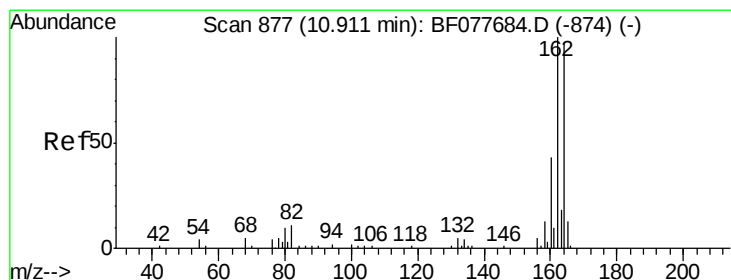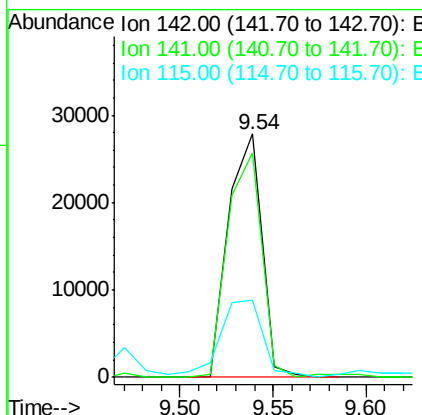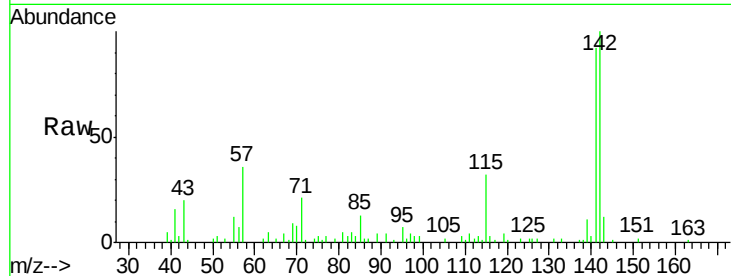

#38
Acenaphthene-d10
Concen: 20.00 ng
RT: 10.82 min Scan# 869
Delta R.T. -0.00 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14

Tgt Ion:164 Resp: 74116
Ion Ratio Lower Upper
164 100
162 106.9 82.4 123.6
160 45.9 35.8 53.6

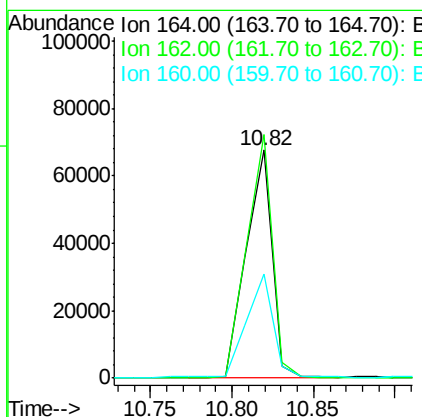


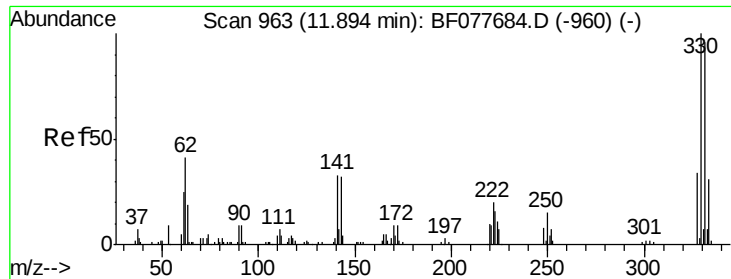




#41
 2,4,6-Tribromophenol
 Concen: 115.41 ng
 RT: 11.80 min Scan# 955
 Delta R.T. -0.00 min
 Lab File: BF078074.D
 Acq: 28 Mar 2015 11:14

Instrument :
 BNA_F
 ClientSampleId :
 PE-4(7.5-8)

Tot Ion:330 Resp: 81843
 Ion Ratio Lower Upper
 330 100
 332 96.8 0.0 0.0#
 141 39.7 0.0 0.0#




Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

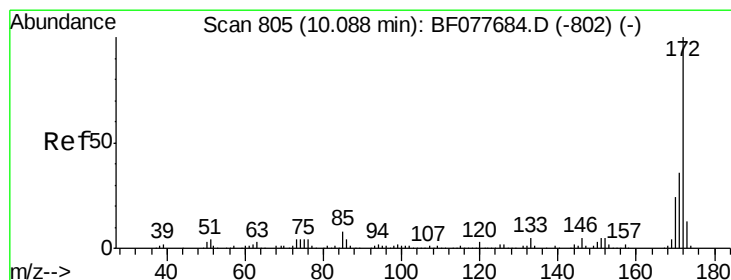
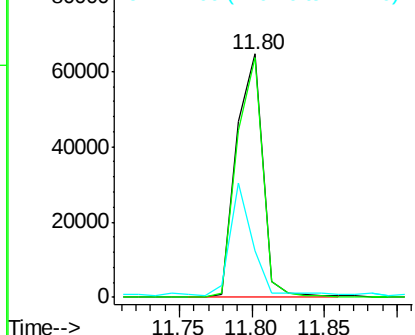



#44
 2-Fluorobiphenyl
 Concen: 86.95 ng
 RT: 10.00 min Scan# 797
 Delta R.T. -0.00 min
 Lab File: BF078074.D
 Acq: 28 Mar 2015 11:14

Tgt Ion:172 Resp: 438489
 Ion Ratio Lower Upper
 172 100
 171 35.7 28.5 42.7
 170 24.3 18.8 28.2

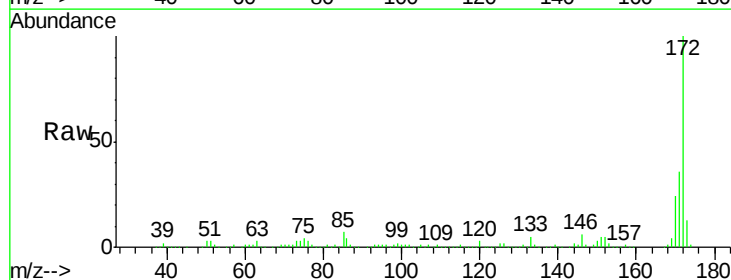

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

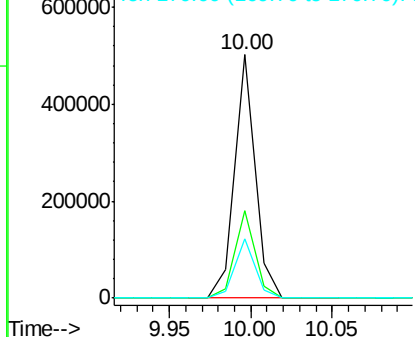



#49

Dimethylphthalate

Concen: 2.21 ng

RT: 10.51 min Scan# 842

Delta R.T. -0.00 min

Lab File: BF078074.D

Acq: 28 Mar 2015 11:14

Instrument :

BNA_F

ClientSampleId :

PE-4(7.5-8)


Tot Ion:163 Resp: 12167

Ion Ratio Lower Upper

163 100

194 4.5 2.7 4.1#




164 10.2 8.2 12.2



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

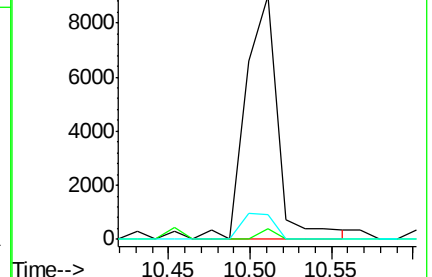

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 12.65 min Scan# 1029

Delta R.T. -0.00 min

Lab File: BF078074.D

Acq: 28 Mar 2015 11:14


Tgt Ion:188 Resp: 146420

Ion Ratio Lower Upper

188 100

94 10.7 8.7 13.1



80 11.3 9.3 13.9




Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0



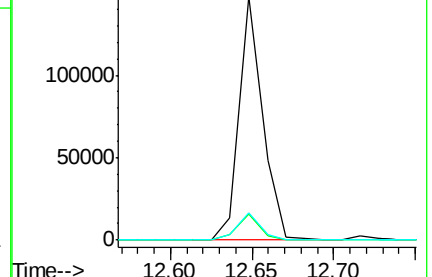



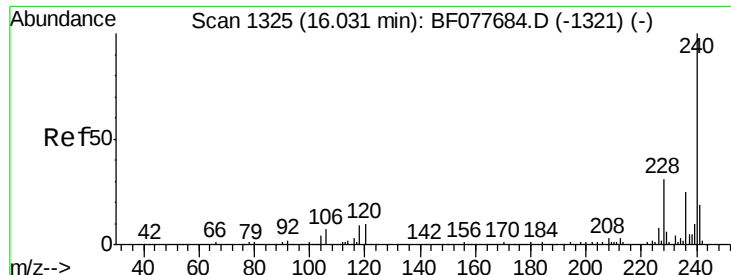

#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.93 min Scan# 1316
Delta R.T. -0.00 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14




Instrument :
BNA_F
ClientSampleId :
PE-4(7.5-8)


Tot Ion:240 Resp: 166153
Ion Ratio Lower Upper
240 100
120 8.6 8.2 12.2
236 24.6 20.0 30.0

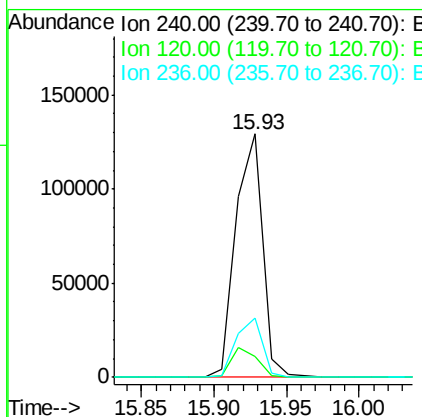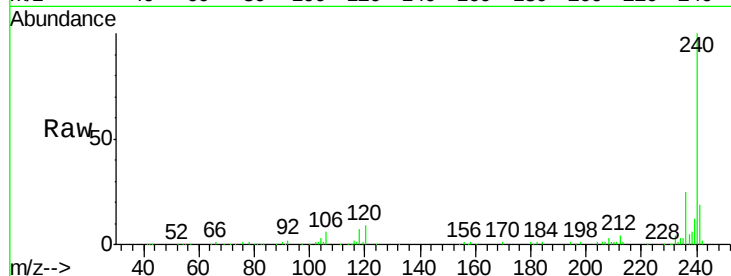

#78
Terphenyl-d14
Concen: 77.43 ng
RT: 14.65 min Scan# 1204
Delta R.T. -0.00 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14

Tgt Ion:244 Resp: 526671
Ion Ratio Lower Upper
244 100
212 6.3 4.9 7.3
122 9.1 6.2 9.4

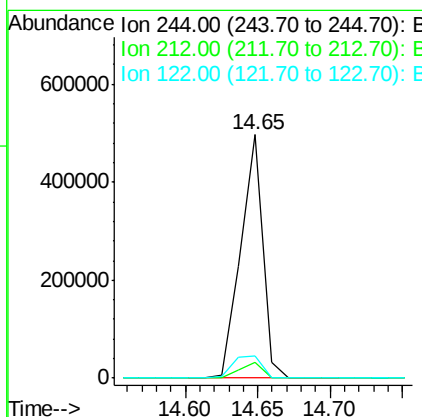


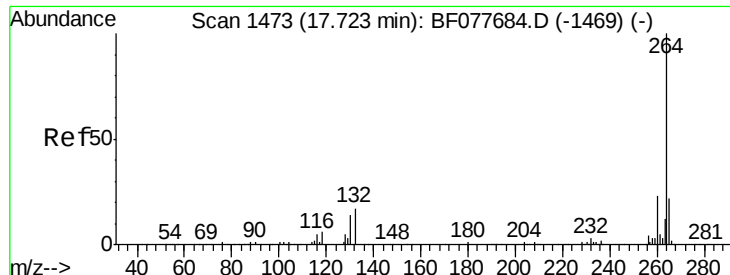

#86
Pervlene-d12
Concen: 20.00 ng
RT: 17.64 min Scan# 1466
Delta R.T. 0.01 min
Lab File: BF078074.D
Acq: 28 Mar 2015 11:14

Instrument :
BNA_F
ClientSampleId :
PE-4(7.5-8)

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.7	18.6	27.8
265	21.6	17.3	25.9

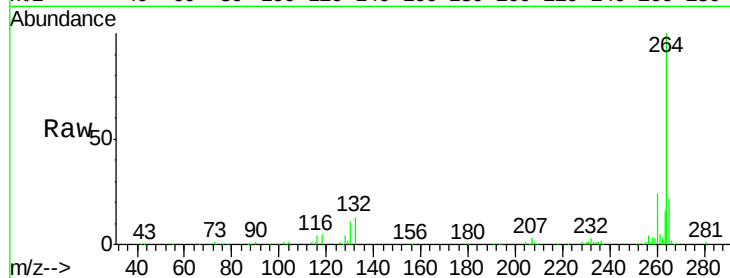

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

