


Data Path : Z:\HPCHEM1\BNA F\Data\BF032715\
 Data File : BF078035.D
 Acq On : 27 Mar 2015 13:26
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 28 05:37:34 2015

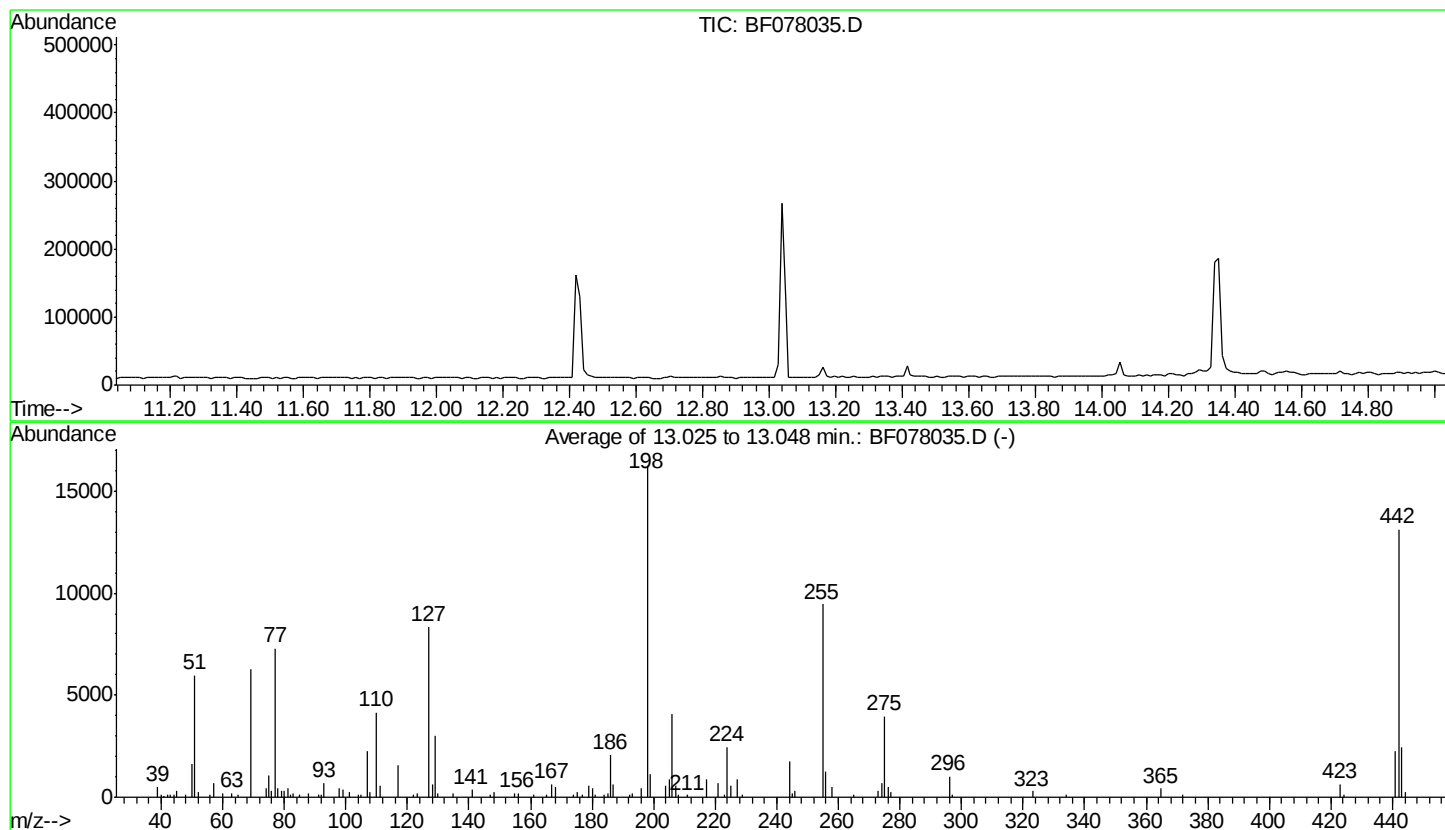

AutoFind: Scans 1062, 1063, 1064; Background Corrected with Scan 1059

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.7	5967	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.6	6265	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.5	8372	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	16247	PASS
199	198	5	9	6.9	1128	PASS
275	198	10	60	24.4	3970	PASS
365	198	1	100	2.6	426	PASS
441	442	0.01	24	17.0	2235	PASS
442	198	50	100	80.7	13118	PASS
443	442	15	24	18.7	2457	PASS