
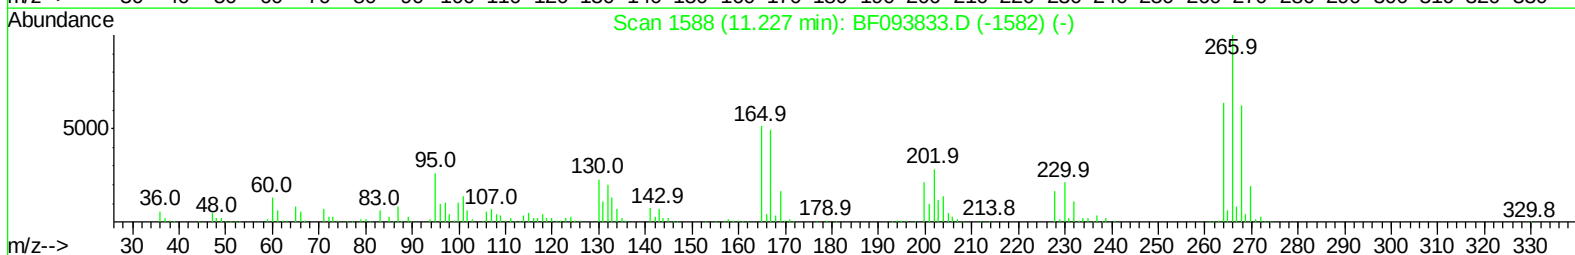
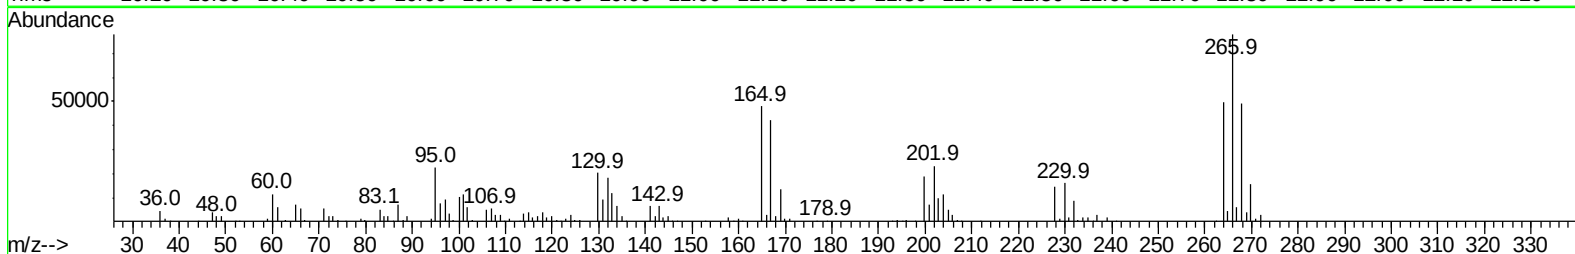


Data Path : Z:\HPCHEM1\BNA F\DATA\BF032717\
Data File : BF093937.D
Acq On : 27 Mar 2017 11:38
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 28 07:09:32 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 27 16:10:49 2017
Response via : Initial Calibration

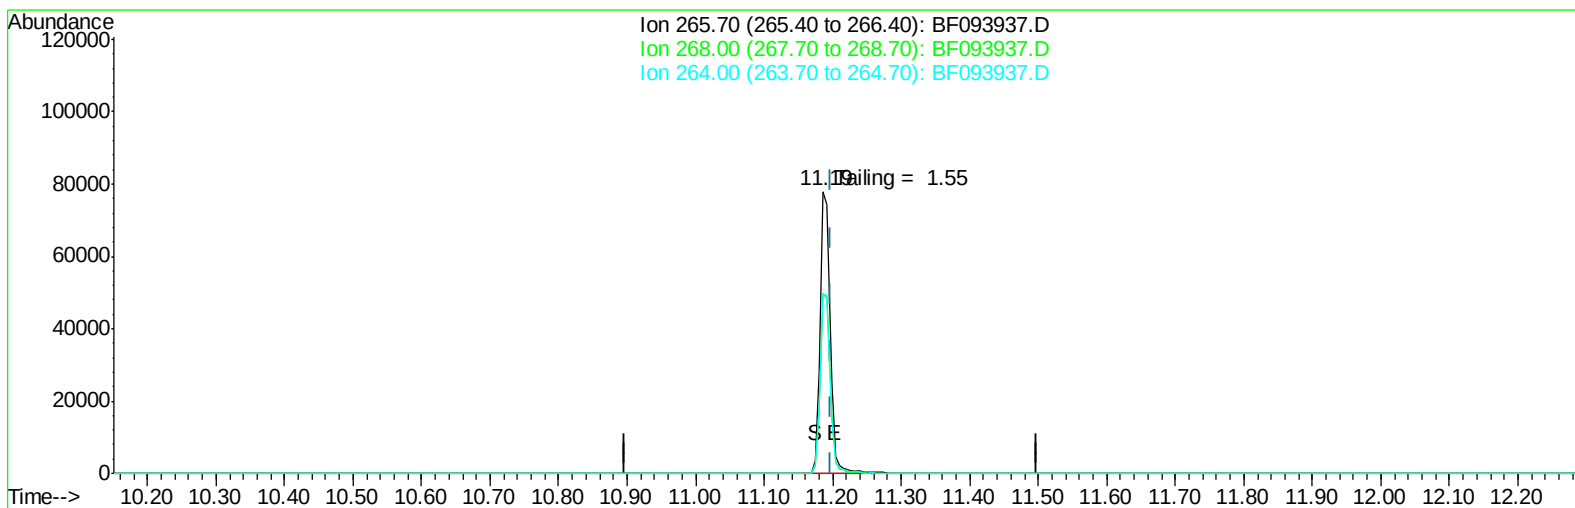

TIC: BF093937.D

(69) Pentachlorophenol (C)

11.186min (-0.012) 0.00ng

response 78574

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.45
264.00	64.60	64.14
0.00	0.00	0.00