

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
 Data File : BF093956.D
 Acq On : 27 Mar 2017 21:50
 Operator : SJ/MA
 Sample : I2409-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PZ-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.069	368	371	376	rBV	183210	174888	3.75%	0.562%
2	4.463	434	438	441	rBV	1946389	1720025	36.91%	5.532%
3	5.522	614	618	622	rBV	1183397	1186618	25.47%	3.817%
4	5.681	639	645	648	rBV	3008357	3072265	65.93%	9.881%
5	5.934	684	688	692	rBV	954457	943130	20.24%	3.033%
6	6.116	714	719	723	rBV	2836779	2772512	59.50%	8.917%
7	6.586	792	799	802	rBV	2142289	2421237	51.96%	7.787%
8	7.439	938	944	948	rBV	1289946	1295792	27.81%	4.168%
9	8.769	1163	1170	1173	rBV	4225710	4659560	100.00%	14.987%
10	9.257	1250	1253	1257	rVB	94293	87784	1.88%	0.282%
11	9.474	1285	1290	1292	rBV3	46495	61727	1.32%	0.199%
12	9.492	1292	1293	1300	rVV	52860	50061	1.07%	0.161%
13	9.586	1301	1309	1313	rVB2	1395847	1449723	31.11%	4.663%
14	10.563	1467	1475	1478	rBV	2272426	2788243	59.84%	8.968%
15	10.757	1505	1508	1511	rBV2	46072	51383	1.10%	0.165%
16	11.410	1613	1619	1623	rVB	1450815	1404791	30.15%	4.518%
17	13.392	1948	1956	1960	rBV2	3547179	4577121	98.23%	14.721%
18	14.115	2076	2079	2086	rVB2	38219	49816	1.07%	0.160%
19	14.545	2149	2152	2160	rVB4	36329	53300	1.14%	0.171%
20	14.662	2167	2172	2177	rBV	1220845	1279682	27.46%	4.116%
21	16.292	2444	2449	2456	rVB	785364	991762	21.28%	3.190%


Sum of corrected areas: 31091420

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
Data File : BF093956.D
Acq On : 27 Mar 2017 21:50
Operator : SJ/MA
Sample : I2409-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PZ-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

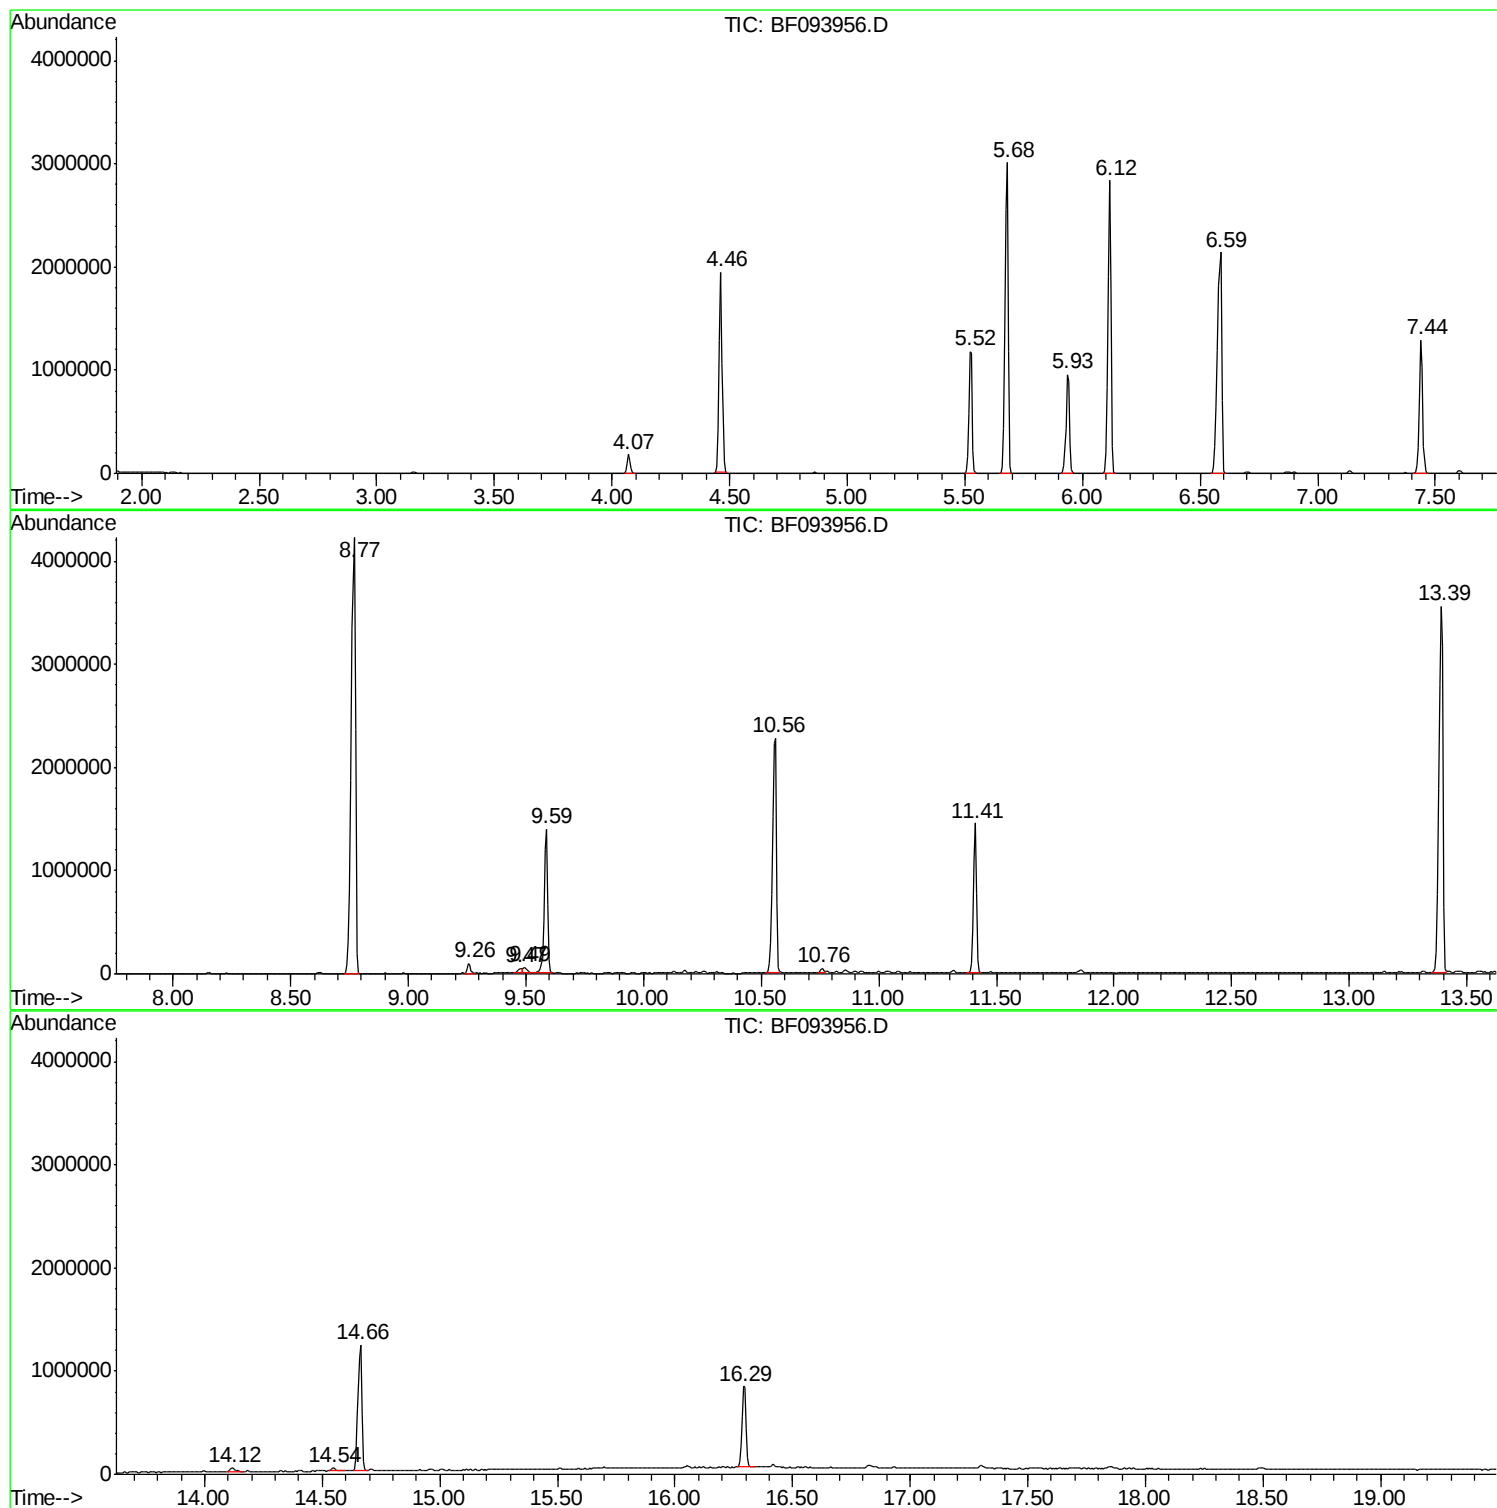

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
Data File : BF093956.D
Acq On : 27 Mar 2017 21:50
Operator : SJ/MA
Sample : I2409-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PZ-3










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.07	3.71 ng	174888	1,4-Dichlorobenzene-d4	5.93

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	25		
3	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	23		
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		
5	Butane	58	C4H10	000106-97-8	9		

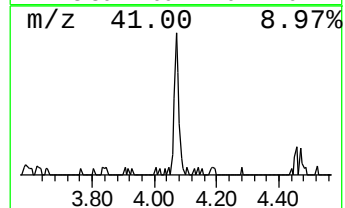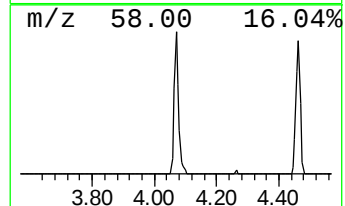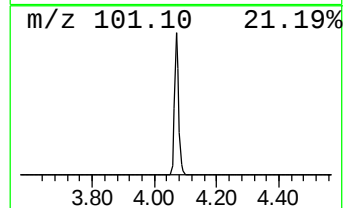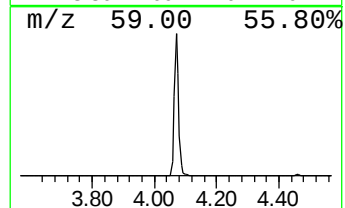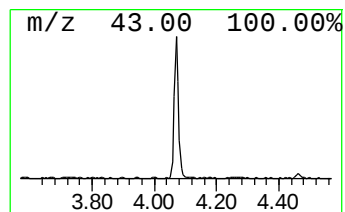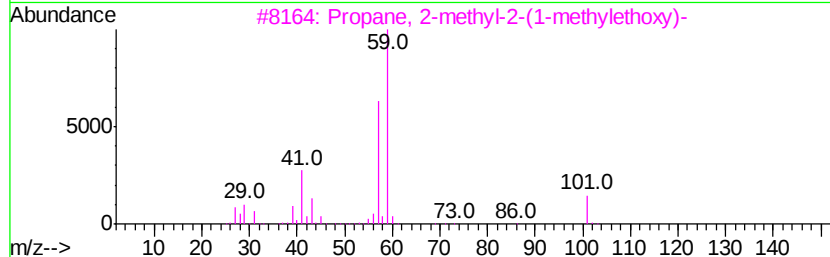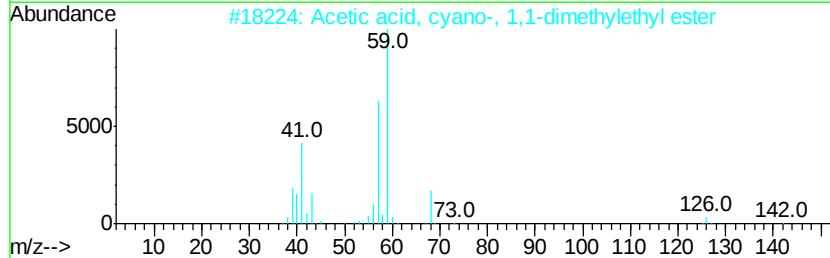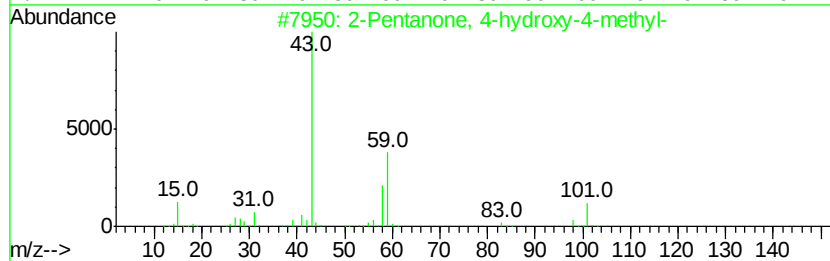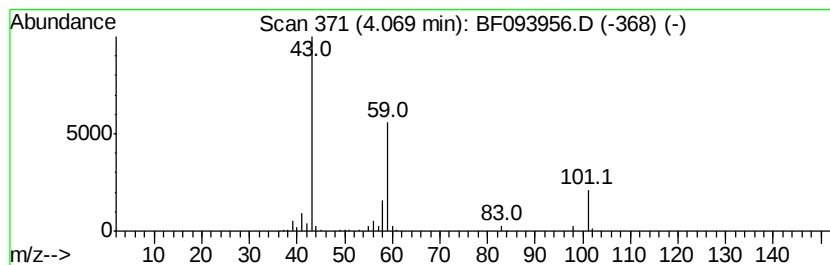

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032717\
Data File : BF093956.D
Acq On : 27 Mar 2017 21:50
Operator : SJ/MA
Sample : I2409-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PZ-3










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown5.68 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.68	65.15 ng	3072270	1,4-Dichlorobenzene-d4	5.93

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

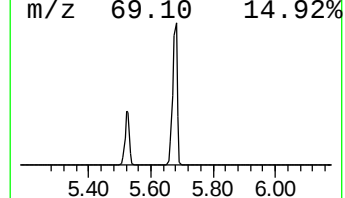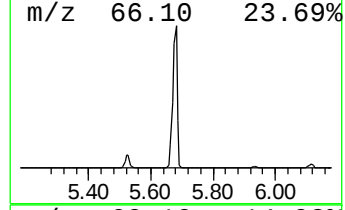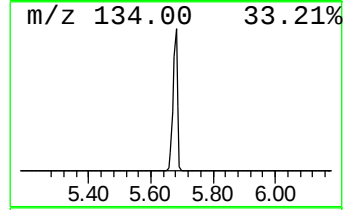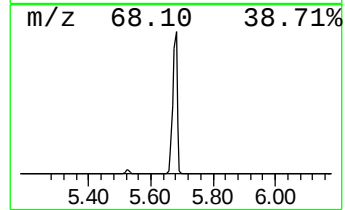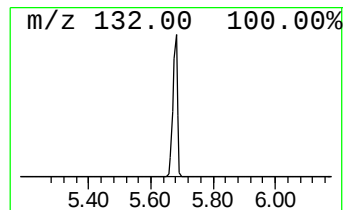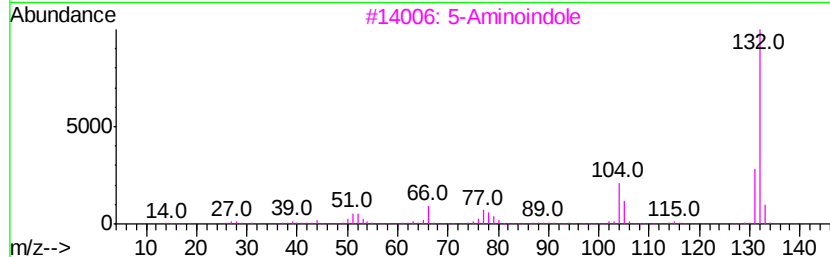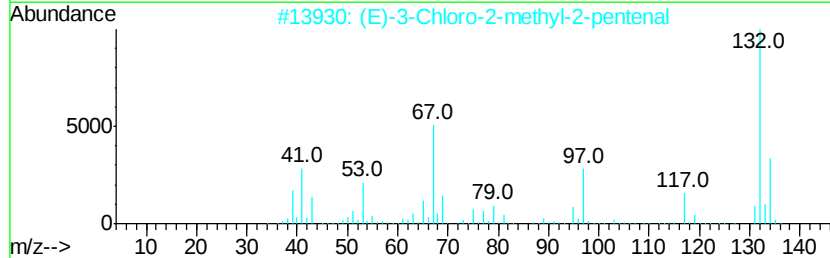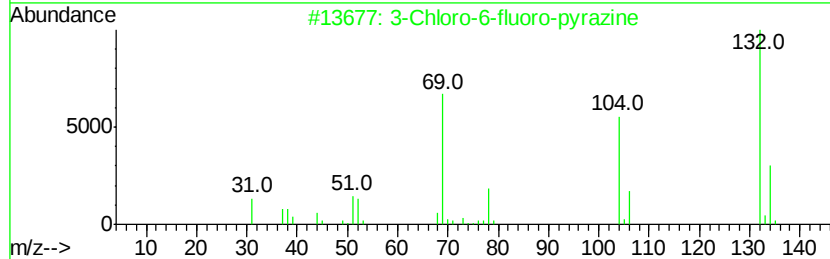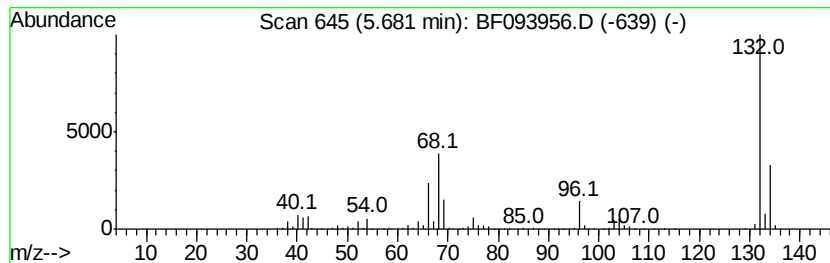

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
Data File : BF093956.D
Acq On : 27 Mar 2017 21:50
Operator : SJ/MA
Sample : I2409-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PZ-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.07	3.7	ng	174888	1	5.93	943130	20.0
unknown5.68	5.68	65.2	ng	3072270	1	5.93	943130	20.0