

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
 Data File : BF093978.D
 Acq On : 28 Mar 2017 7:57
 Operator : SJ/MA
 Sample : I2387-01
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 032317-PRRT-E-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.075	367	372	383	rVB	454466	517709	9.98%	1.682%
2	4.463	434	438	442	rBV	1997879	1976171	38.10%	6.420%
3	4.857	502	505	513	rVB	90057	83579	1.61%	0.272%
4	5.528	614	619	622	rBV	1481481	1301895	25.10%	4.229%
5	5.681	640	645	648	rBV	3052025	3030582	58.42%	9.845%
6	5.940	684	689	692	rBV	959608	953974	18.39%	3.099%
7	6.116	714	719	723	rBV	3329651	3555889	68.55%	11.551%
8	6.587	792	799	802	rBV	2417603	3012434	58.07%	9.786%
9	7.440	939	944	948	rBV	1344587	1287338	24.82%	4.182%
10	8.769	1163	1170	1173	rBV	4562576	5187426	100.00%	16.851%
11	9.586	1300	1309	1313	rBV	1287969	1363154	26.28%	4.428%
12	10.557	1468	1474	1477	rBV	1869749	1877059	36.18%	6.098%
13	11.410	1614	1619	1623	rVB	1210799	1181320	22.77%	3.837%
14	13.392	1949	1956	1959	rBV	3295070	3842968	74.08%	12.484%
15	14.657	2166	2171	2177	rBV	806175	825606	15.92%	2.682%
16	16.292	2444	2449	2458	rBV2	676824	786664	15.16%	2.555%


Sum of corrected areas: 30783768

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
Data File : BF093978.D
Acq On : 28 Mar 2017 7:57
Operator : SJ/MA
Sample : I2387-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
032317-PRRT-E-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

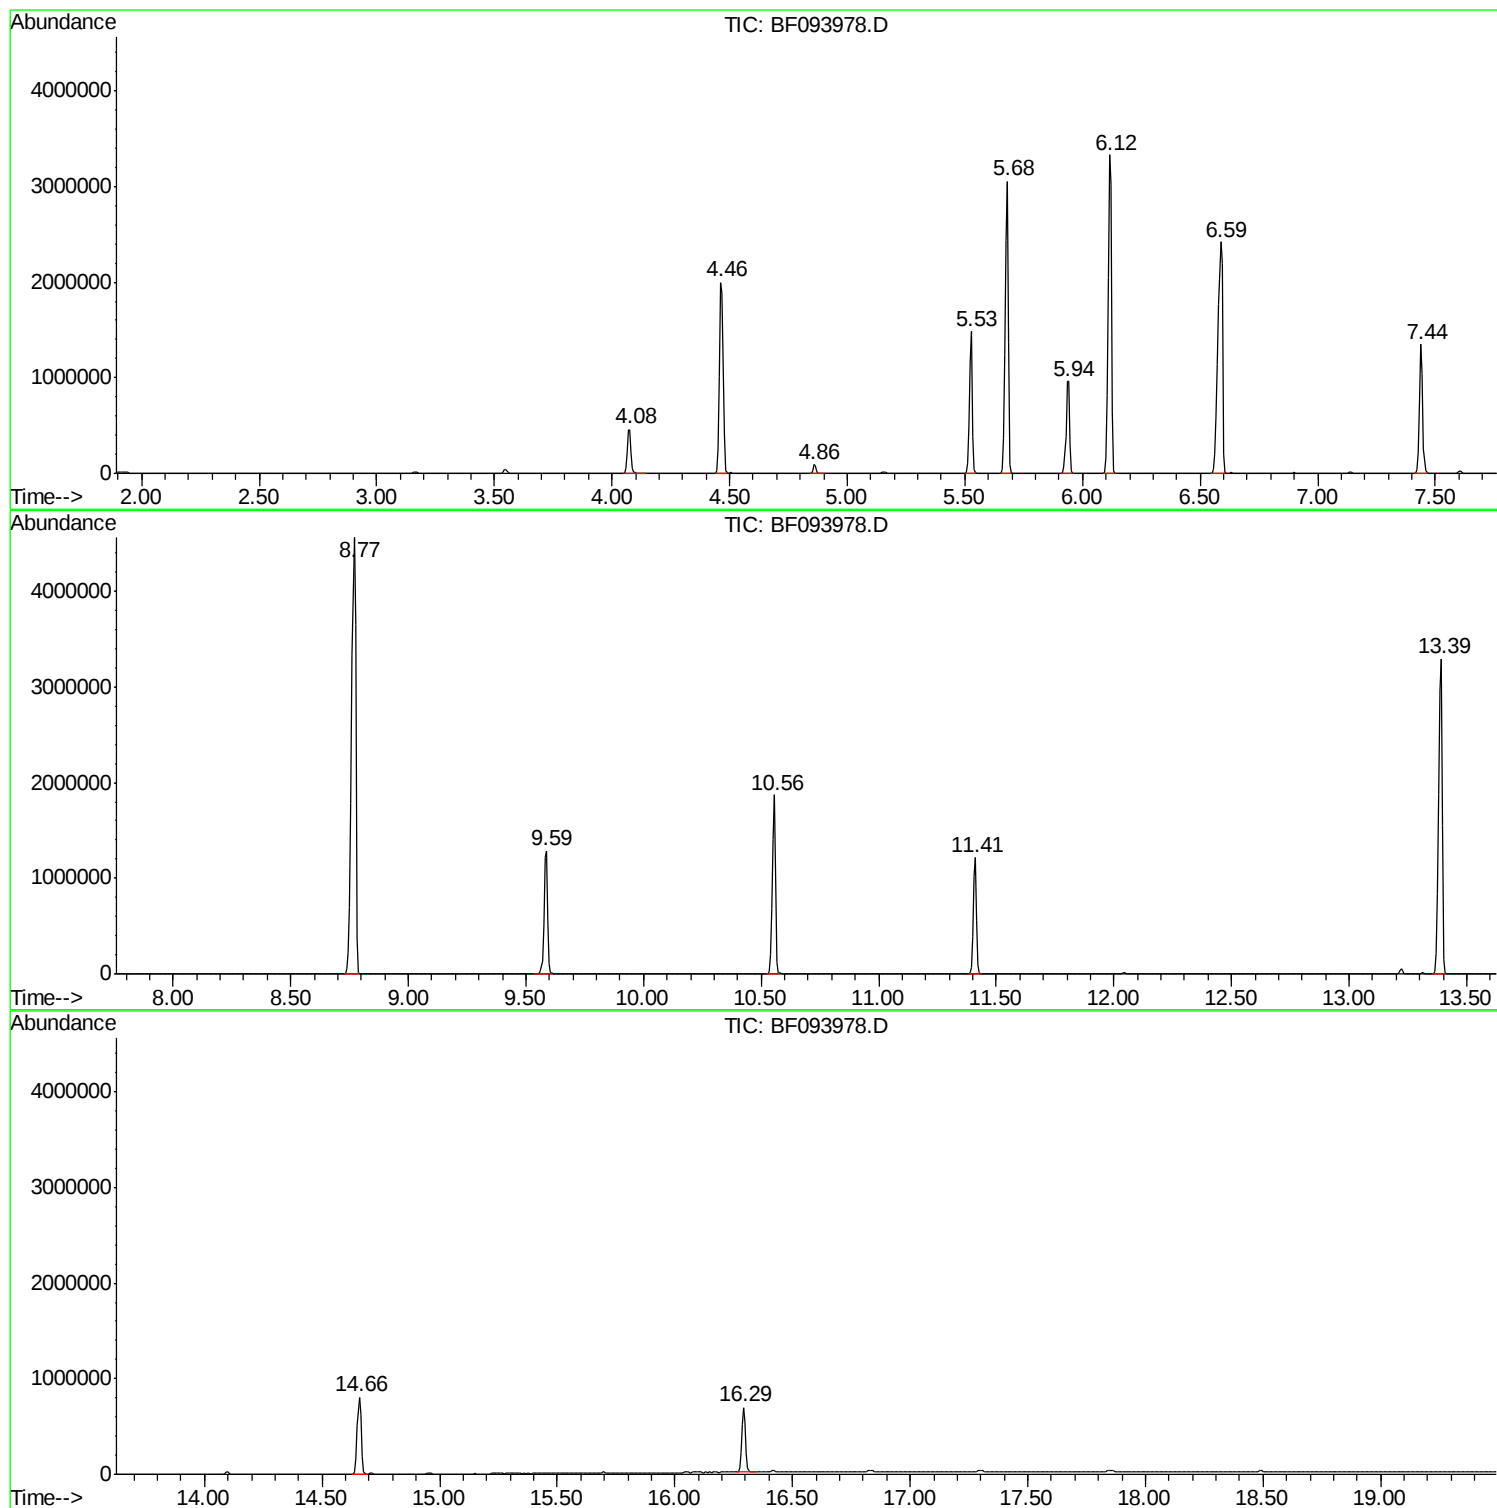

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
Data File : BF093978.D
Acq On : 28 Mar 2017 7:57
Operator : SJ/MA
Sample : I2387-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
032317-PRRT-E-D-M










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.08	10.85 ng	517709	1,4-Dichlorobenzene-d4	5.94

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	50
2			Acetic acid, cyano-, 1,1-dimethyl...	141	C7H11NO2	001116-98-9	23
3			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9
4			Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9
5			Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

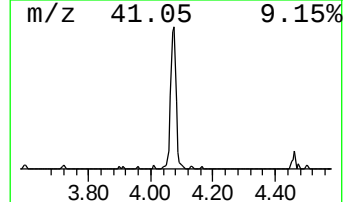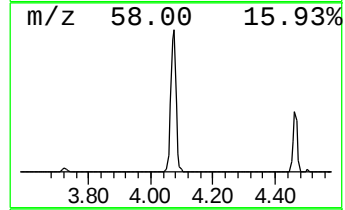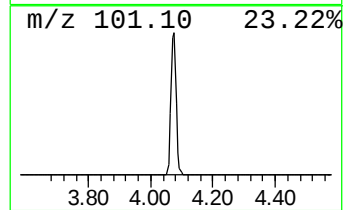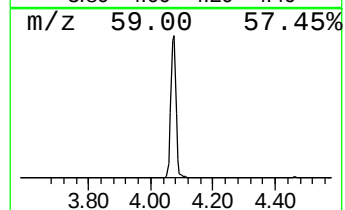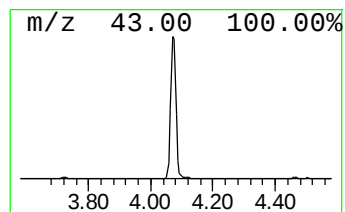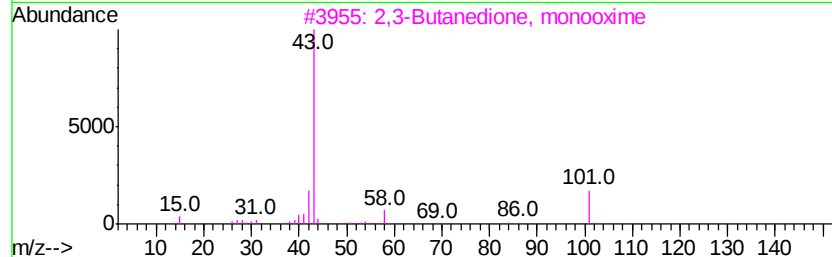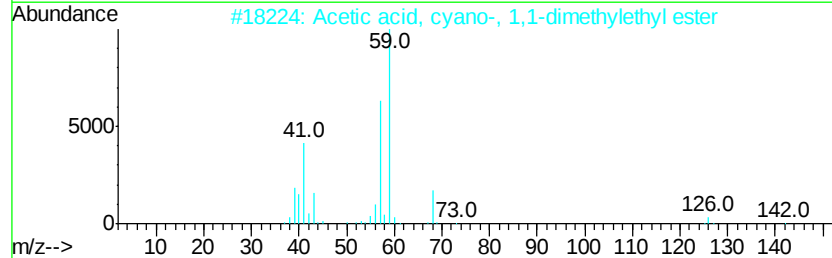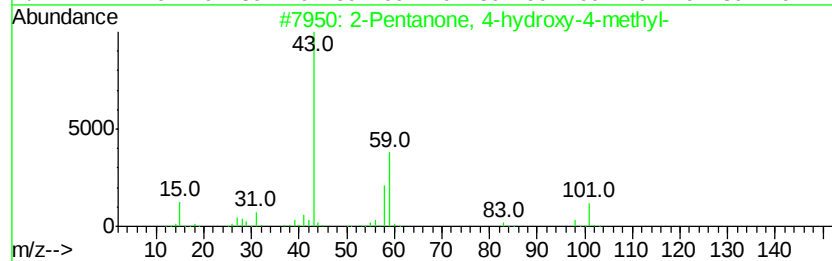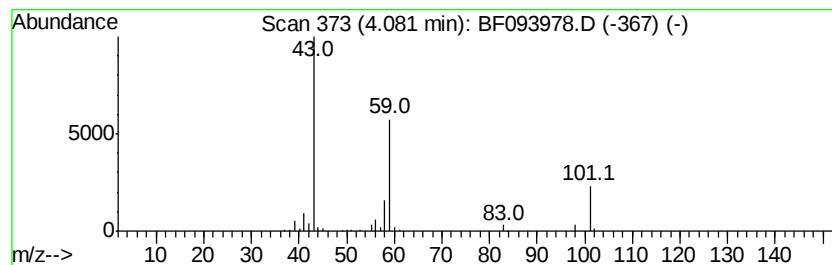

Data Path : Z:\HPCHEM1\BNA F\DATA\BF032717\
Data File : BF093978.D
Acq On : 28 Mar 2017 7:57
Operator : SJ/MA
Sample : I2387-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
032317-PRRT-E-D-M









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown5.68 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.68	63.54 ng	3030580	1,4-Dichlorobenzene-d4	5.94

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
5		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9

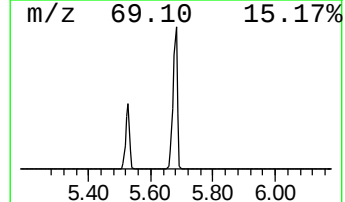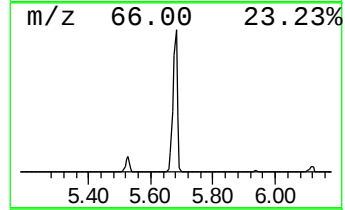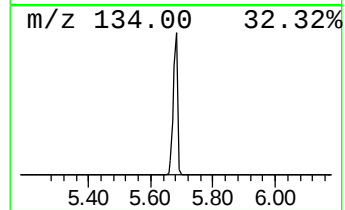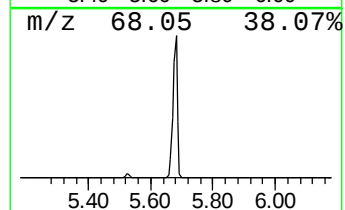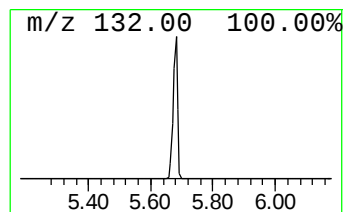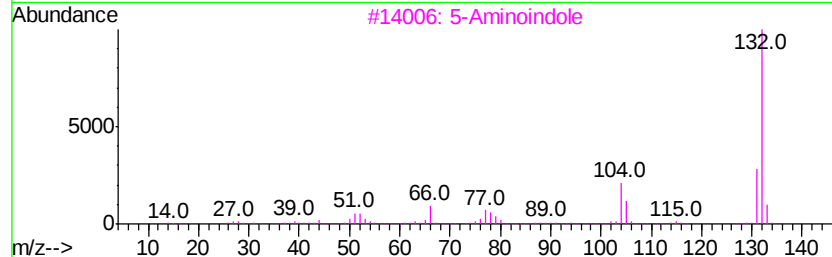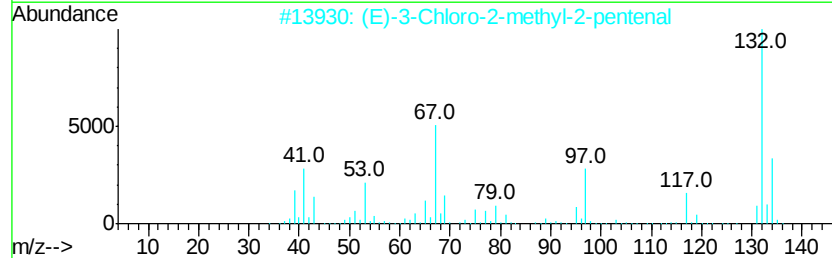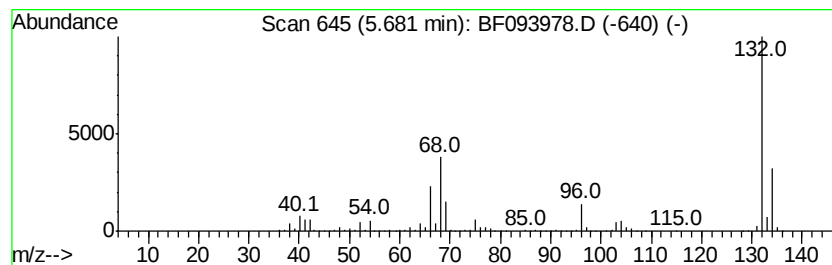

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032717\
Data File : BF093978.D
Acq On : 28 Mar 2017 7:57
Operator : SJ/MA
Sample : I2387-01
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
032317-PRRT-E-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.08	10.9	ng	517709	1	5.94	953974	20.0
unknown5.68	5.68	63.5	ng	3030580	1	5.94	953974	20.0