


Data Path : Z:\HPCHEM1\BNA_F\Data\BF032717\
 Data File : BF093937.D
 Acq On : 27 Mar 2017 11:38
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

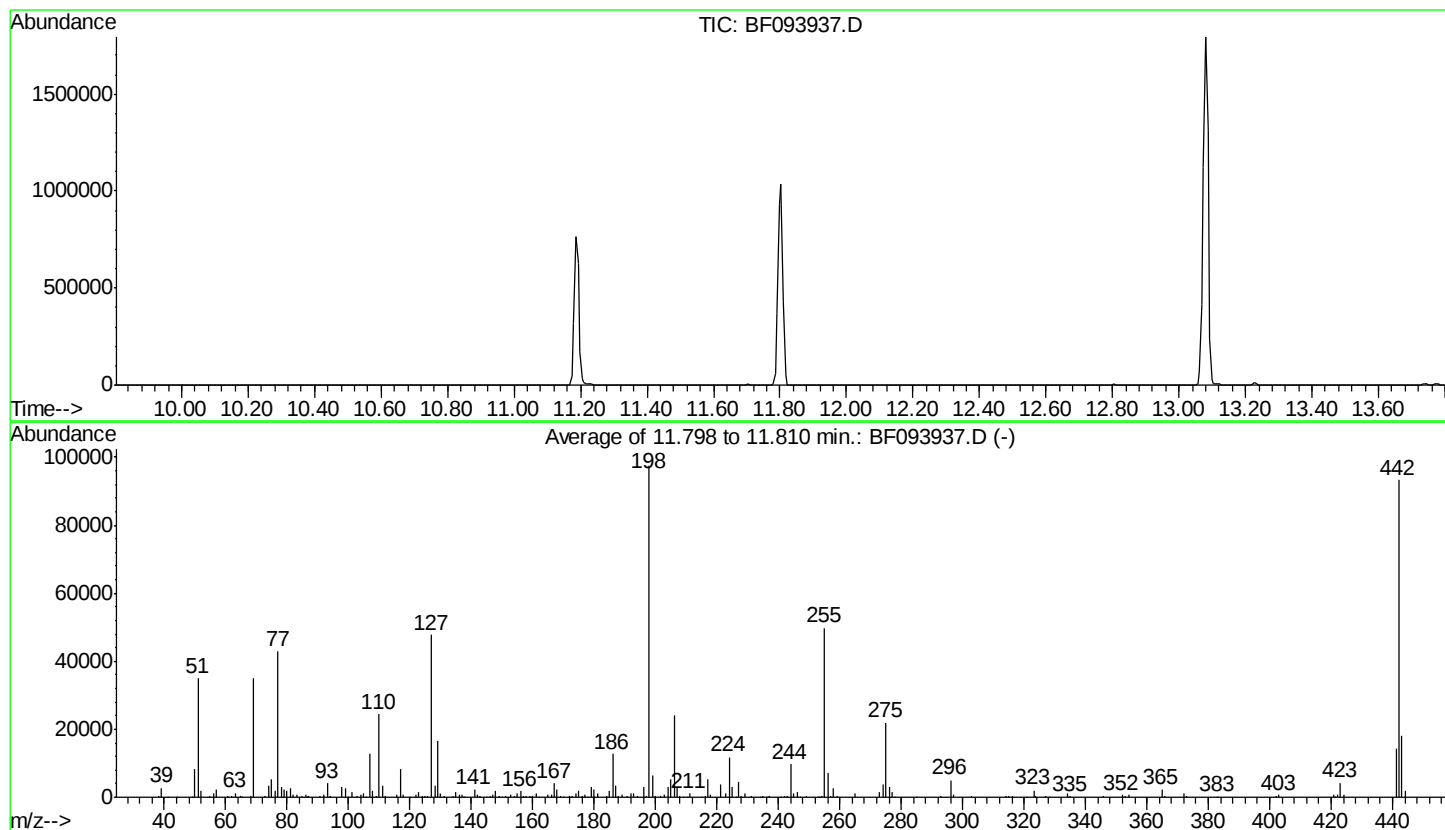

AutoFind: Scans 1685, 1686, 1687; Background Corrected with Scan 1679

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	34900	PASS
68	69	0.00	2	1.6	562	PASS
69	198	0.00	100	36.0	35087	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.9	47712	PASS
197	198	0.00	2	0.6	541	PASS
198	198	100	100	100.0	97552	PASS
199	198	5	9	6.6	6459	PASS
275	198	10	60	22.4	21882	PASS
365	198	1	100	2.3	2246	PASS
441	442	0.01	24	15.6	14501	PASS
442	198	50	100	95.6	93224	PASS
443	442	15	24	19.4	18109	PASS