


Data Path : Z:\HPCHEM1\BNA F\Data\BF032717\
 Data File : BF093973.D
 Acq On : 28 Mar 2017 5:39
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 27 16:10:49 2017

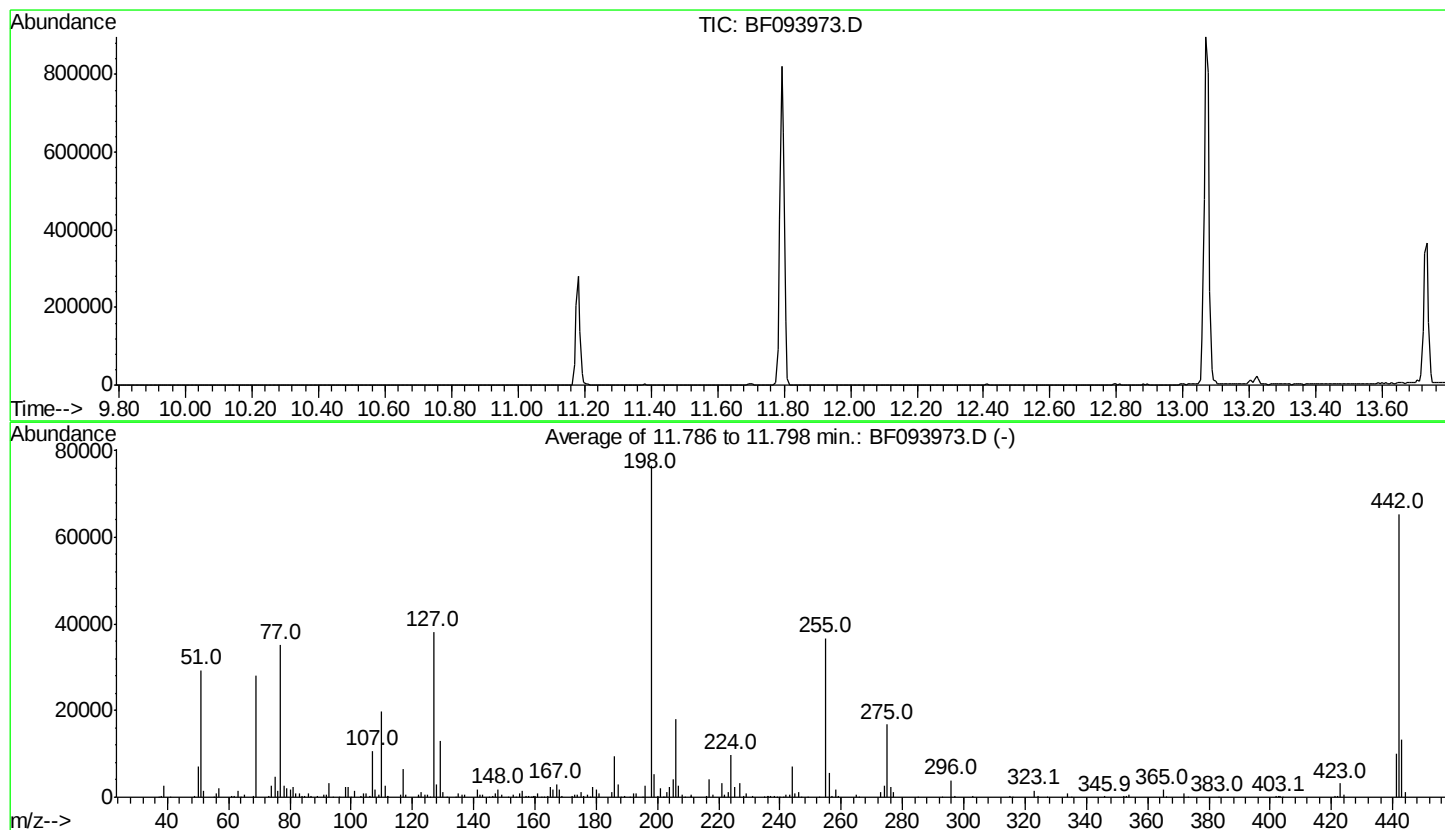

AutoFind: Scans 1683, 1684, 1685; Background Corrected with Scan 1678

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.4	29370	PASS
68	69	0.00	2	1.6	441	PASS
69	198	0.00	100	36.6	28010	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	38221	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	76490	PASS
199	198	5	9	7.1	5393	PASS
275	198	10	60	21.9	16788	PASS
365	198	1	100	2.2	1667	PASS
441	442	0.01	24	15.5	10123	PASS
442	198	50	100	85.5	65370	PASS
443	442	15	24	20.3	13281	PASS