


Data Path : Z:\HPCHEM1\BNA F\Data\BF032718\
 Data File : BF103969.D
 Acq On : 27 Mar 2018 14:06
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF031518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 23 13:26:17 2018

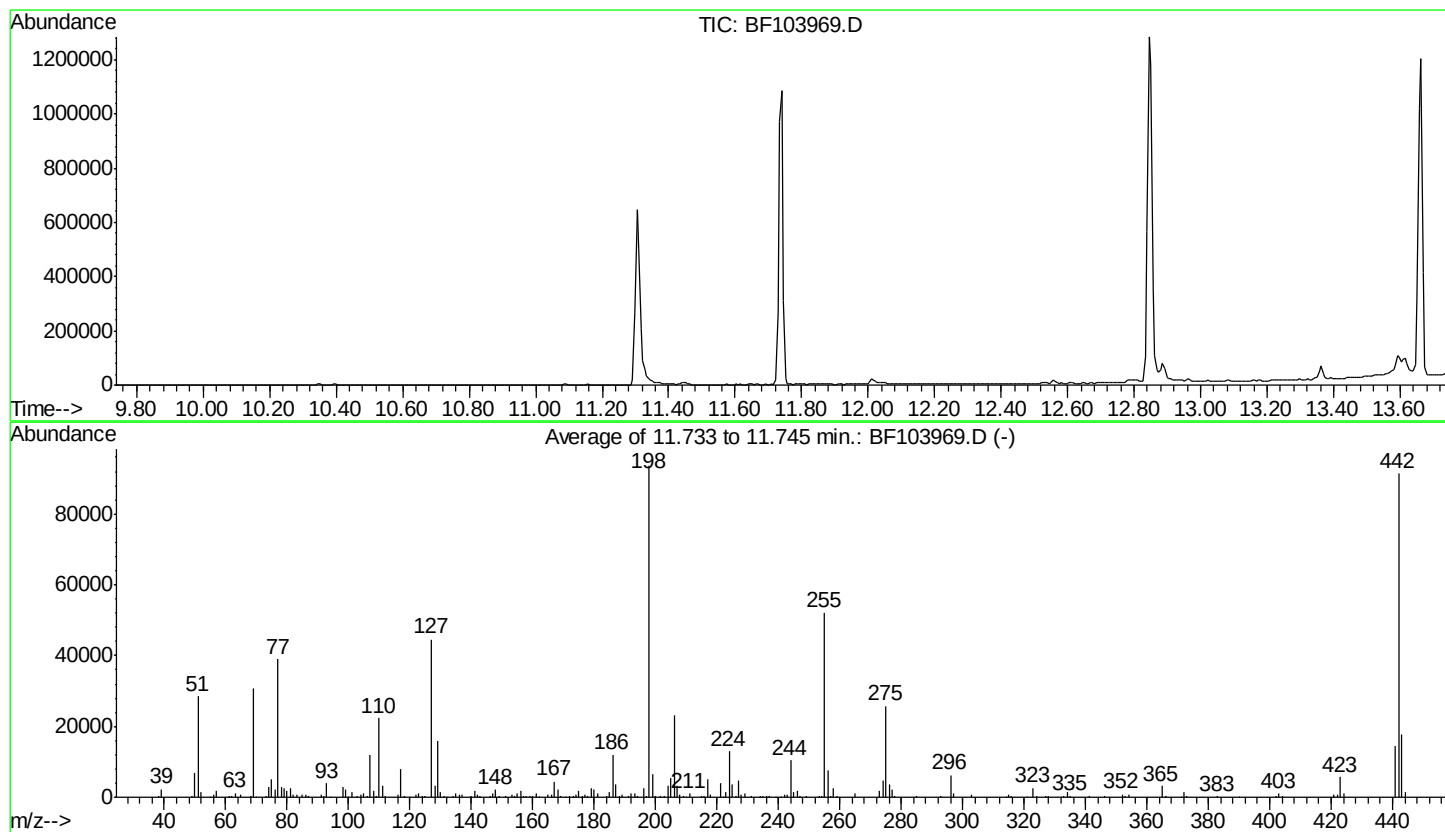

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.4	28452	PASS
68	69	0.00	2	1.7	538	PASS
69	198	0.00	100	33.0	30881	PASS
70	69	0.00	2	0.4	117	PASS
127	198	10	80	47.6	44586	PASS
197	198	0.00	2	0.4	353	PASS
198	198	100	100	100.0	93653	PASS
199	198	5	9	7.0	6578	PASS
275	198	10	60	27.5	25757	PASS
365	198	1	100	3.4	3143	PASS
441	443	0.01	100	80.5	14302	PASS
442	198	50	100	97.8	91560	PASS
443	442	15	24	19.4	17766	PASS