
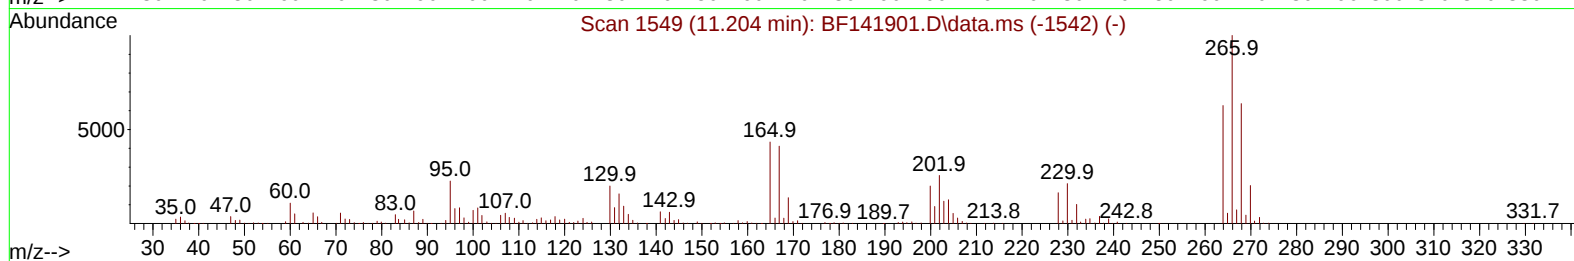
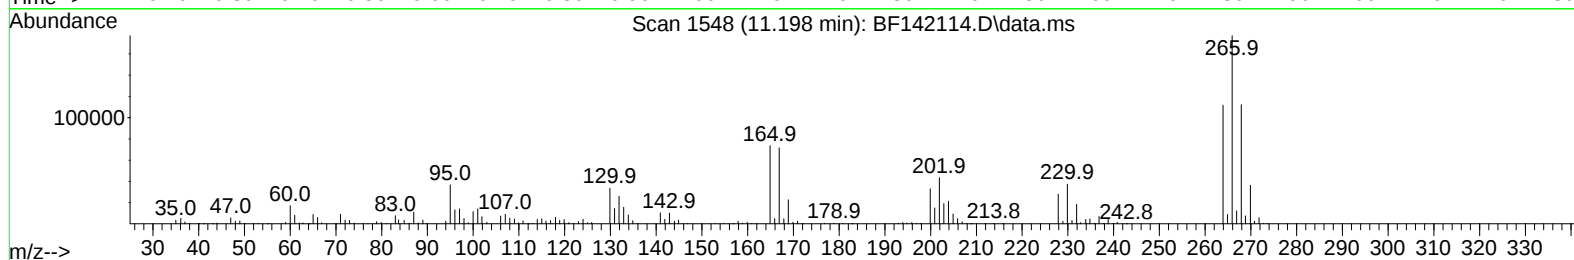


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142114.D
Acq On : 27 Mar 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 12:35:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

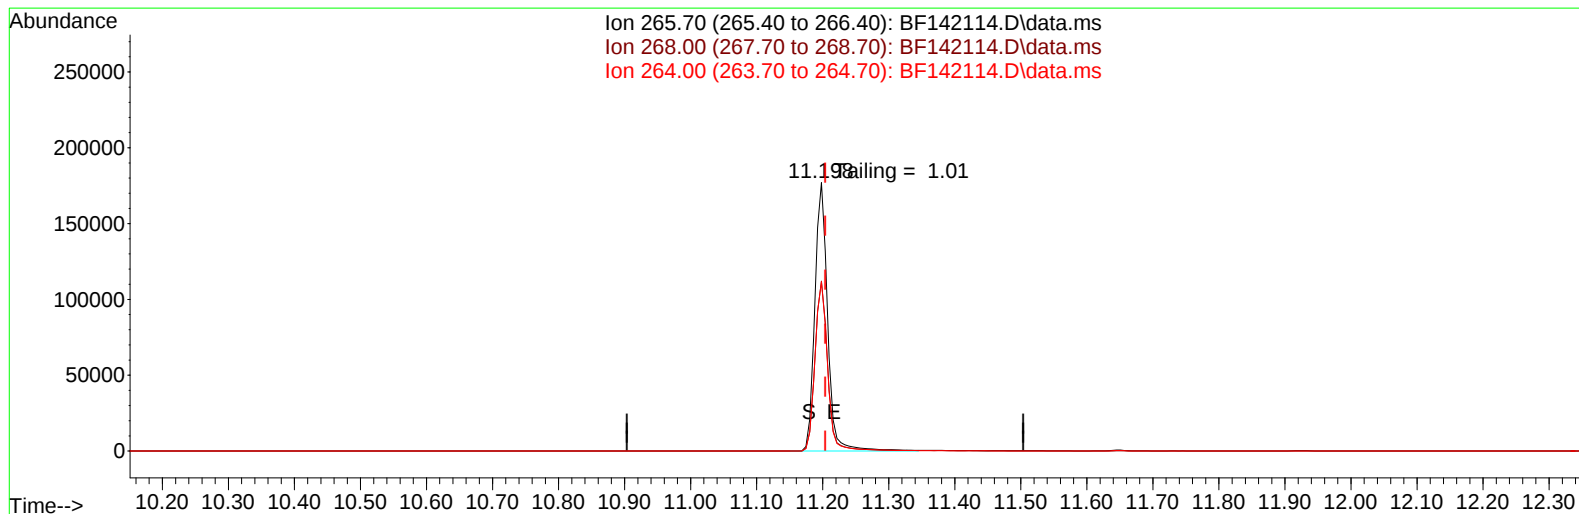

TIC: BF142114.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.006) 17376.35 ng

response 239487

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.35
264.00	62.70	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142114.D
Acq On : 27 Mar 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 27 12:35:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

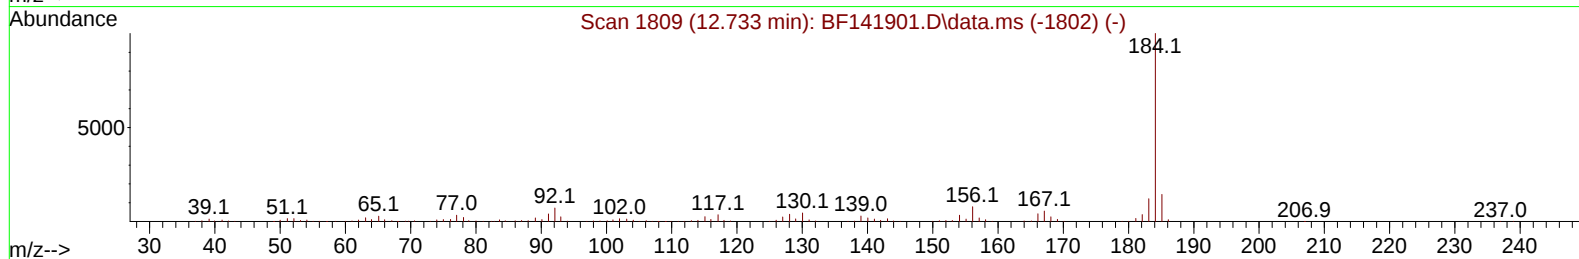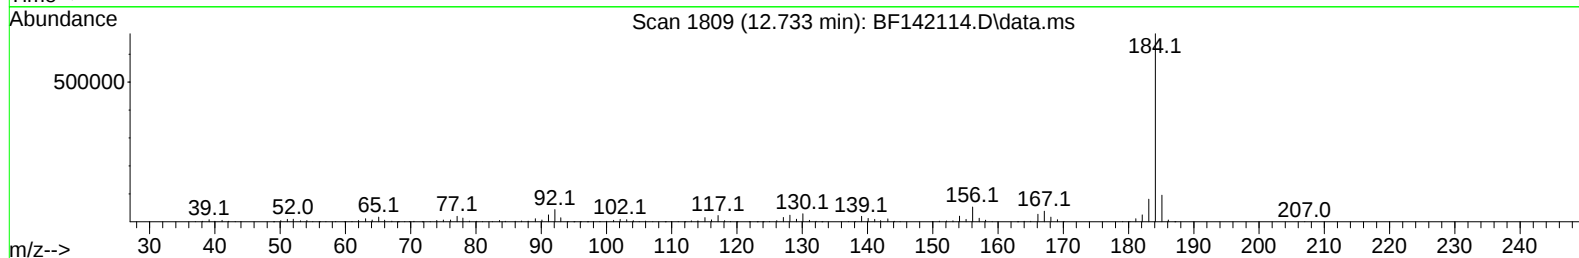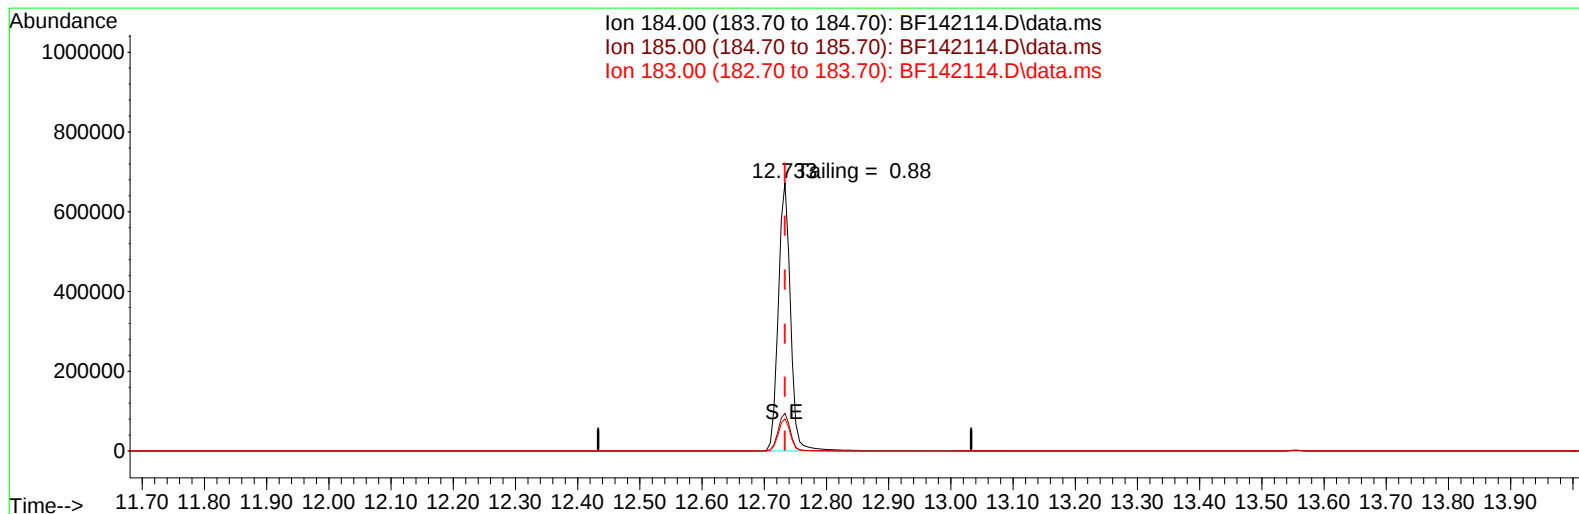

TIC: BF142114.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 49001.38 ng

response 921576

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.11
183.00	12.10	12.04
0.00	0.00	0.00