

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
 Data File : BF142118.D
 Acq On : 27 Mar 2025 11:02
 Operator : RC/JU
 Sample : PB167326BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB167326BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF142118.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.187	8	16	26	rVB	41511	73526	1.17%	0.237%
2	5.493	571	578	583	rBV	2685870	3671390	58.22%	11.831%
3	6.498	742	749	754	rBV	2414343	3584189	56.84%	11.550%
4	6.869	807	812	824	rBV	588838	729492	11.57%	2.351%
5	7.434	901	908	943	rBV	1761874	2502897	39.69%	8.065%
6	8.151	1024	1030	1049	rBV	721012	974877	15.46%	3.141%
7	9.228	1207	1213	1218	rBV	4114137	5331427	84.54%	17.180%
8	9.904	1323	1328	1352	rBV	871184	1191858	18.90%	3.841%
9	10.698	1457	1463	1487	rBV	2896606	3819088	60.56%	12.307%
10	11.392	1576	1581	1599	rBV	926998	1245394	19.75%	4.013%
11	12.980	1845	1851	1857	rBV	4726291	6306106	100.00%	20.321%
12	14.033	2025	2030	2046	rBV	603286	821411	13.03%	2.647%
13	15.510	2274	2281	2293	rBV	461970	780846	12.38%	2.516%




Sum of corrected areas: 31032501

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142118.D
Acq On : 27 Mar 2025 11:02
Operator : RC/JU
Sample : PB167326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167326BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

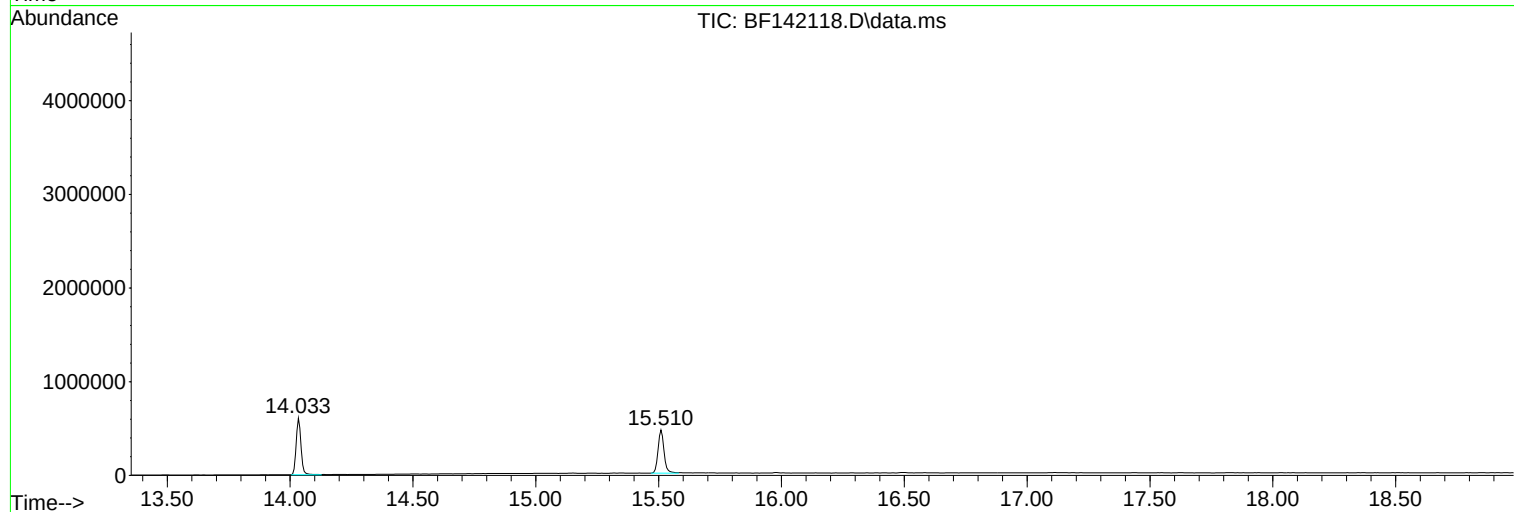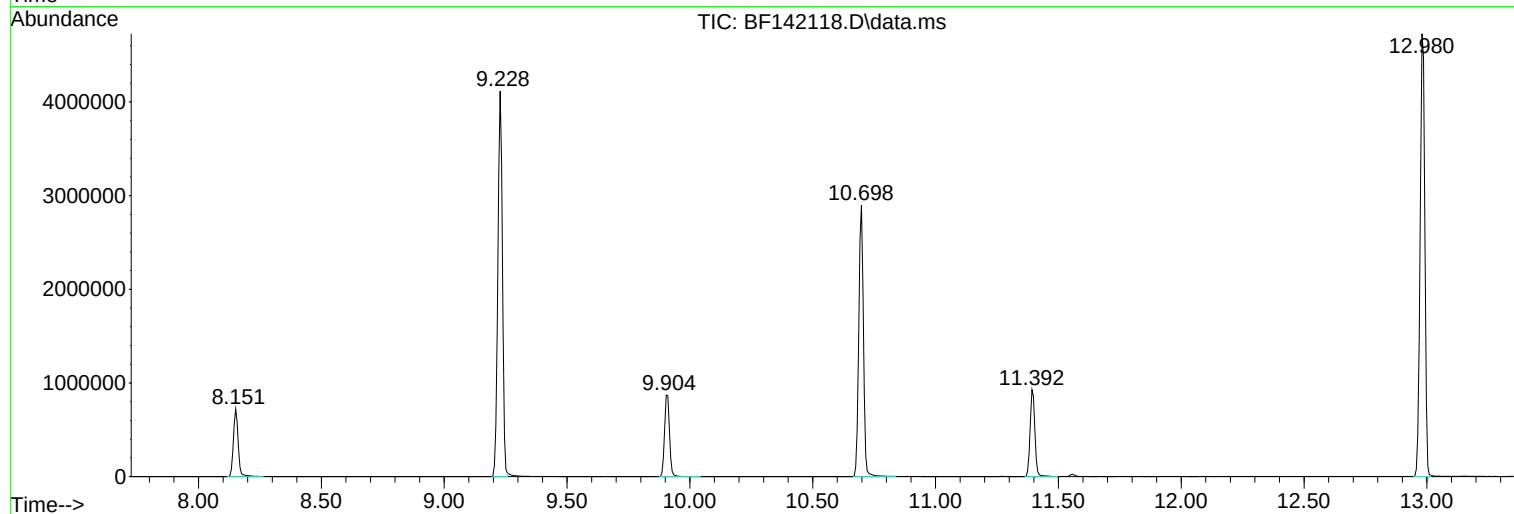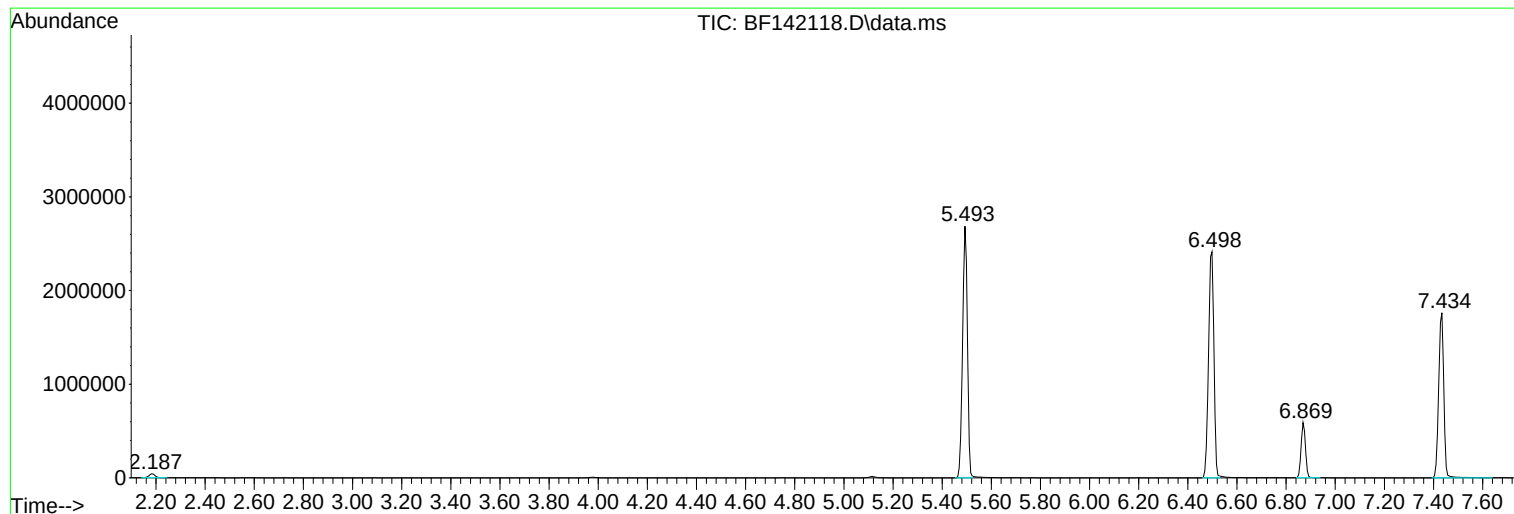

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142118.D
Acq On : 27 Mar 2025 11:02
Operator : RC/JU
Sample : PB167326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167326BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.187	2.02 ng	73526	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	36
3			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	32
4			Octanal, 7-methoxy-3,7-dimethyl-	186	C11H22O2	003613-30-7	25
5			3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	17

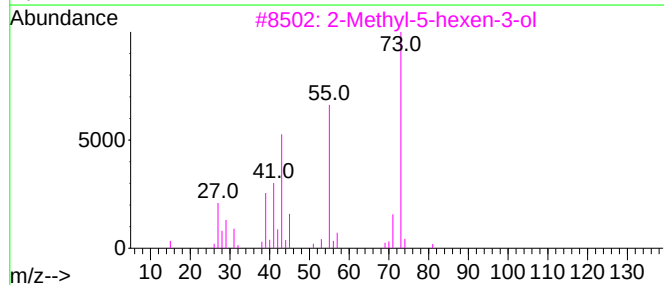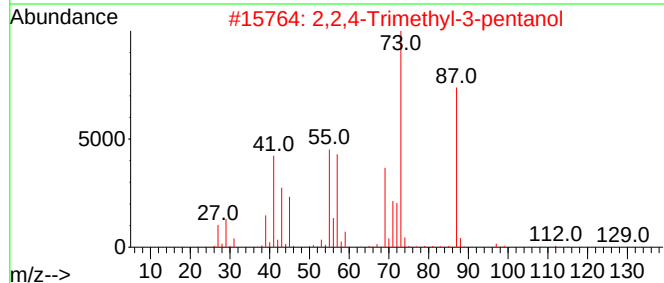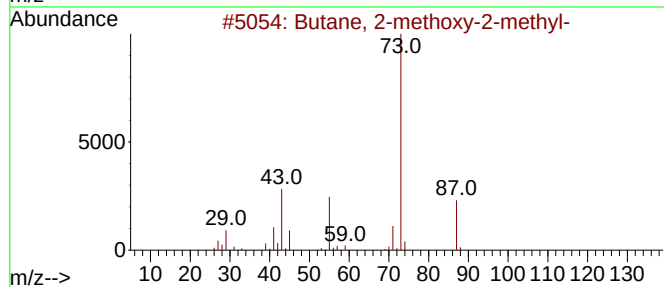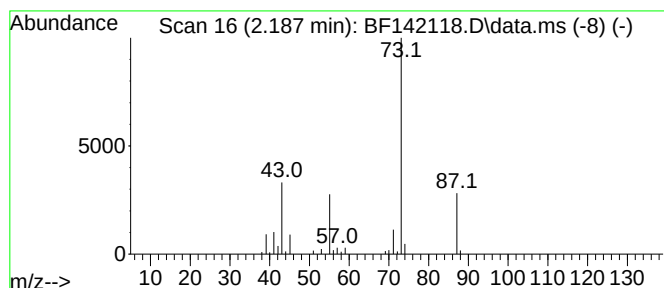

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142118.D
Acq On : 27 Mar 2025 11:02
Operator : RC/JU
Sample : PB167326BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB167326BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.187	2.0	ng	73526	1	6.869	729492	20.0