
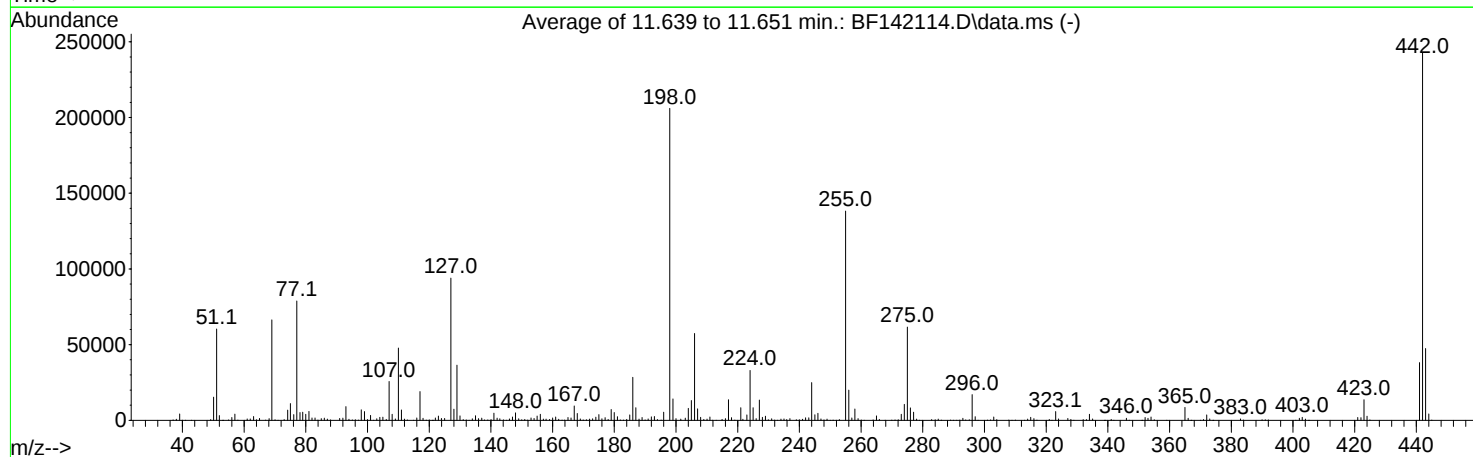


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142114.D
Acq On : 27 Mar 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

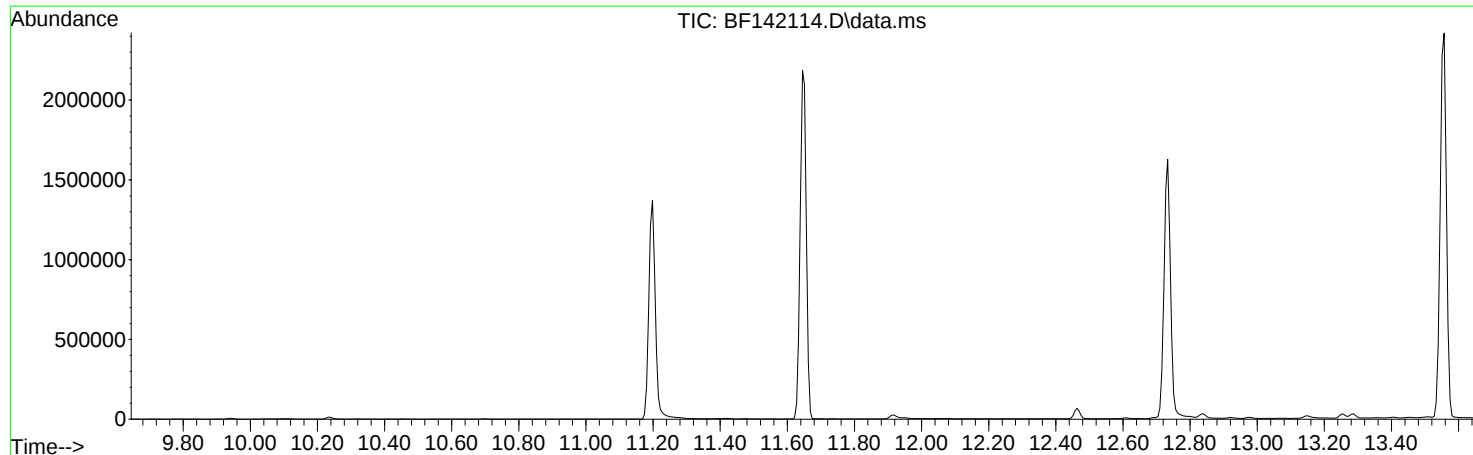

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.3	60355	PASS
68	69	0.00	2	1.8	1201	PASS
69	198	0.00	100	32.2	66315	PASS
70	69	0.00	2	0.6	423	PASS
127	198	10	80	45.6	93891	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	206016	PASS
199	198	5	9	6.9	14187	PASS
275	198	10	60	29.9	61624	PASS
365	198	1	100	4.1	8525	PASS
441	198	0.01	100	18.5	38120	PASS
442	442	50	100	100.0	242923	PASS
443	442	15	24	19.5	47427	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/27/2025	BNA_F	<u>BF142114.D</u>
Compound Name	Response	Retention Time
DDT	643663	13.557
DDD	15818	13.257
DDE	1255	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17073	660736	2.58

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142114.D
Acq On : 27 Mar 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 27 12:35:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

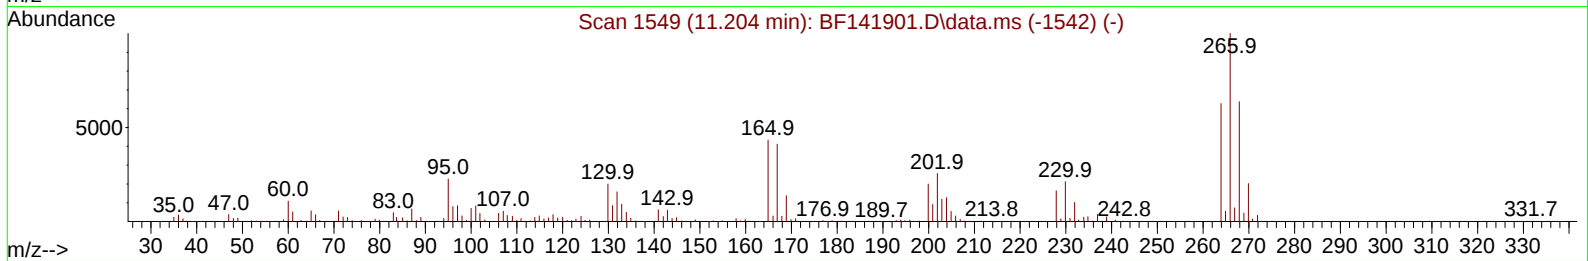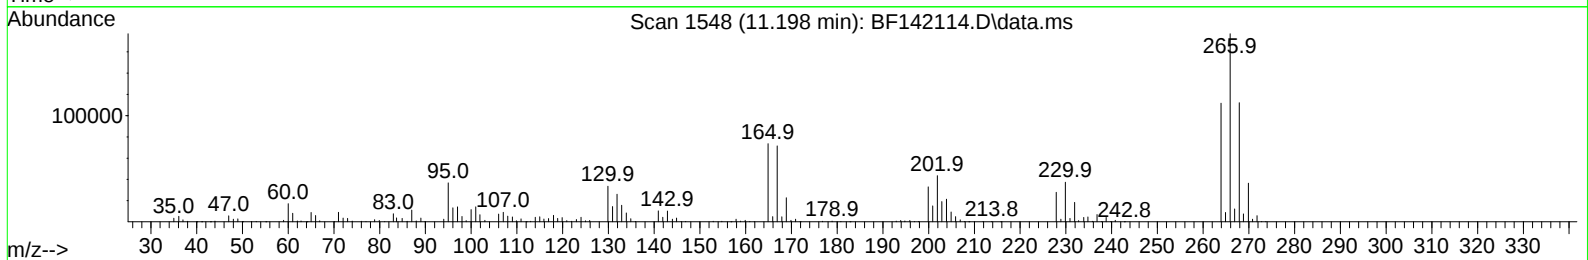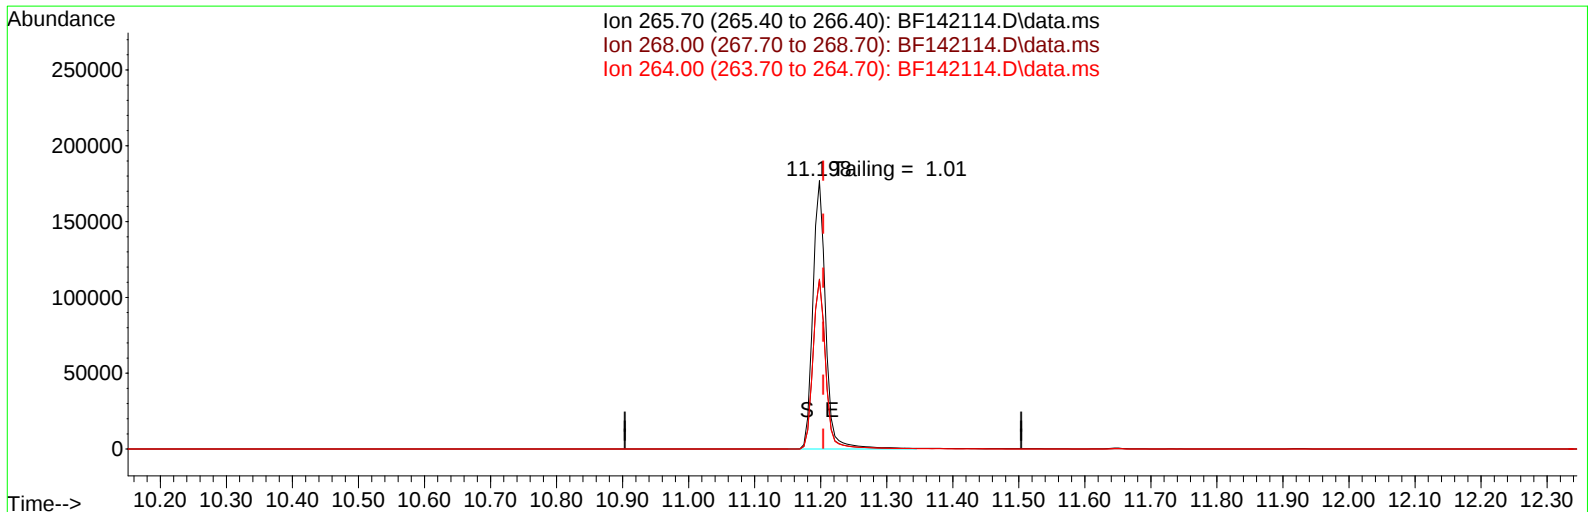

TIC: BF142114.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 17376.35 ng




response 239487

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.35
264.00	62.70	63.09
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142114.D
Acq On : 27 Mar 2025 09:04
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 27 12:35:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

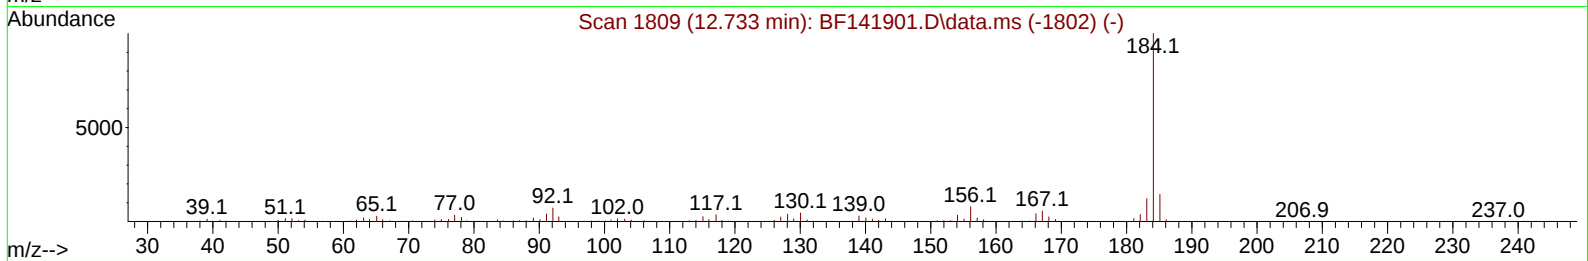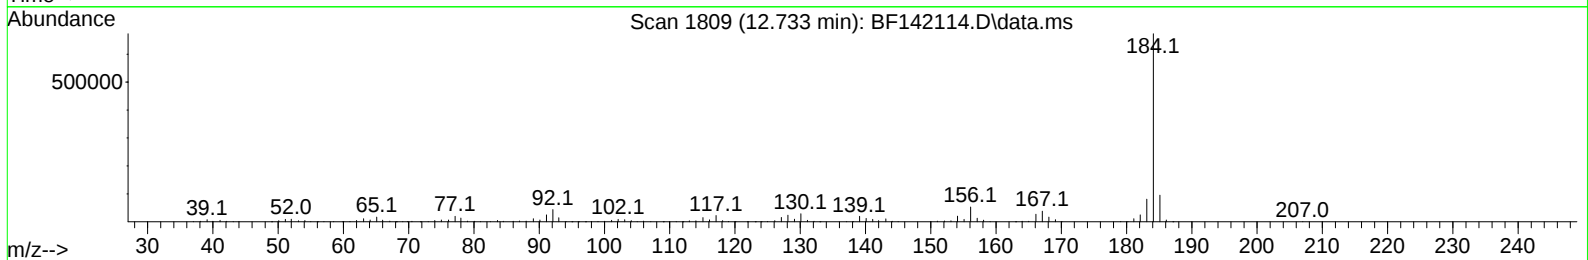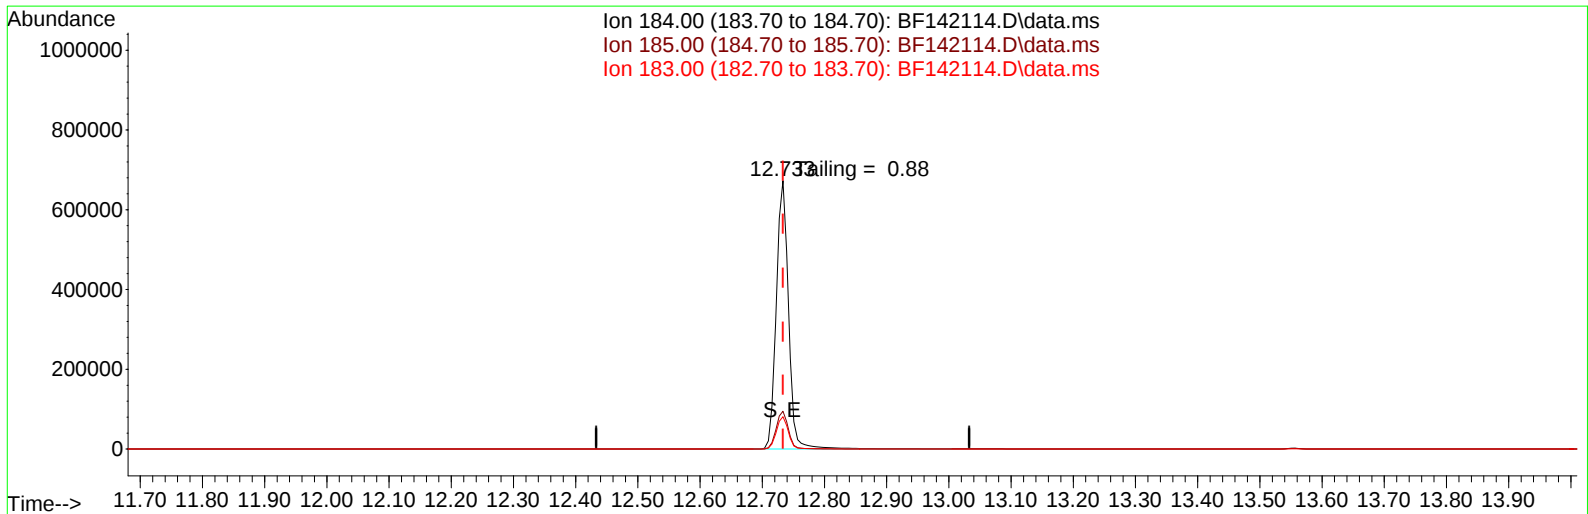

TIC: BF142114.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 49001.38 ng

response 921576

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.11
183.00	12.10	12.04
0.00	0.00	0.00