


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142126.D
Acq On : 27 Mar 2025 15:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Mar 10 15:46:22 2025

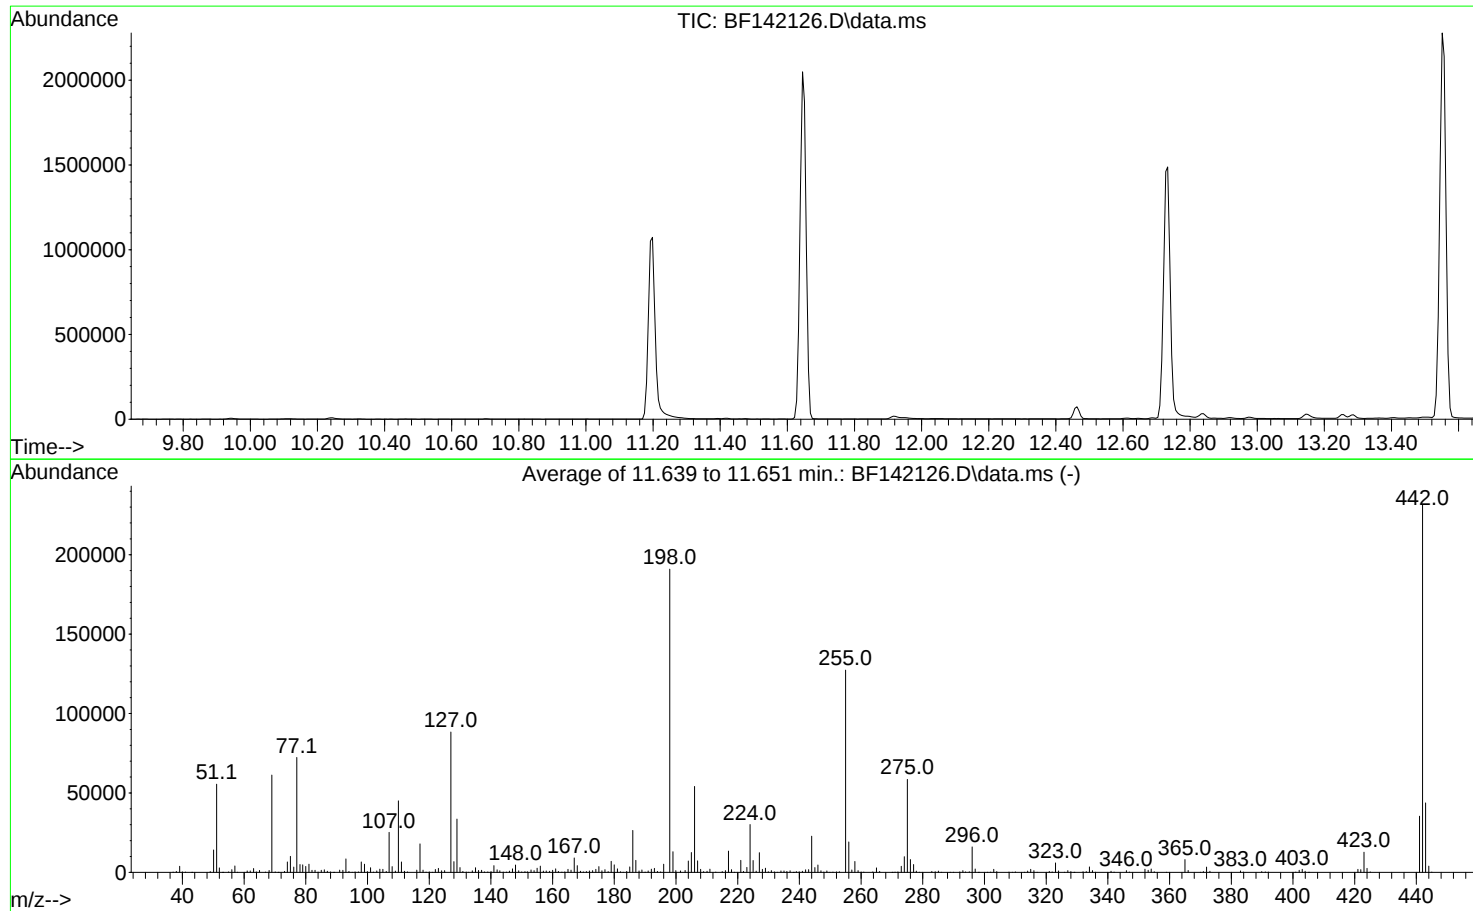

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	55525	PASS
68	69	0.00	2	2.0	1195	PASS
69	198	0.00	100	32.1	61269	PASS
70	69	0.00	2	0.6	345	PASS
127	198	10	80	46.3	88307	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	190891	PASS
199	198	5	9	6.8	13020	PASS
275	198	10	60	30.7	58581	PASS
365	198	1	100	4.2	8040	PASS
441	198	0.01	100	18.5	35333	PASS
442	442	50	100	100.0	231616	PASS
443	442	15	24	18.9	43752	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/27/2025	BNA_F	<u>BF142126.D</u>
Compound Name	Response	Retention Time
DDT	603372	13.551
DDD	13482	13.257
DDE	1561	12.916
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15043	618415	2.43

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142126.D
Acq On : 27 Mar 2025 15:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 27 16:42:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

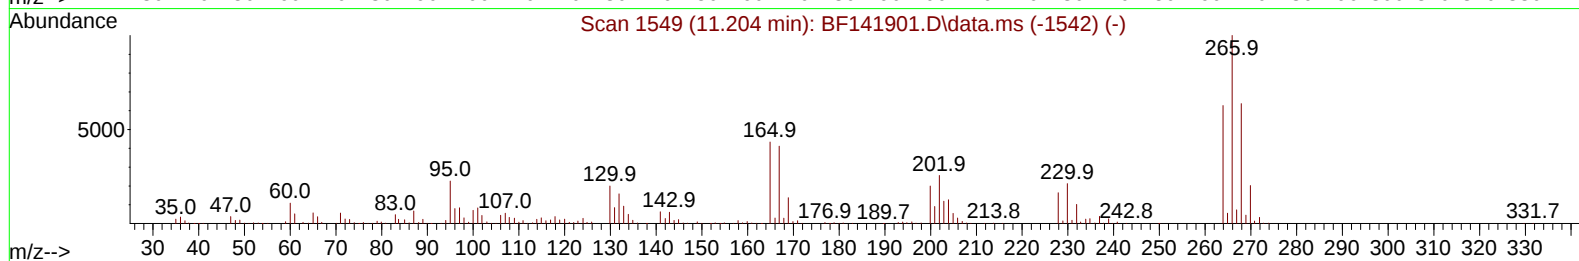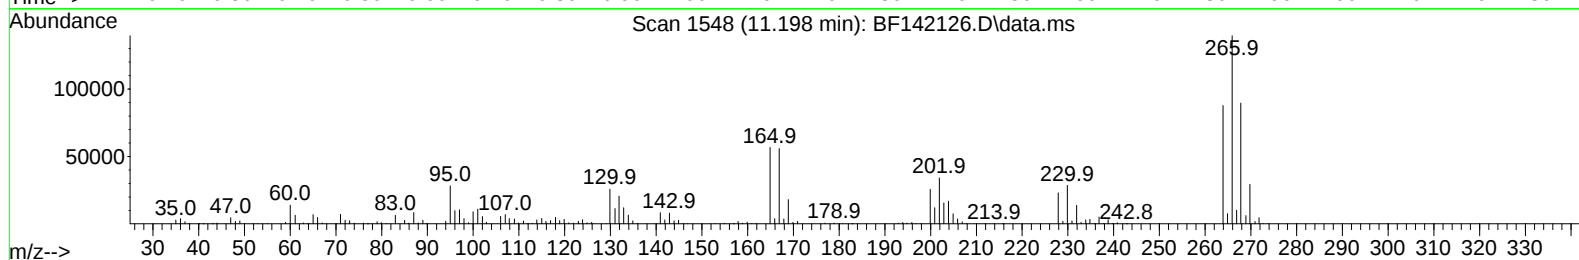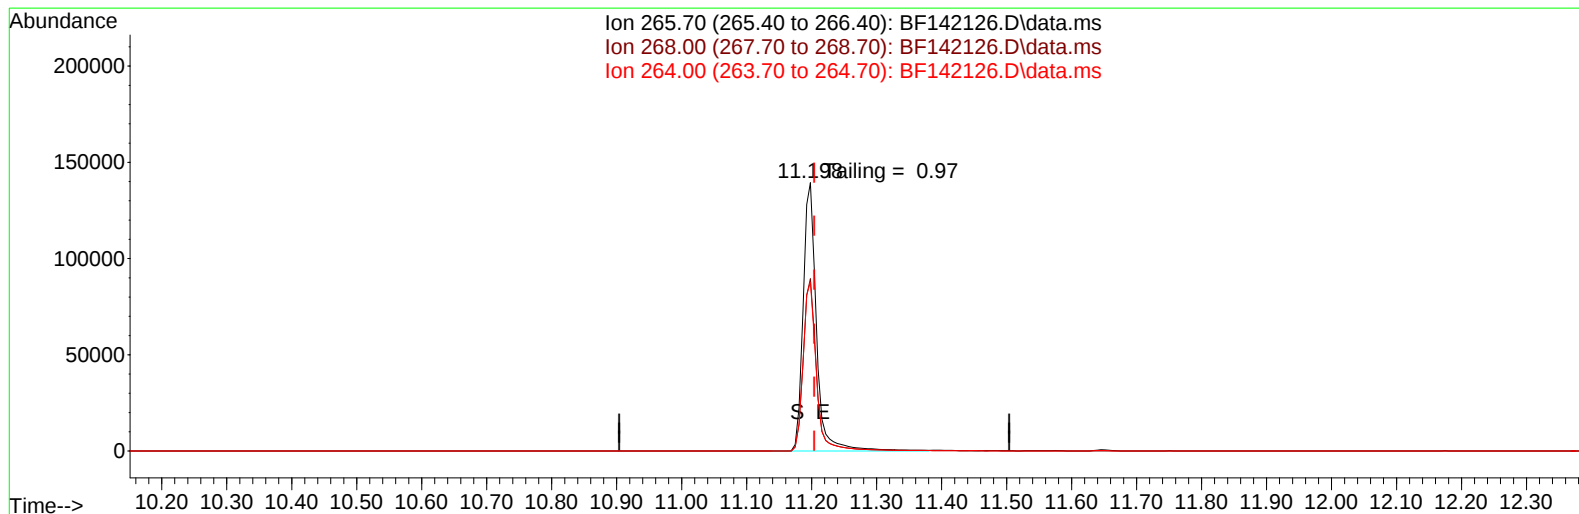

TIC: BF142126.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.006) 14307.77 ng




response 200959

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	64.21
264.00	62.70	62.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF032725\
Data File : BF142126.D
Acq On : 27 Mar 2025 15:41
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 27 16:42:14 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF031025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 10 15:46:22 2025
Response via : Initial Calibration

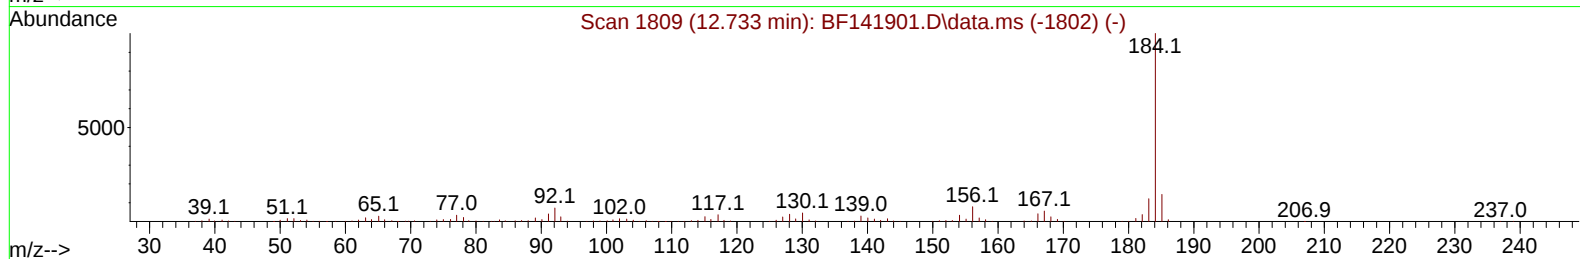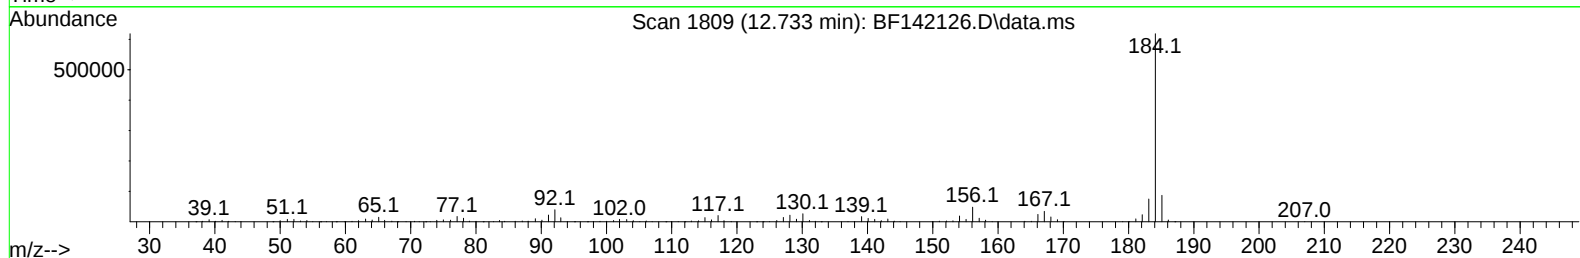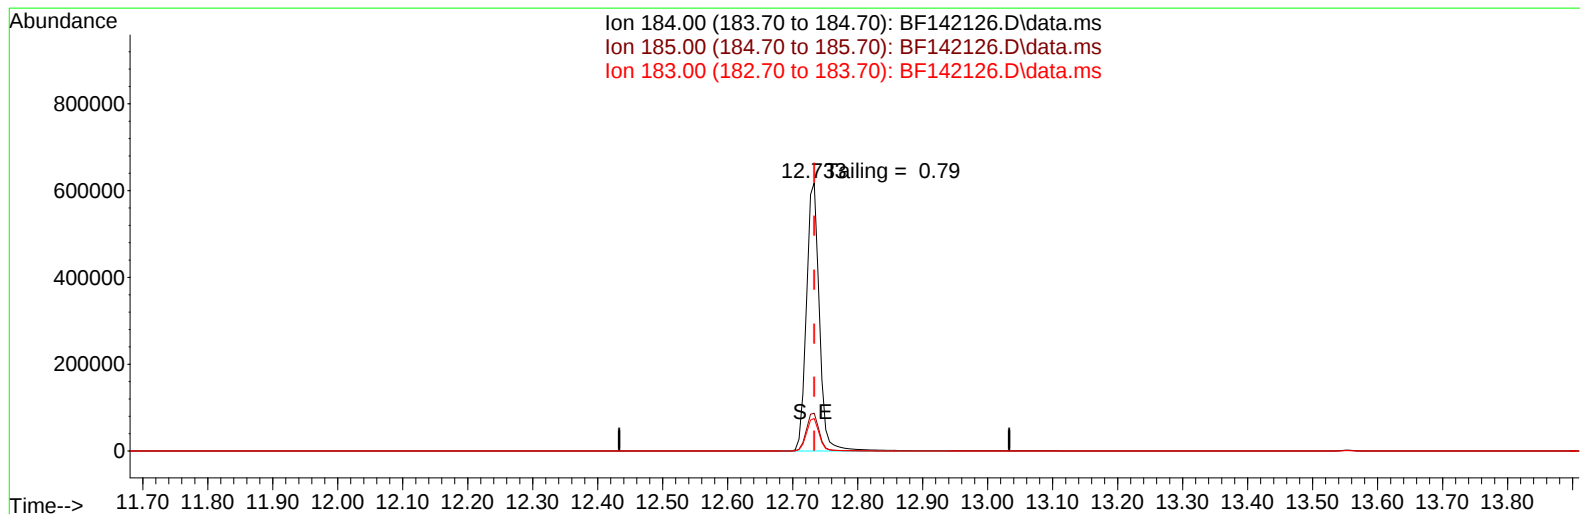

TIC: BF142126.D\data.ms

(77) Benzidine

12.733min (+ 0.000) 53672.63 ng

response 864155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.11
183.00	12.10	12.09
0.00	0.00	0.00