

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032816\
 Data File : BF085835.D
 Acq On : 29 Mar 2016 7:05
 Operator : UM/SJ
 Sample : H1905-07MS
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TRACK-D-GRID-10AMS

Quant Time: Mar 29 06:30:46 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\BFDDTBREAKDOWN.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 01 16:14:27 2010
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	10.56	152	67824	40.00	ng	0.30
2) Naphthalene-d8	11.90	136	1119	40.00	ng	0.18
3) Acenaphthene-d10	15.02	164	213	40.00	ng	0.11
4) Phenanthrene-d10	15.34	188	574	40.00	ng	0.25
8) Chrysene-d12	0.00	240	0	0.00	ng	-30.93
9) Perylene-d12	0.00	264	0	0.00	ng	-34.56
Target Compounds						Qvalue
5) DDE	10.88	246	242	N.D.		
6) DDD	10.95	235	749	N.D.		
7) DDT	11.16	235	3945	N.D.		


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF032816\
Data File : BF085835.D
Acq On : 29 Mar 2016 7:05
Operator : UM/SJ
Sample : H1905-07MS
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TRACK-D-GRID-10AMS

Quant Time: Mar 29 06:30:46 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\BFDDTBREAKDOWN.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 01 16:14:27 2010
Response via : Initial Calibration

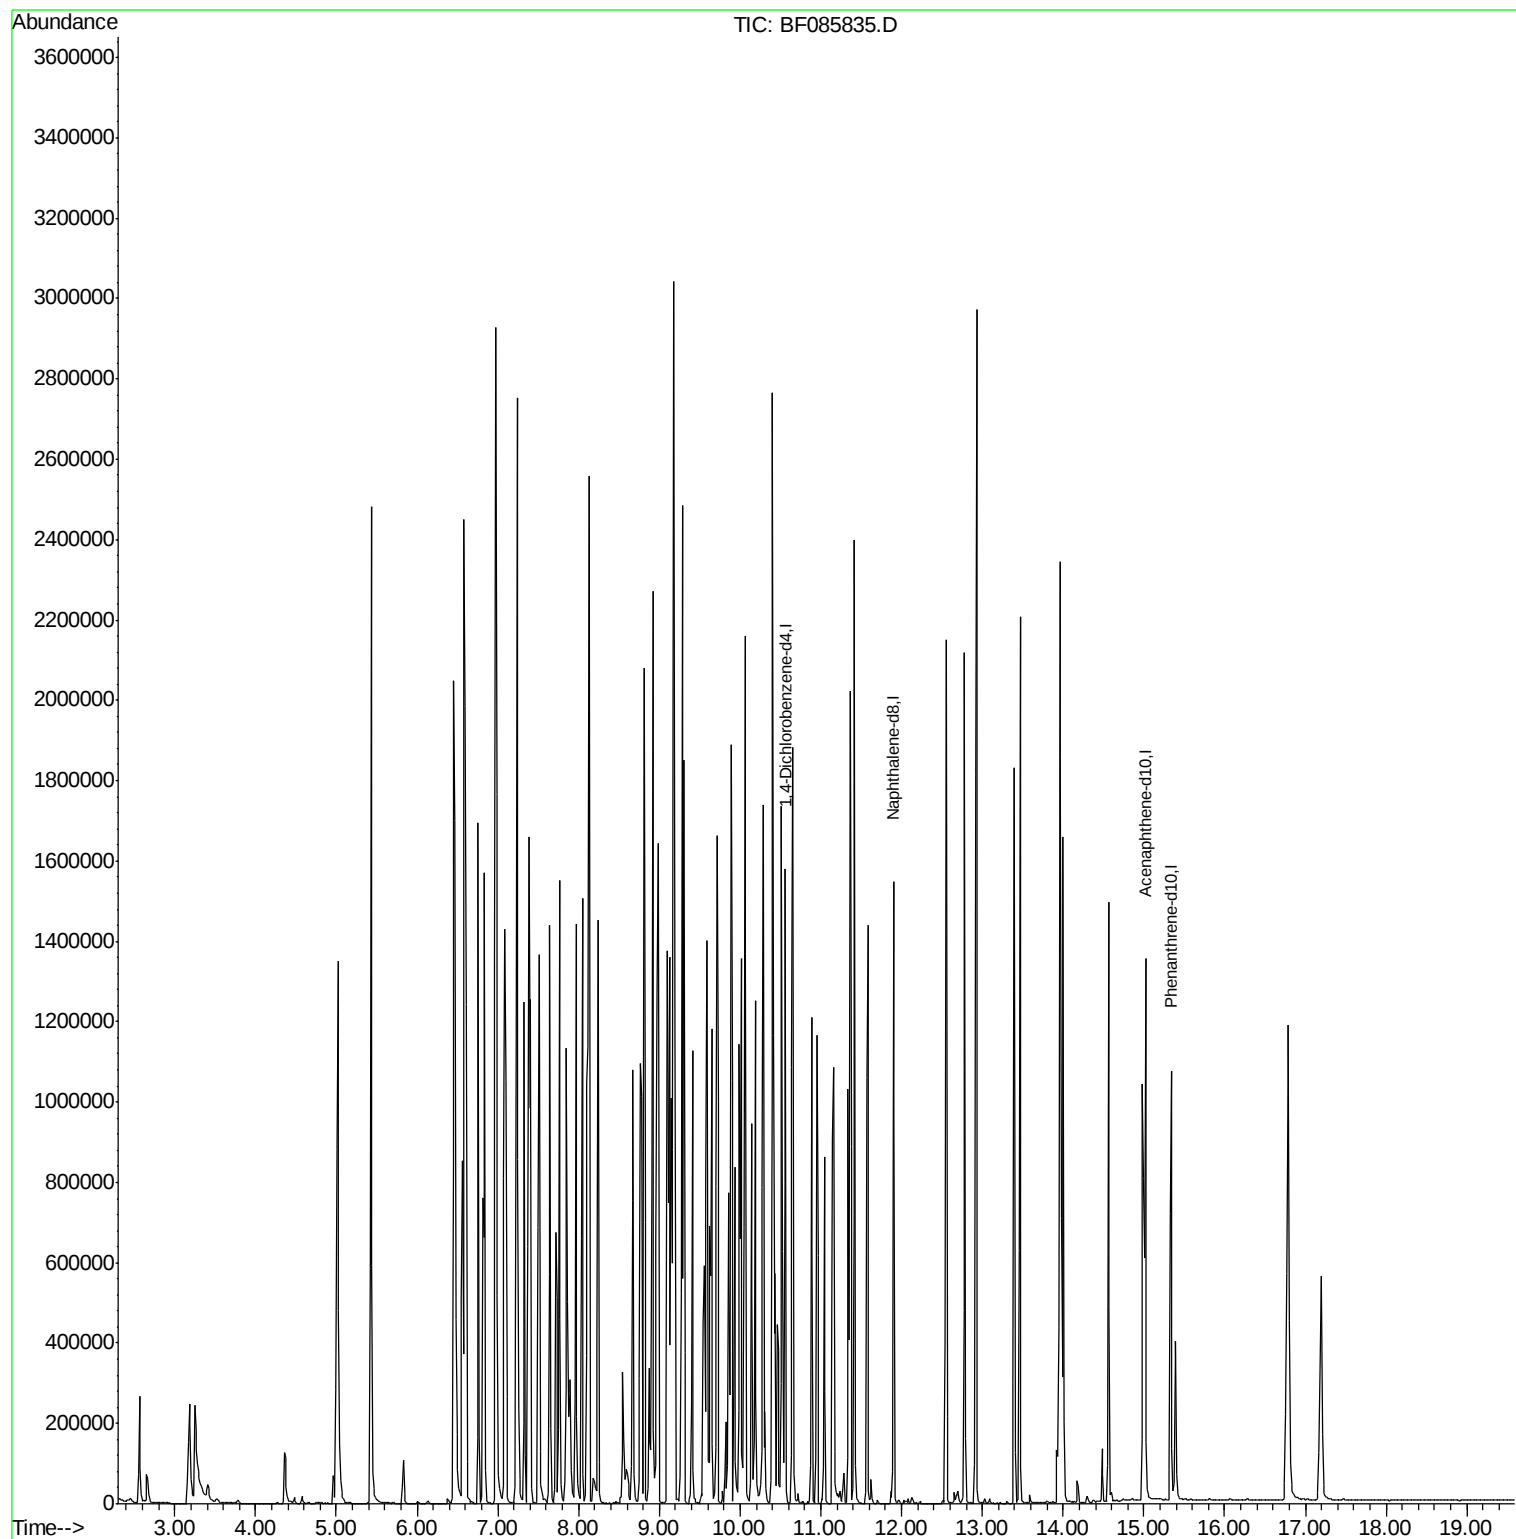

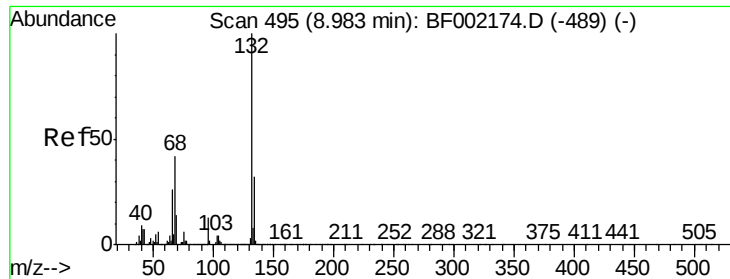

#5

DDE

Concen: Below Cal

RT: 10.88 min Scan# 752

Delta R.T. 0.44 min

Lab File: BF085835.D

Acq: 29 Mar 2016 7:05

Instrument :

BNA_F

ClientSampleId :

TRACK-D-GRID-10AMS

Tgt Ion:246 Resp: 242


Ion Ratio Lower Upper

246 100

248 73295.9 1434.9 2152.3#

318 0.0 161.5 242.3#

176 0.0 3844.2 5766.4#

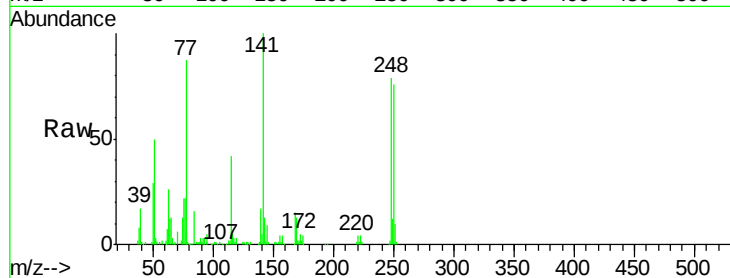


Abundance Ion 246.00 (245.70 to 246.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 318.00 (317.70 to 318.70): E

Ion 176.00 (175.70 to 176.70): E

Time-->

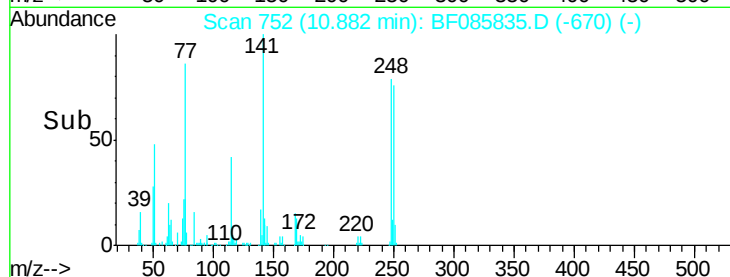


Abundance Ion 246.00 (245.70 to 246.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 318.00 (317.70 to 318.70): E

Ion 176.00 (175.70 to 176.70): E

Time-->

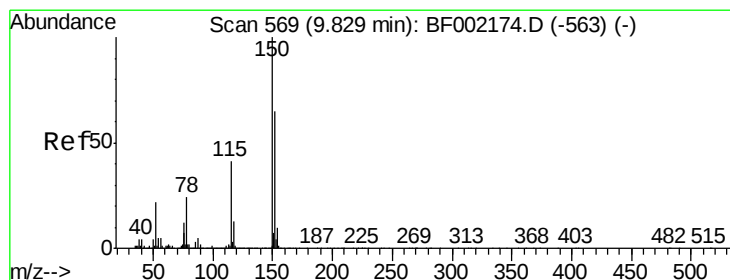

#6

DDD

Concen: Below Cal

RT: 10.95 min Scan# 758

Delta R.T. 0.12 min

Lab File: BF085835.D

Acq: 29 Mar 2016 7:05


Tgt Ion:235 Resp: 749

Ion Ratio Lower Upper

235 100

237 176.8 4800.0 7200.0#

165 546.5 4800.0 7200.0#

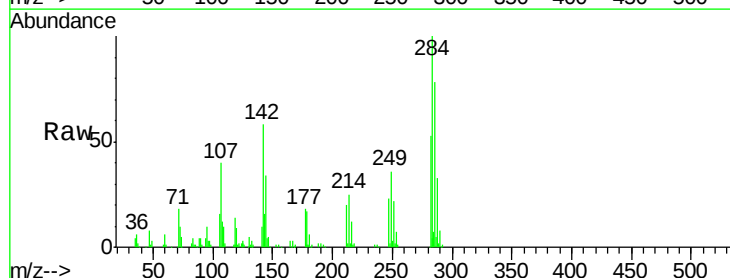


Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E

Time-->

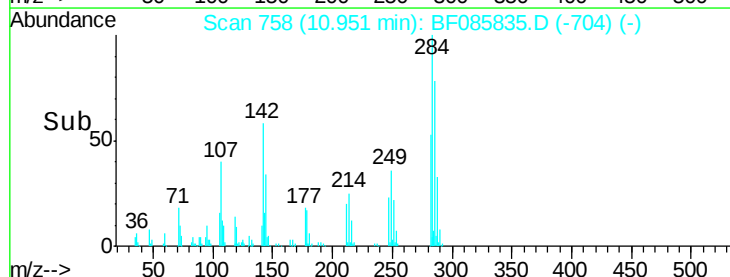


Abundance Ion 235.00 (234.70 to 235.70): E

Ion 237.00 (236.70 to 237.70): E

Ion 165.00 (164.70 to 165.70): E


Time-->

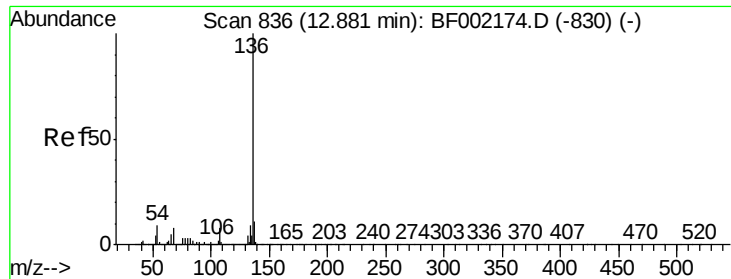

#7
DDT
Concen: Below Cal
RT: 11.16 min Scan# 776
Delta R.T. -0.04 min
Lab File: BF085835.D
Acq: 29 Mar 2016 7:05

Instrument :
BNA_F
ClientSampleId :
TRACK-D-GRID-10AMS

Tgt Ion: 235 Resp: 3945
Ion Ratio Lower Upper
235 100
237 153.6 0.0 0.0#
165 2282.3 0.2 0.2#

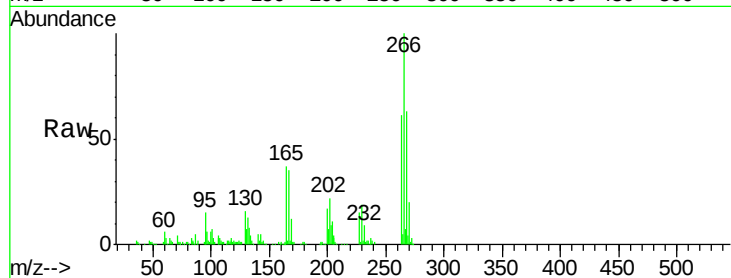

Abundance Ion 235.00 (234.70 to 235.70): E
Ion 237.00 (236.70 to 237.70): E
Ion 165.00 (164.70 to 165.70): E

