
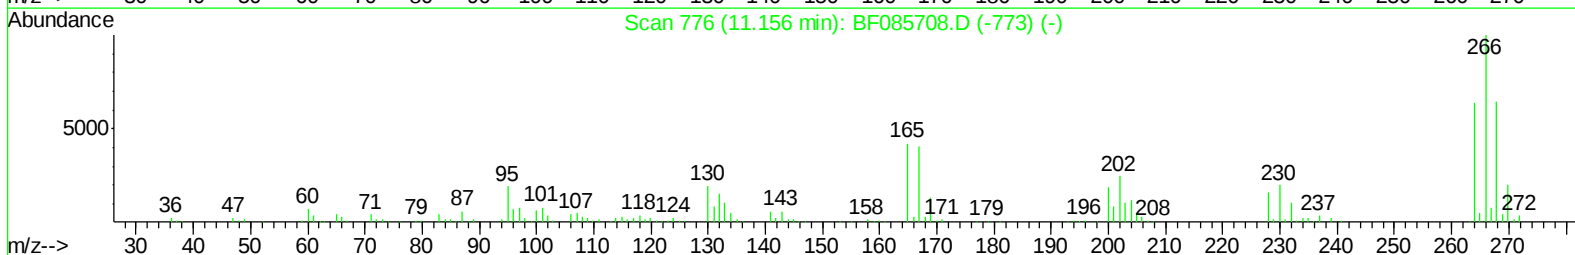
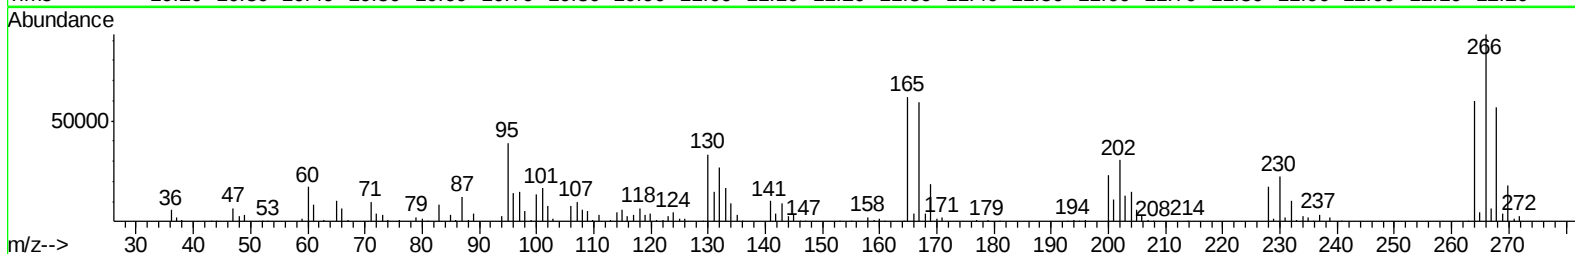


Data Path : Z:\HPCHEM1\BNA_F\Data\BF032816\
Data File : BF085794.D
Acq On : 28 Mar 2016 11:39
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 03:46:37 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 15:27:05 2016
Response via : Initial Calibration

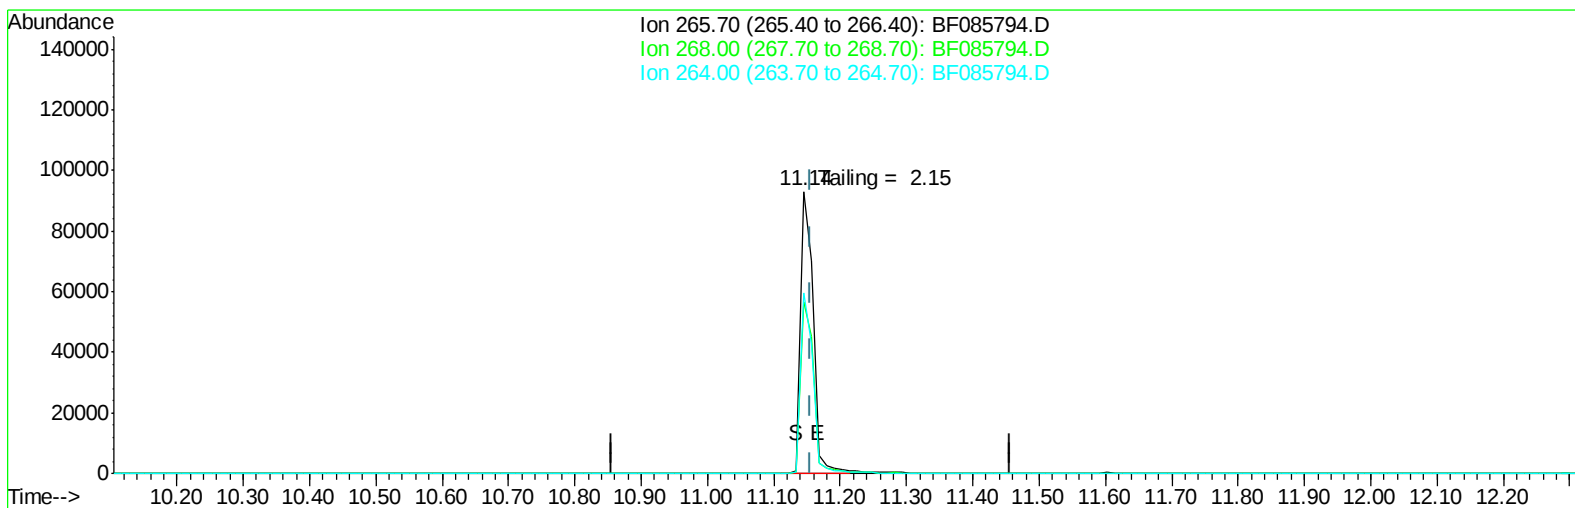

TIC: BF085794.D

(69) Pentachlorophenol (C)




11.145min (-0.011) 49114.87ng

response 123058

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	60.90
264.00	63.30	64.24
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF032816\
 Data File : BF085794.D
 Acq On : 28 Mar 2016 11:39
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 03:46:37 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 28 15:27:05 2016
 Response via : Initial Calibration

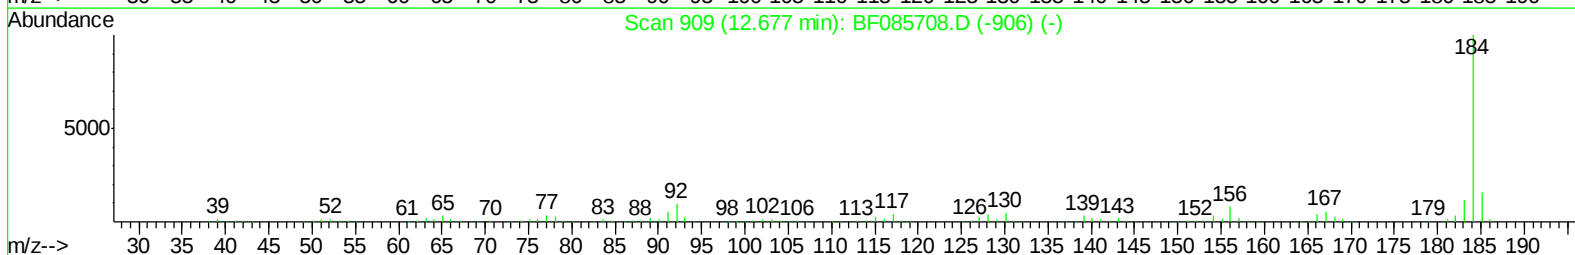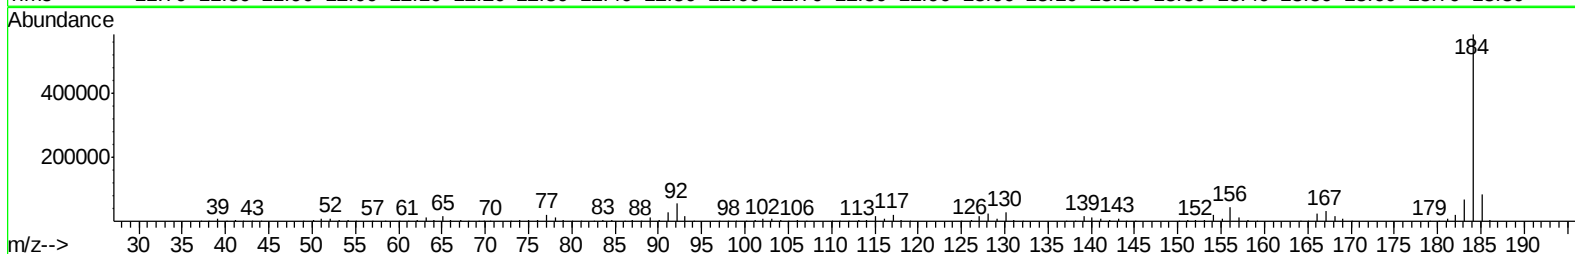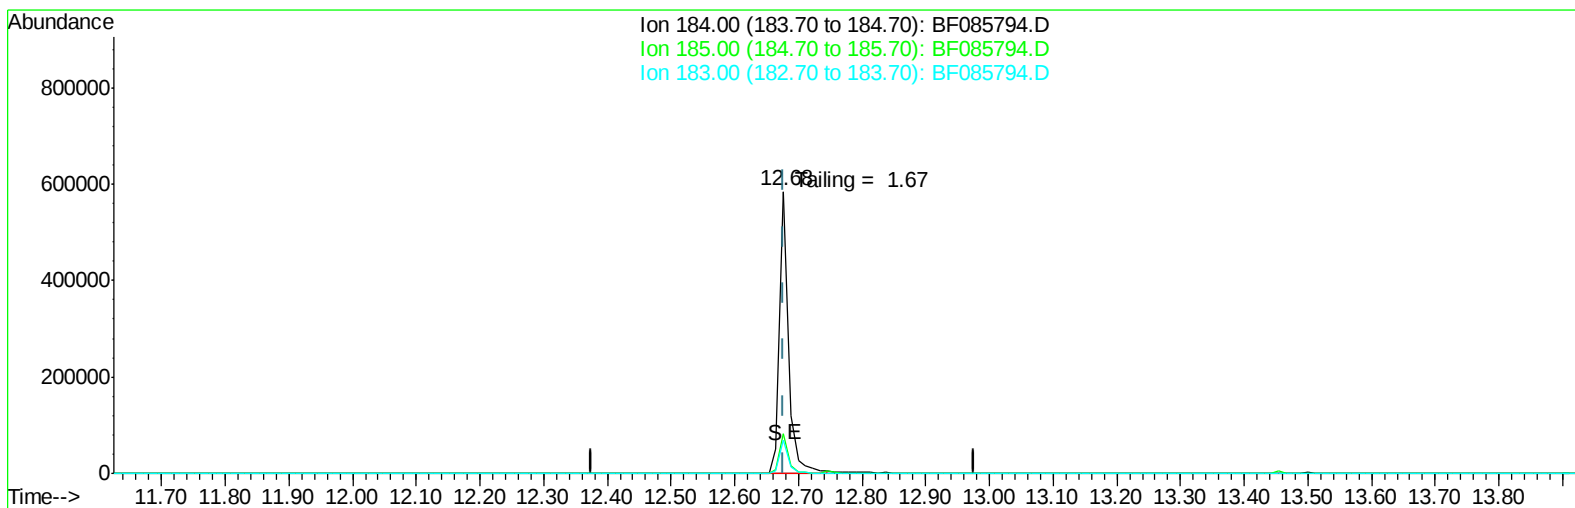

TIC: BF085794.D

(76) Benzidine

12.677min (-0.000) 14811.29ng m

response 558654

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.20
183.00	11.80	11.73
0.00	0.00	0.00