
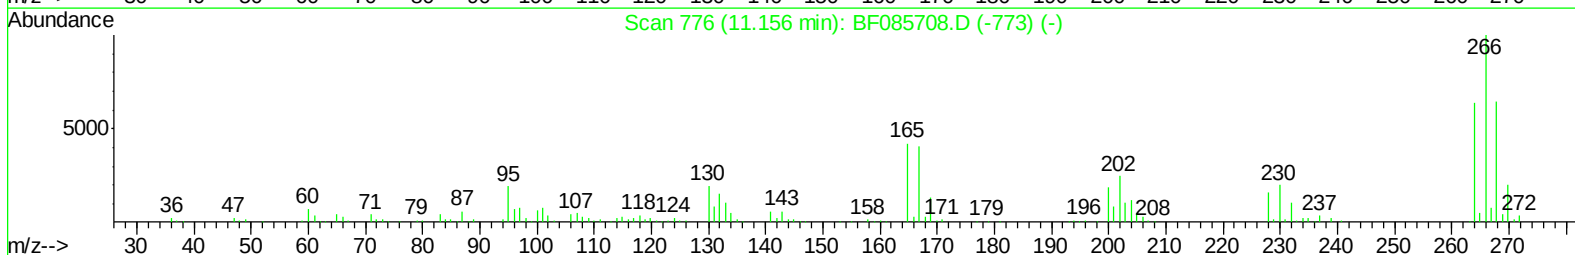
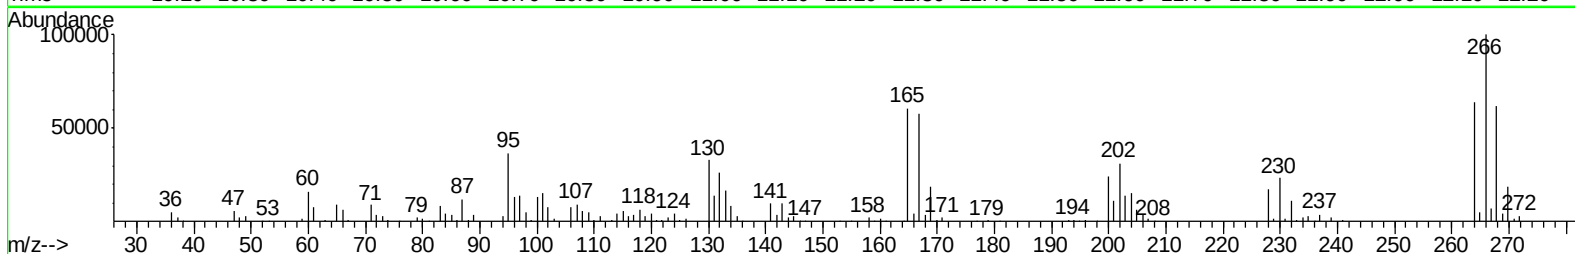


Data Path : Z:\HPCHEM1\BNA_F\Data\BF032816\
Data File : BF085801.D
Acq On : 28 Mar 2016 15:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 03:48:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 15:27:05 2016
Response via : Initial Calibration

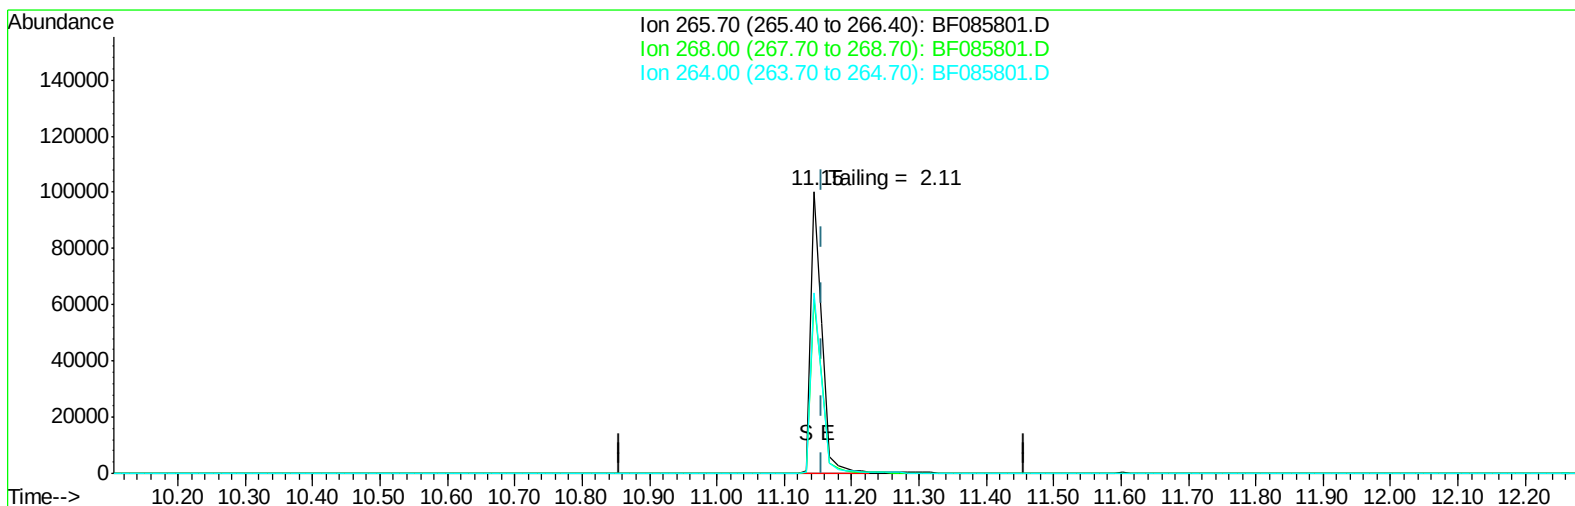

TIC: BF085801.D

(69) Pentachlorophenol (C)




11.145min (-0.011) 52221.17ng

response 116303

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.84
264.00	63.30	63.99
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF032816\
Data File : BF085801.D
Acq On : 28 Mar 2016 15:03
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 29 03:48:53 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032416.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 28 15:27:05 2016
Response via : Initial Calibration

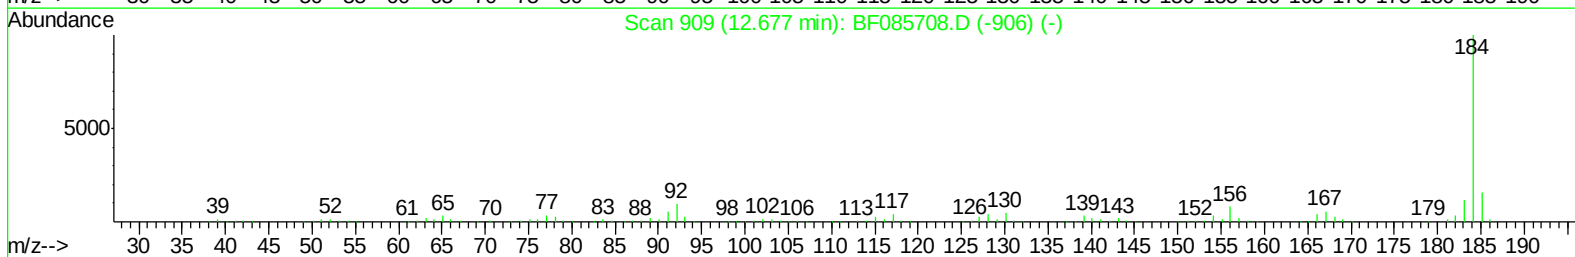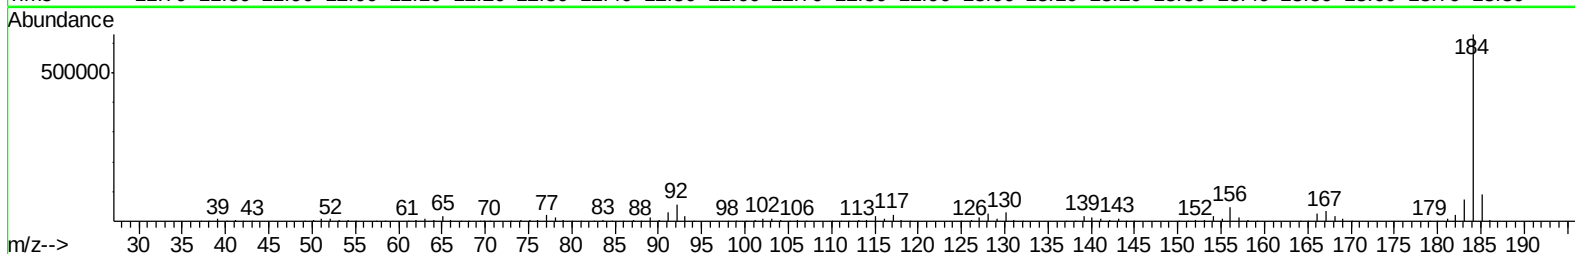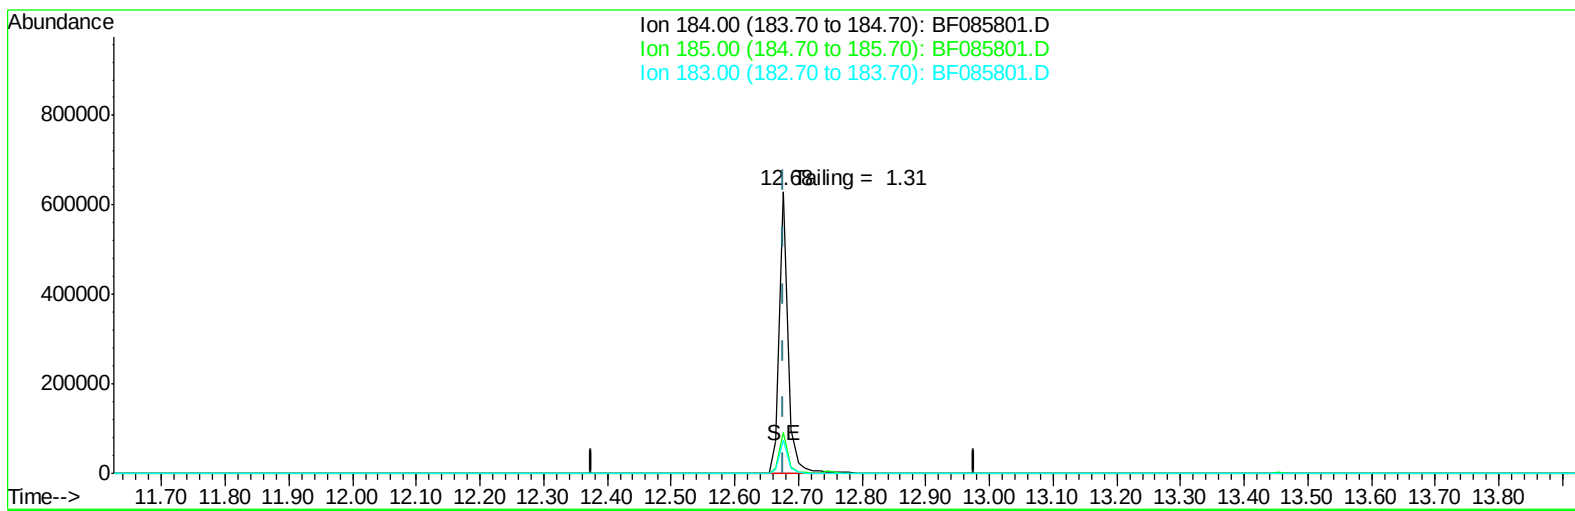

TIC: BF085801.D

(76) Benzidine

12.677min (+0.000) 16892.06ng

response 594304

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	14.48
183.00	11.80	11.80
0.00	0.00	0.00